

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111620\
 Data File : VW017261.D
 Acq On : 16 Nov 2020 16:54
 Operator : SY/VA
 Sample : L4739-17
 Misc : 6.45G/10ML/MSVOA W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB104

Quant Time: Nov 17 07:21:53 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Nov 17 06:08:23 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	436629	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	381047	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	144761	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	91561	16.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.60%
7) Chloroethane-d5	2.89	69	80911	19.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.36%
10) 1,1-Dichloroethene-d2	4.02	63	133695	13.59	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	54.36%
20) 2-Butanone-d5	7.08	46	51642	41.99	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.98%
24) Chloroform-d	7.65	84	216294	21.22	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.88%
26) 1,2-Dichloroethane-d4	8.31	65	116465	22.98	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.92%
29) Benzene-d6	8.27	84	410086	21.13	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.52%
33) 1,2-Dichloropropane-d6	9.27	67	116990	21.80	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.20%
37) Toluene-d8	10.32	98	379359	20.73	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.92%
38) trans-1,3-Dichloropropene-	10.58	79	50430	20.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.36%
39) 2-Hexanone-d5	10.93	63	43056	45.97	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.94%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	100790	21.56	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.24%
61) 1,2-Dichlorobenzene-d4	13.85	152	110457	21.66	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.64%


Target Compounds					Ovalue
13) Acetone	4.13	43	5270	6.400 ug/L	99
22) cis-1,2-Dichloroethene	7.17	96	40675	6.858 ug/L	98
35) Trichloroethene	9.09	95	209411	37.362 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW111620\
Data File : VW017261.D
Acq On : 16 Nov 2020 16:54
Operator : SY/VA
Sample : L4739-17
Misc : 6.45G/10ML/MSVOA W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GB104

Quant Time: Nov 17 07:21:53 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Tue Nov 17 06:08:23 2020
Response via : Initial Calibration

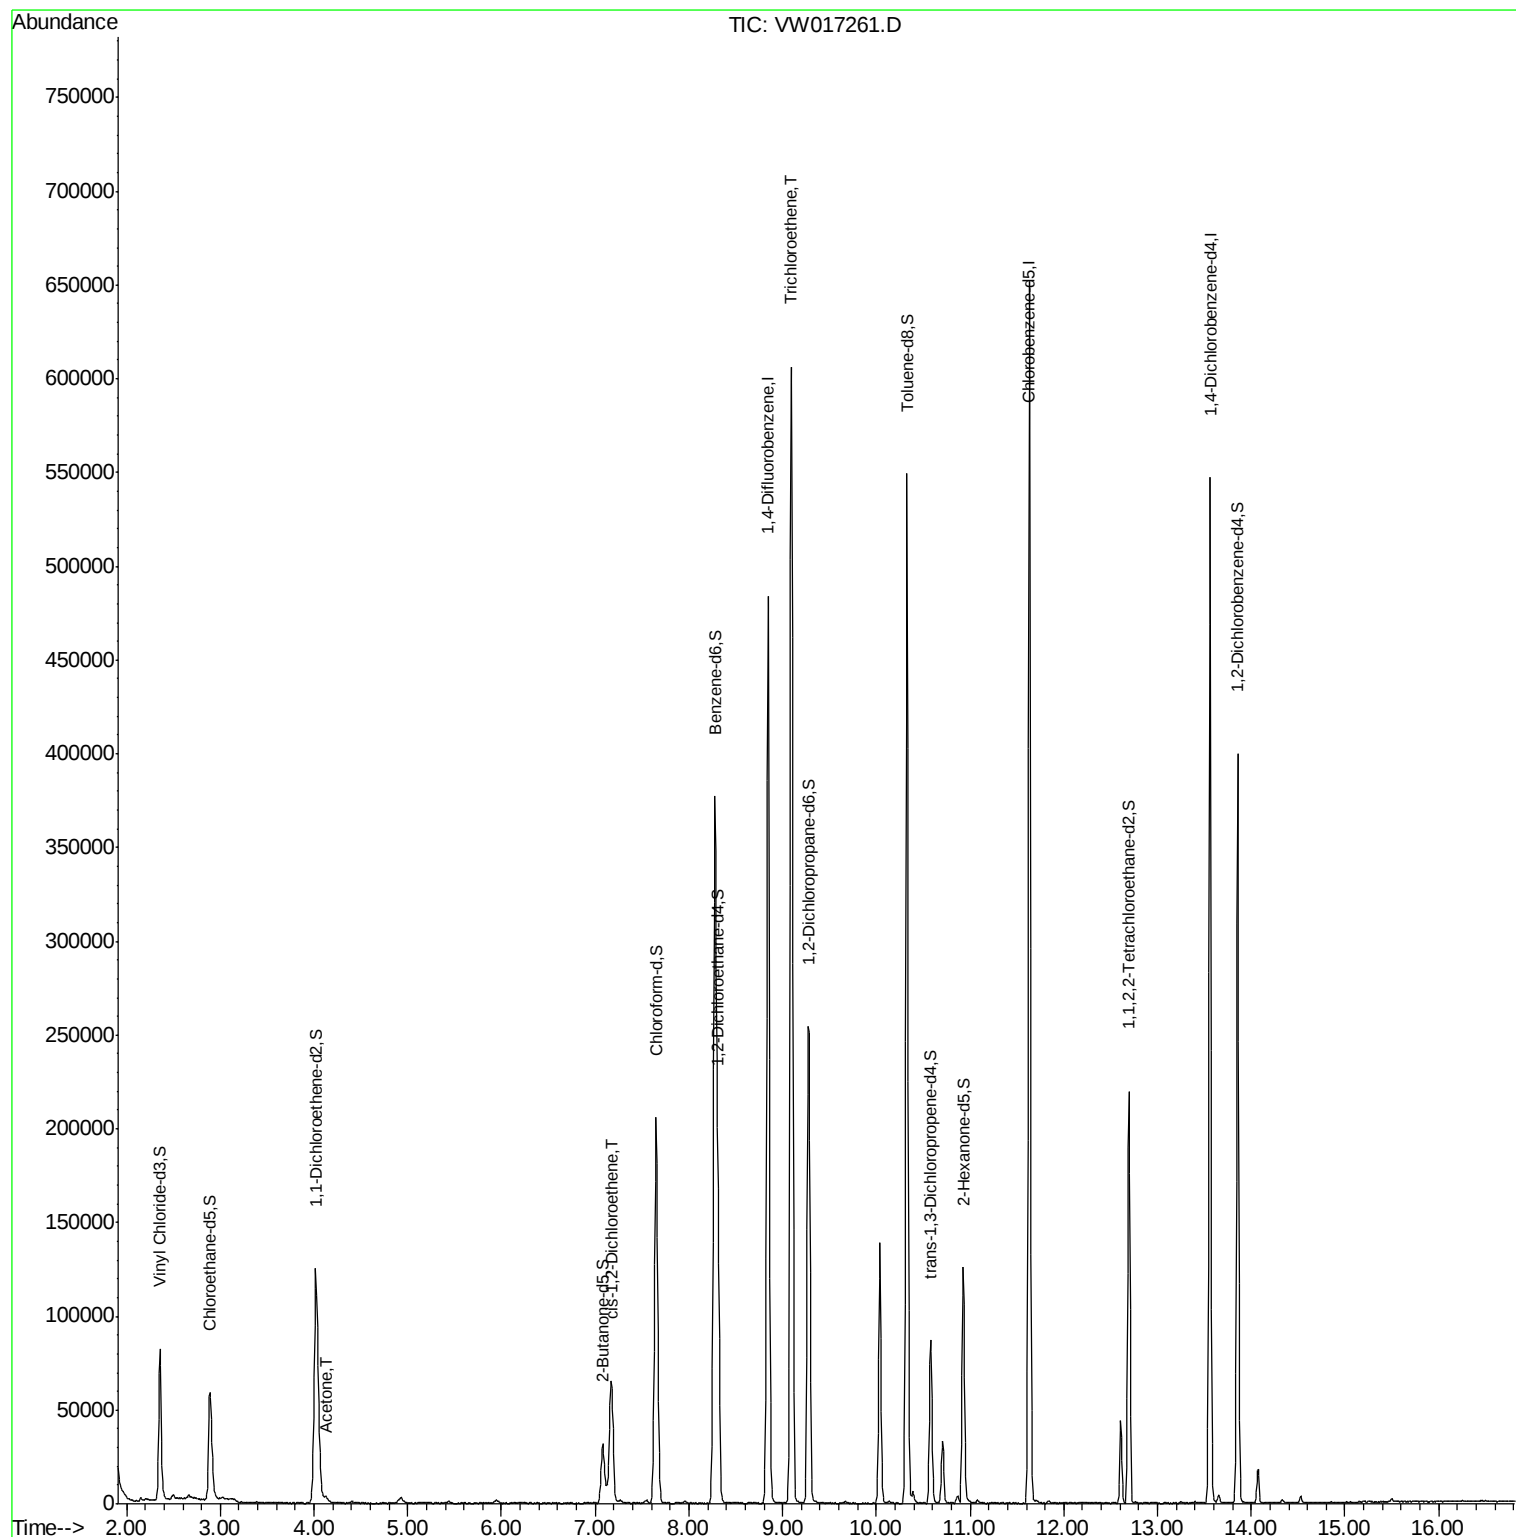

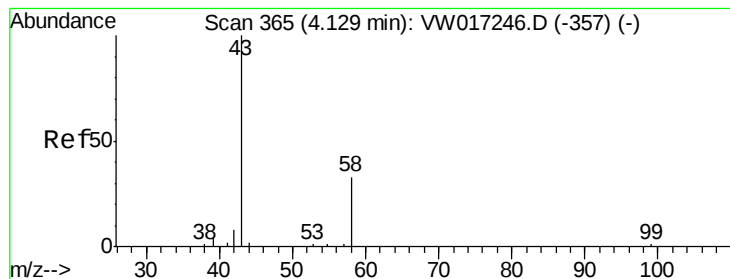

#13

Acetone

Concen: 6.400 ug/L

RT: 4.13 min Scan# 365

Delta R.T. -0.00 min

Lab File: VW017261.D

Acq: 16 Nov 2020 16:54

Instrument :

MSVOA_W

ClientSampled :





GB104

Tot Ion: 43 Resp: 5270

Ion Ratio Lower Upper

43 100

58 33.9 0.0 69.2

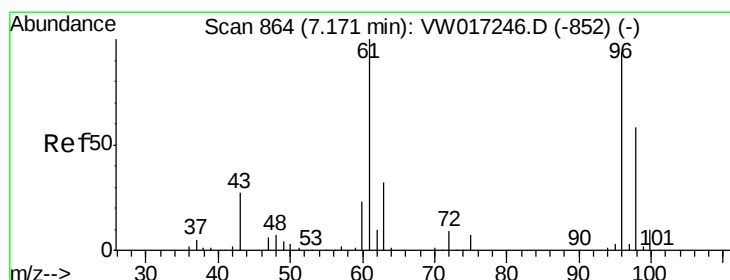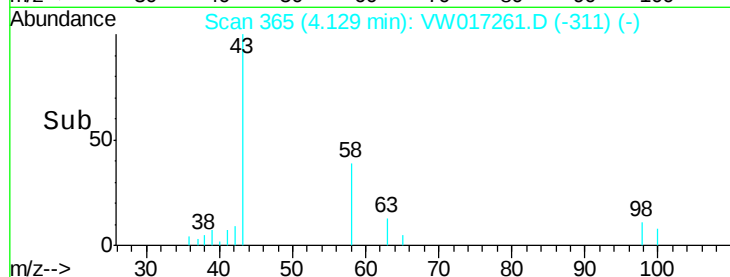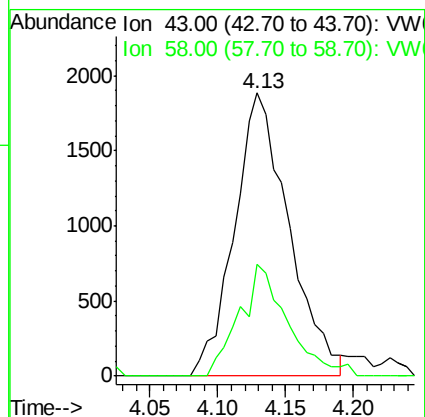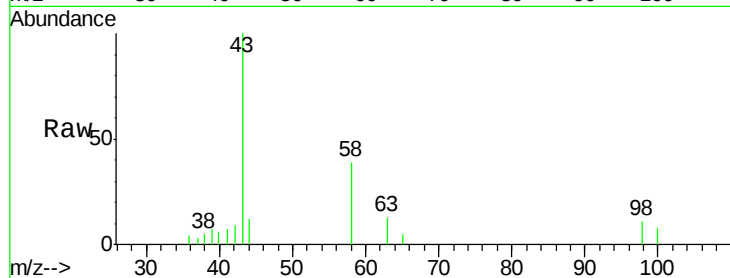

#22

cis-1,2-Dichloroethene

Concen: 6.858 ug/L

RT: 7.17 min Scan# 864

Delta R.T. -0.00 min

Lab File: VW017261.D

Acq: 16 Nov 2020 16:54




Tgt Ion: 96 Resp: 40675


Ion Ratio Lower Upper

96 100

61 108.2 77.4 143.8

98 63.3 45.1 83.7

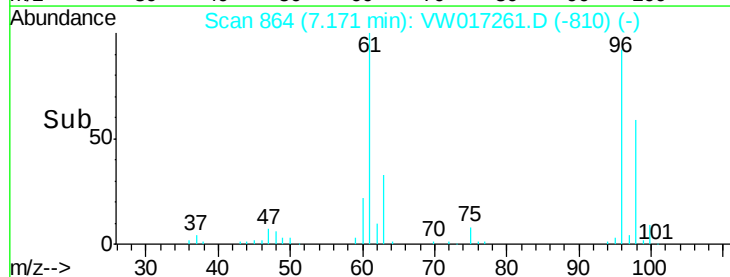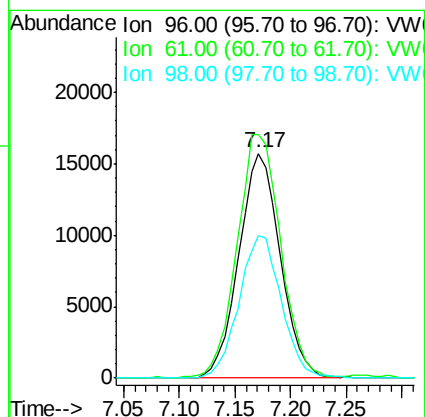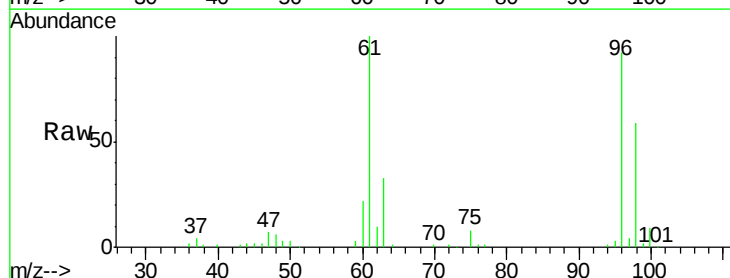


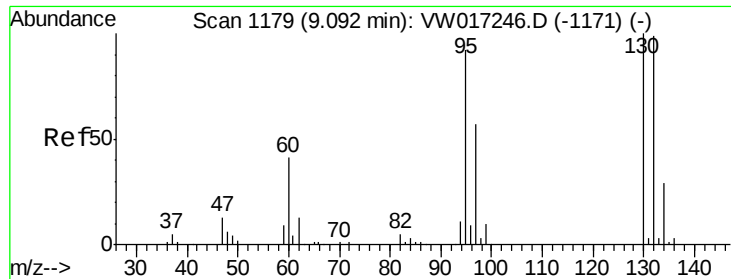

#35
 Trichloroethene
 Concen: 37.362 ug/L
 RT: 9.09 min Scan# 1179
 Delta R.T. -0.00 min
 Lab File: VW017261.D
 Acq: 16 Nov 2020 16:54

Instrument :
 MSVOA_W
 ClientSampleId :
 GB104

Tot Ion:	95	Resp:	209411
Ion	Ratio	Lower	Upper
95	100		
97	64.9	45.0	83.6
132	105.5	73.7	136.9
130	109.0	77.1	143.1

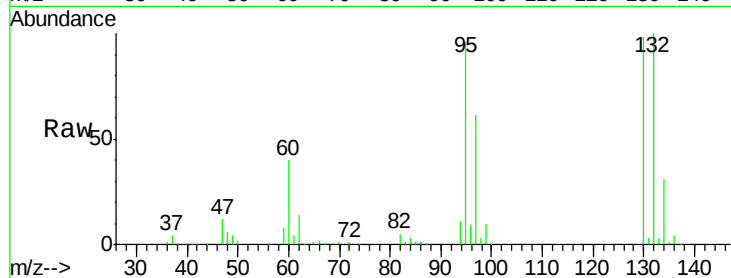

Abundance Ion 95.00 (94.70 to 95.70): VW
 Ion 97.00 (96.70 to 97.70): VW
 Ion 132.00 (131.70 to 132.70): V
 Ion 130.00 (129.70 to 130.70): V

