


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW111620\
 Data File : VW017245.D
 Acq On : 16 Nov 2020 09:38
 Operator : SY/VA
 Sample : BFB07
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB07

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Title : VOC Analysis
 Last Update : Tue Nov 17 06:08:23 2020

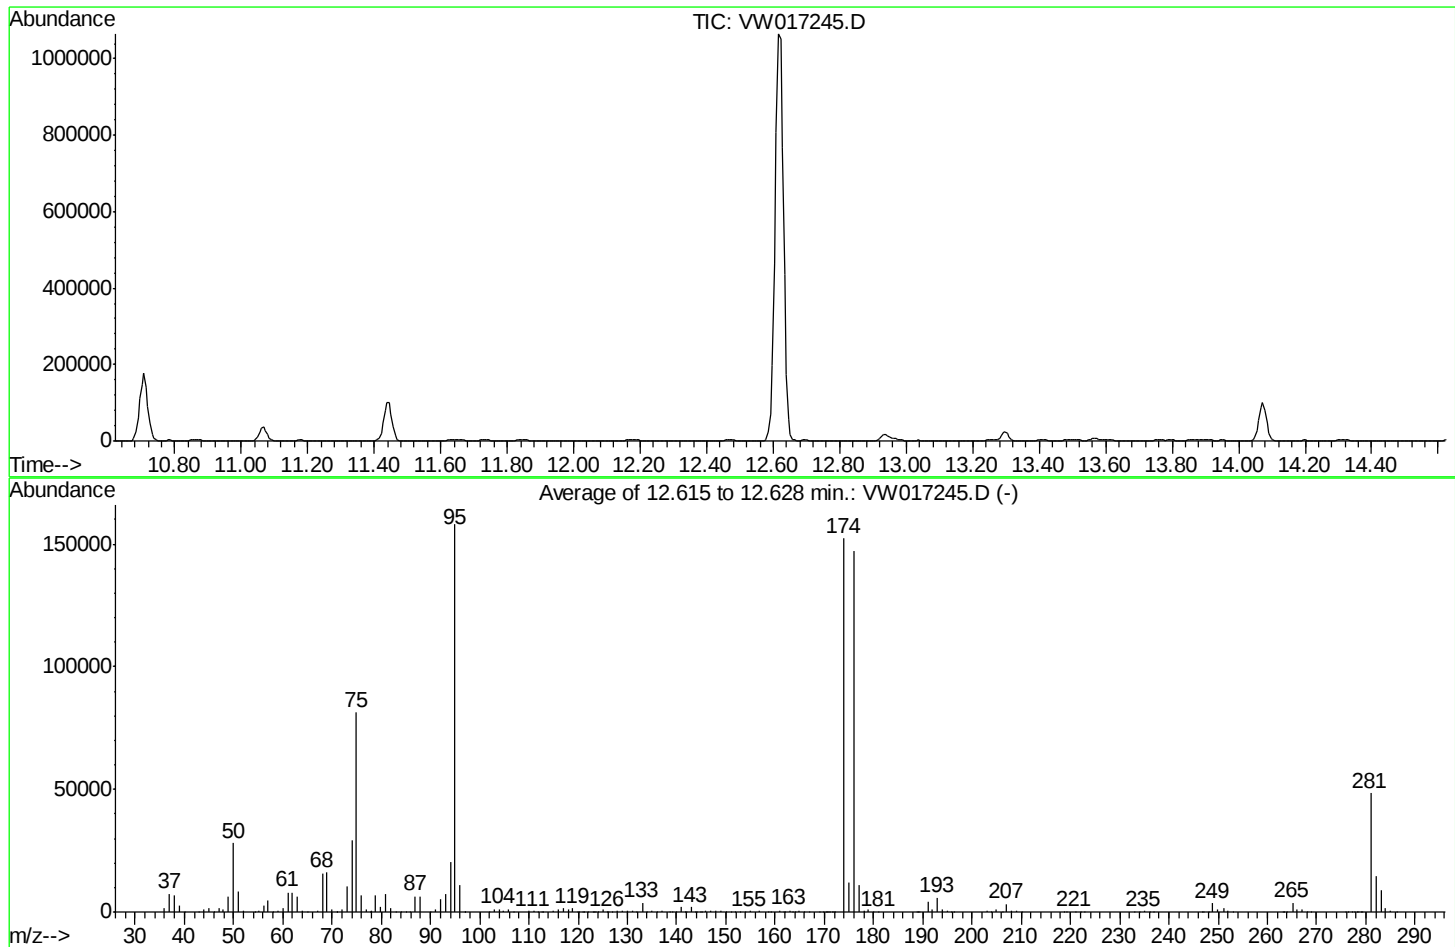

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	28144	PASS
75	95	30	80	51.4	81314	PASS
95	95	100	100	100.0	158058	PASS
96	95	5	9	6.8	10823	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	96.3	152256	PASS
175	174	5	9	7.9	12016	PASS
176	174	95	101	96.7	147226	PASS
177	176	5	9	7.4	10943	PASS

m/z	Abundance
36.00	1384.0
37.00	8049.0
38.00	7465.0
39.00	2698.0
40.00	214.0
43.00	290.0
44.00	1295.0
45.10	2180.0
46.10	143.0
46.90	1657.0
48.00	1124.0
49.00	7508.0
50.00	31464.0
51.00	9226.0
52.00	438.0
55.00	664.0
56.10	3176.0
57.00	5433.0
58.00	249.0
59.00	1035.0
60.00	1836.0
61.00	8565.0
62.00	8750.0
63.00	6567.0
64.00	639.0
65.00	162.0
67.10	579.0
68.00	16928.0
69.00	17256.0
70.00	1370.0
70.90	140.0
72.10	889.0
73.00	13281.0
74.00	31352.0
75.00	86136.0
76.00	6898.0
77.00	875.0
77.80	686.0
78.90	7067.0
79.90	2271.0
80.90	7736.0
81.90	1345.0
83.10	234.0
85.00	174.0
85.80	205.0
86.90	6551.0
88.00	6484.0
90.00	61.0
90.90	861.0
92.00	5250.0
93.00	7859.0
94.00	21400.0
95.00	165824.0
96.00	11827.0
96.90	336.0
101.90	93.0
102.90	1010.0
104.00	1249.0
104.90	478.0
105.90	851.0
106.90	347.0
109.90	429.0
111.00	460.0
111.90	450.0
112.70	305.0
114.90	690.0
115.90	747.0
116.90	1596.0
118.00	1474.0
118.90	2124.0
119.80	213.0
120.90	250.0
121.90	55.0
123.20	51.0
124.10	156.0
125.00	2004.0
126.80	74.0
128.00	638.0
128.90	446.0
129.90	930.0
130.90	347.0
131.90	228.0
133.00	6435.0
135.00	889.0
136.00	123.0
137.00	316.0
138.60	58.0
139.10	57.0
140.90	1811.0
141.80	266.0
143.00	2006.0
143.80	160.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07

144.80	300.0
145.90	287.0
146.90	831.0
148.00	451.0
148.80	405.0
149.90	374.0
151.00	78.0
151.80	101.0
153.00	157.0
154.00	113.0
154.90	337.0
156.90	393.0
159.00	348.0
160.90	741.0
161.80	118.0
162.10	113.0
162.90	1201.0
164.00	282.0
165.00	861.0
165.80	138.0
166.90	110.0
169.80	76.0
170.60	124.0
171.10	180.0
171.70	406.0
173.90	153664.0
175.00	11600.0
175.90	146880.0
176.90	11594.0
178.00	797.0
179.00	1768.0
180.00	369.0
181.00	168.0
188.90	617.0
191.00	6154.0
192.00	1633.0
193.00	9912.0
194.00	1750.0
195.00	952.0
195.70	104.0
196.20	72.0
203.00	854.0
203.80	241.0
205.00	1728.0
206.10	421.0
207.00	5303.0
208.00	1119.0
209.00	571.0
210.00	138.0
219.10	204.0
221.00	372.0
221.90	62.0
222.90	86.0
233.00	86.0
233.90	71.0
235.00	661.0
235.90	214.0
236.90	297.0
247.10	149.0
248.00	150.0
249.00	6120.0
249.90	1464.0
251.10	2421.0
251.90	555.0
253.00	306.0
263.10	93.0
263.90	85.0
265.10	6324.0
266.00	1630.0
267.00	1487.0
268.00	253.0
269.00	174.0
275.90	54.0
276.40	58.0
277.60	185.0
279.00	363.0
281.10	67912.0
282.10	23824.0
283.10	15091.0
284.10	2737.0
285.00	759.0
286.20	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07

m/z	Abundance
36.00	1639.0
37.00	8110.0
38.00	7760.0
39.10	2734.0
39.90	167.0
43.00	323.0
44.10	1471.0
45.00	1964.0
45.90	184.0
47.00	1612.0
48.00	1238.0
49.00	7048.0
50.00	30760.0
51.00	9392.0
52.00	386.0
55.10	523.0
56.00	3160.0
57.00	5322.0
58.10	267.0
59.00	609.0
60.00	1385.0
61.00	9396.0
62.00	8723.0
63.00	6533.0
64.00	705.0
65.00	122.0
67.00	522.0
68.00	18344.0
69.00	17536.0
70.10	1314.0
71.10	113.0
72.00	913.0
73.00	11565.0
74.00	32704.0
75.00	90416.0
76.00	7783.0
77.00	1001.0
78.00	782.0
78.90	7499.0
79.90	2137.0
80.90	8159.0
81.90	1739.0
82.90	248.0
83.90	61.0
87.00	7165.0
87.90	7123.0
90.90	783.0
92.00	5734.0
93.00	8288.0
94.00	22536.0
95.00	173952.0
96.00	11806.0
97.10	383.0
102.90	905.0
104.00	1124.0
104.90	505.0
106.00	1081.0
106.90	214.0
109.80	279.0
110.80	364.0
111.80	196.0
112.90	280.0
115.00	398.0
115.90	918.0
116.90	1498.0
117.90	981.0
118.90	1393.0
119.70	99.0
121.00	79.0
122.80	83.0
123.60	111.0
124.00	123.0
125.00	1159.0
126.10	335.0
128.00	626.0
128.90	353.0
129.90	745.0
131.00	340.0
131.90	115.0
133.00	3798.0
134.80	697.0
136.00	85.0
137.00	399.0
138.70	60.0
139.10	80.0
139.80	180.0
140.90	2062.0
142.00	309.0
142.90	2342.0
144.00	84.0
145.00	288.0
145.90	296.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07

146.90	522.0
147.90	598.0
148.80	315.0
149.90	249.0
151.10	75.0
151.90	171.0
152.90	196.0
154.00	152.0
154.90	467.0
156.90	528.0
158.70	171.0
159.10	165.0
161.00	477.0
162.00	182.0
162.90	879.0
164.90	495.0
165.90	84.0
166.70	77.0
169.70	59.0
170.80	150.0
171.90	540.0
174.00	166080.0
175.00	13433.0
176.00	165760.0
176.90	12132.0
178.00	567.0
178.90	1138.0
179.90	177.0
181.00	104.0
189.10	533.0
191.00	3956.0
192.00	673.0
192.90	4751.0
194.00	1036.0
194.90	621.0
195.80	58.0
196.20	56.0
203.00	390.0
203.90	102.0
205.00	894.0
206.10	265.0
207.00	2958.0
208.00	745.0
209.10	401.0
218.70	57.0
220.80	158.0
222.00	74.0
233.00	57.0
234.90	439.0
236.00	133.0
246.80	142.0
248.10	146.0
248.90	3017.0
250.00	900.0
251.00	1458.0
252.00	333.0
253.00	269.0
263.50	51.0
265.10	3198.0
266.00	1108.0
267.10	1051.0
268.10	212.0
268.90	80.0
277.60	167.0
278.10	131.0
278.90	281.0
281.00	55592.0
282.10	14413.0
283.10	7270.0
283.90	1584.0
285.00	577.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07

m/z	Abundance
36.00	1097.0
37.00	5797.0
38.00	5320.0
39.10	1763.0
40.00	209.0
43.00	144.0
44.00	1118.0
45.00	1156.0
46.00	121.0
47.00	1231.0
47.90	892.0
49.00	4843.0
50.00	22208.0
51.00	6944.0
52.00	280.0
54.30	69.0
55.00	376.0
56.00	2056.0
57.00	3695.0
57.90	154.0
58.10	155.0
59.00	258.0
59.90	1115.0
61.00	6357.0
62.00	5940.0
63.00	5370.0
64.10	547.0
64.80	85.0
67.00	378.0
68.00	12288.0
69.00	13638.0
70.00	1114.0
70.80	68.0
72.00	858.0
73.00	7338.0
74.00	23752.0
75.00	67392.0
76.00	5815.0
77.00	871.0
78.00	411.0
78.90	5658.0
79.90	1557.0
80.90	5702.0
82.00	1155.0
83.00	140.0
83.90	51.0
86.90	5535.0
87.90	5461.0
90.90	791.0
92.00	4255.0
93.00	5640.0
94.00	16768.0
95.00	134400.0
96.00	8838.0
97.00	265.0
102.70	320.0
103.00	289.0
103.90	897.0
104.90	242.0
105.80	743.0
106.80	125.0
110.00	305.0
110.90	251.0
111.80	174.0
112.90	263.0
115.10	255.0
115.90	839.0
117.00	1258.0
117.90	756.0
119.00	1029.0
120.10	70.0
121.10	53.0
122.90	67.0
125.10	482.0
125.80	293.0
126.70	112.0
128.00	442.0
129.00	261.0
129.90	552.0
130.90	232.0
133.00	1234.0
133.80	446.0
134.90	492.0
136.00	73.0
136.90	342.0
138.70	55.0
139.90	173.0
140.90	2067.0
141.80	120.0
142.90	1827.0
144.00	90.0
145.00	271.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07

145.90	314.0
146.80	383.0
148.00	328.0
148.90	266.0
150.00	187.0
152.90	137.0
153.90	84.0
154.90	437.0
156.80	257.0
159.00	202.0
160.80	389.0
163.00	210.0
163.60	73.0
164.90	310.0
166.00	68.0
169.10	58.0
170.30	55.0
172.10	510.0
174.00	137024.0
175.00	11015.0
176.00	129040.0
177.00	9105.0
177.90	413.0
179.00	430.0
179.90	98.0
188.70	108.0
189.30	82.0
191.10	1784.0
192.10	451.0
192.90	2599.0
194.10	490.0
195.00	336.0
203.00	306.0
204.90	500.0
206.10	132.0
207.00	1247.0
207.90	278.0
209.00	101.0
218.70	57.0
221.00	98.0
235.00	219.0
248.90	1536.0
250.10	436.0
251.10	635.0
251.90	178.0
265.00	1505.0
266.00	612.0
267.10	608.0
267.90	127.0
268.80	76.0
277.10	55.0
278.40	121.0
279.20	152.0
281.10	21384.0
282.00	6252.0
283.10	4046.0
284.10	830.0
285.10	368.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07

Scan 1749 (12.567 min): VW017245.D
BFB07

m/z	Abundance
40.10	167.0
44.00	167.0
57.00	56.0
73.10	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB07