
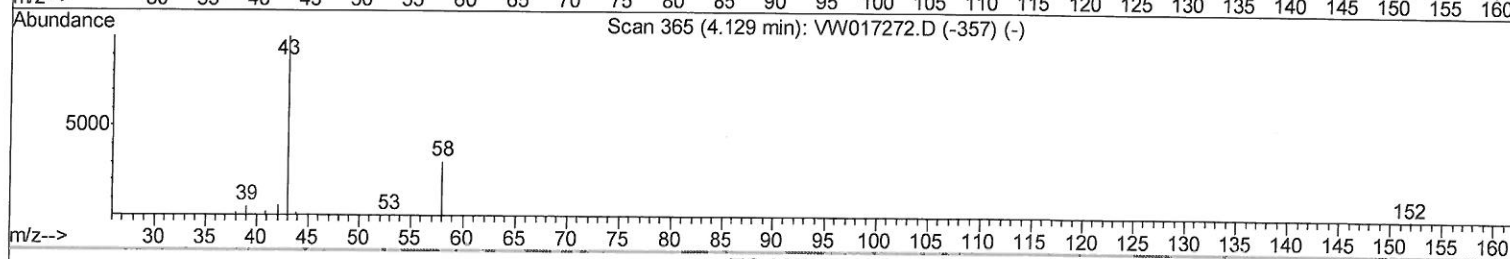
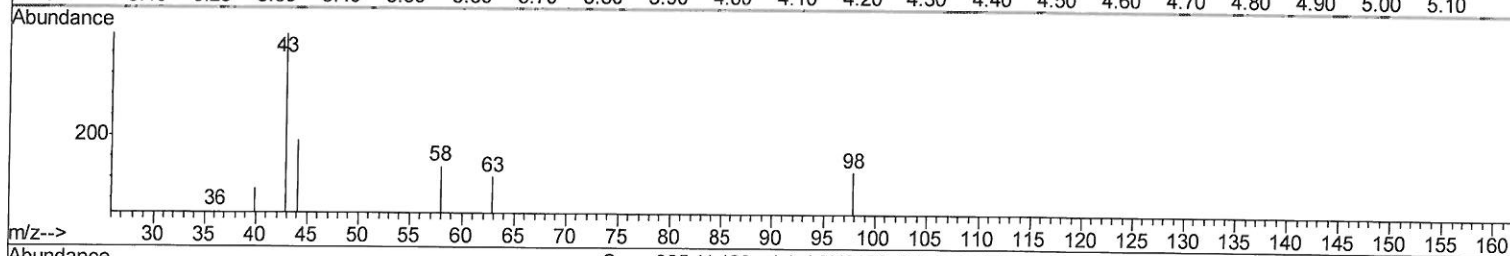


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111720\
Data File : VW017283.D
Acq On : 17 Nov 2020 14:00
Operator : SY/VA
Sample : L4710-21RE
Misc : 4.46G/10ML/MSVOA W/SOIL
ALS Vial : 14 Sample Multiplier: 1

MMDadoda
11/19/2020 11:09:21 AM

Quant Time: Nov 18 02:16:38 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 18 02:13:37 2020
Response via : Initial Calibration

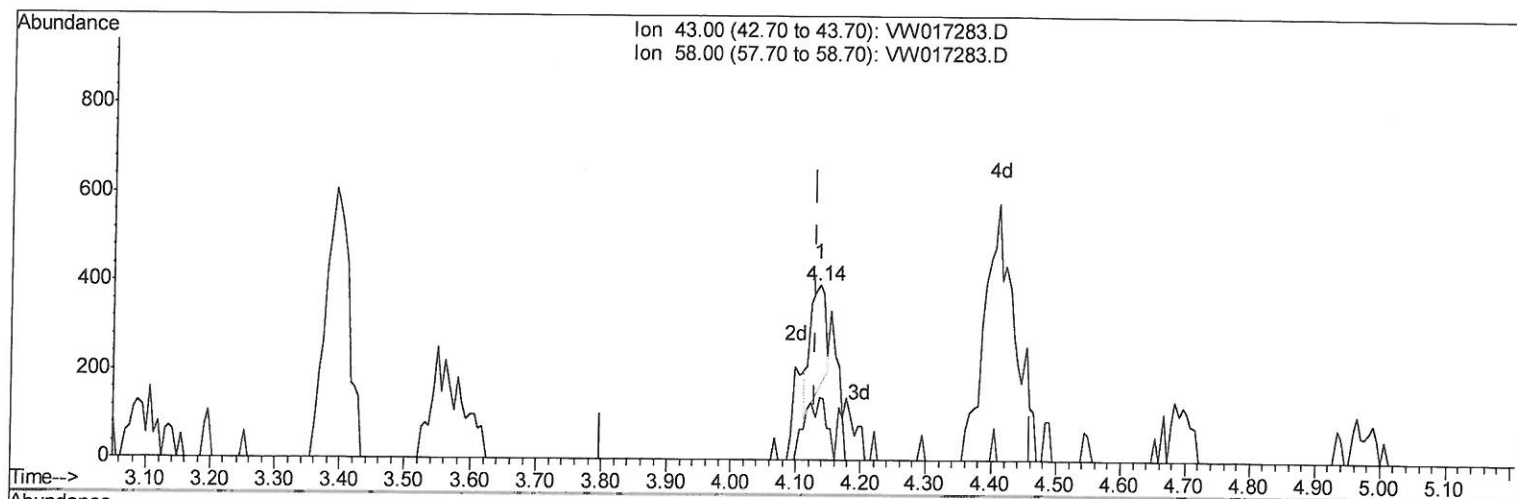

TIC: VW017283.D

response 388

Ion	Exp%	Act%
43.00	100	100
58.00	34.60	39.69
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111720\
 Data File : VW017283.D
 Acq On : 17 Nov 2020 14:00
 Operator : SY/VA
 Sample : L4710-21RE
 Misc : 4.46G/10ML/MSVOA W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AY5RE

Manual Integrations
 APPROVED

MMDadoda
 11/19/2020 11:09:21 AM

Quant Time: Nov 18 02:16:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 18 02:13:37 2020
 Response via : Initial Calibration

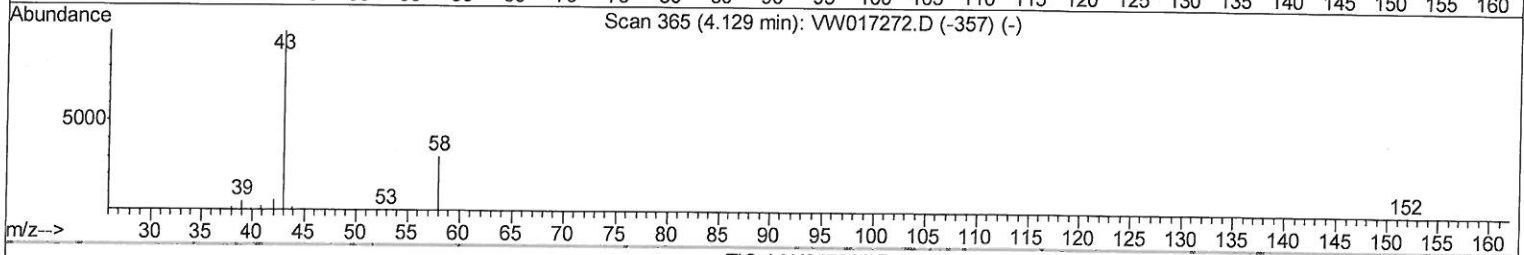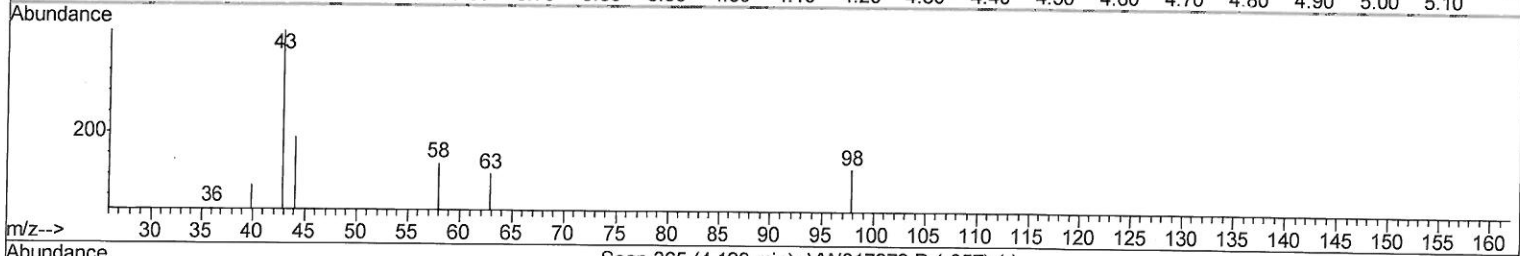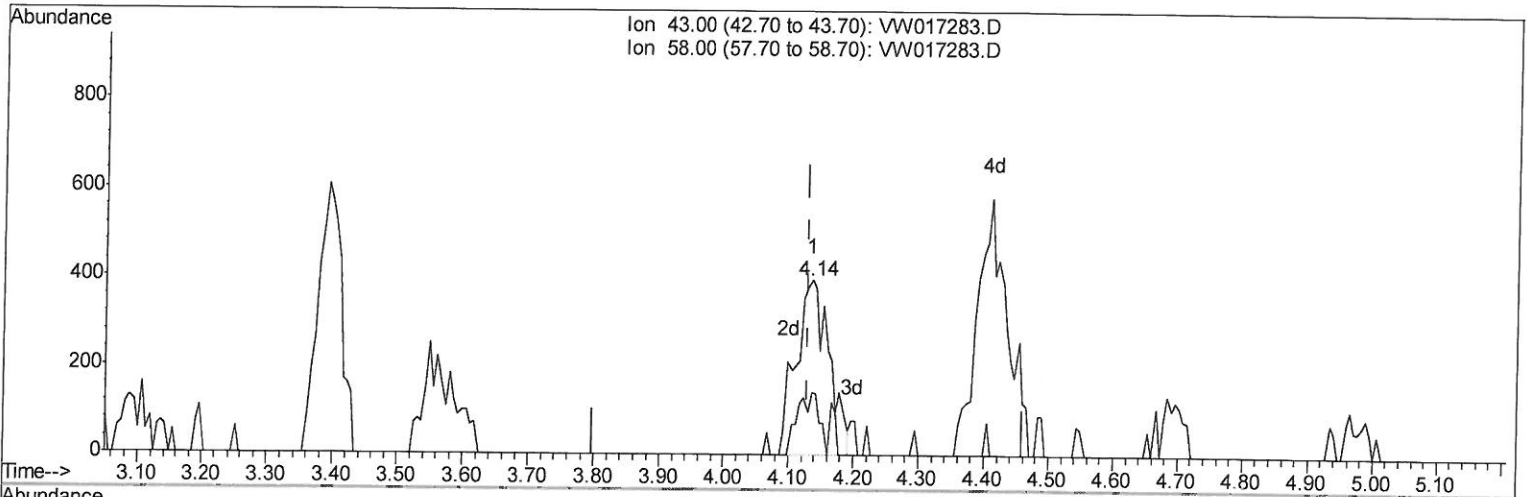

TIC: VW017283.D

(13) Acetone (T)

4.135min (+0.006) 2.05ug/L m

11/25/2024

response 1384

Ion	Exp%	Act%
43.00	100	100
58.00	34.60	11.13
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111720\
Data File : VW017283.D
Acq On : 17 Nov 2020 14:00
Operator : SY/VA
Sample : L4710-21RE
Misc : 4.46G/10ML/MSVOA W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AY5RE

Manual Integrations
APPROVED

MMDadoda
11/19/2020 11:09:21 AM

Quant Time: Nov 18 02:16:38 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 18 02:13:37 2020
Response via : Initial Calibration

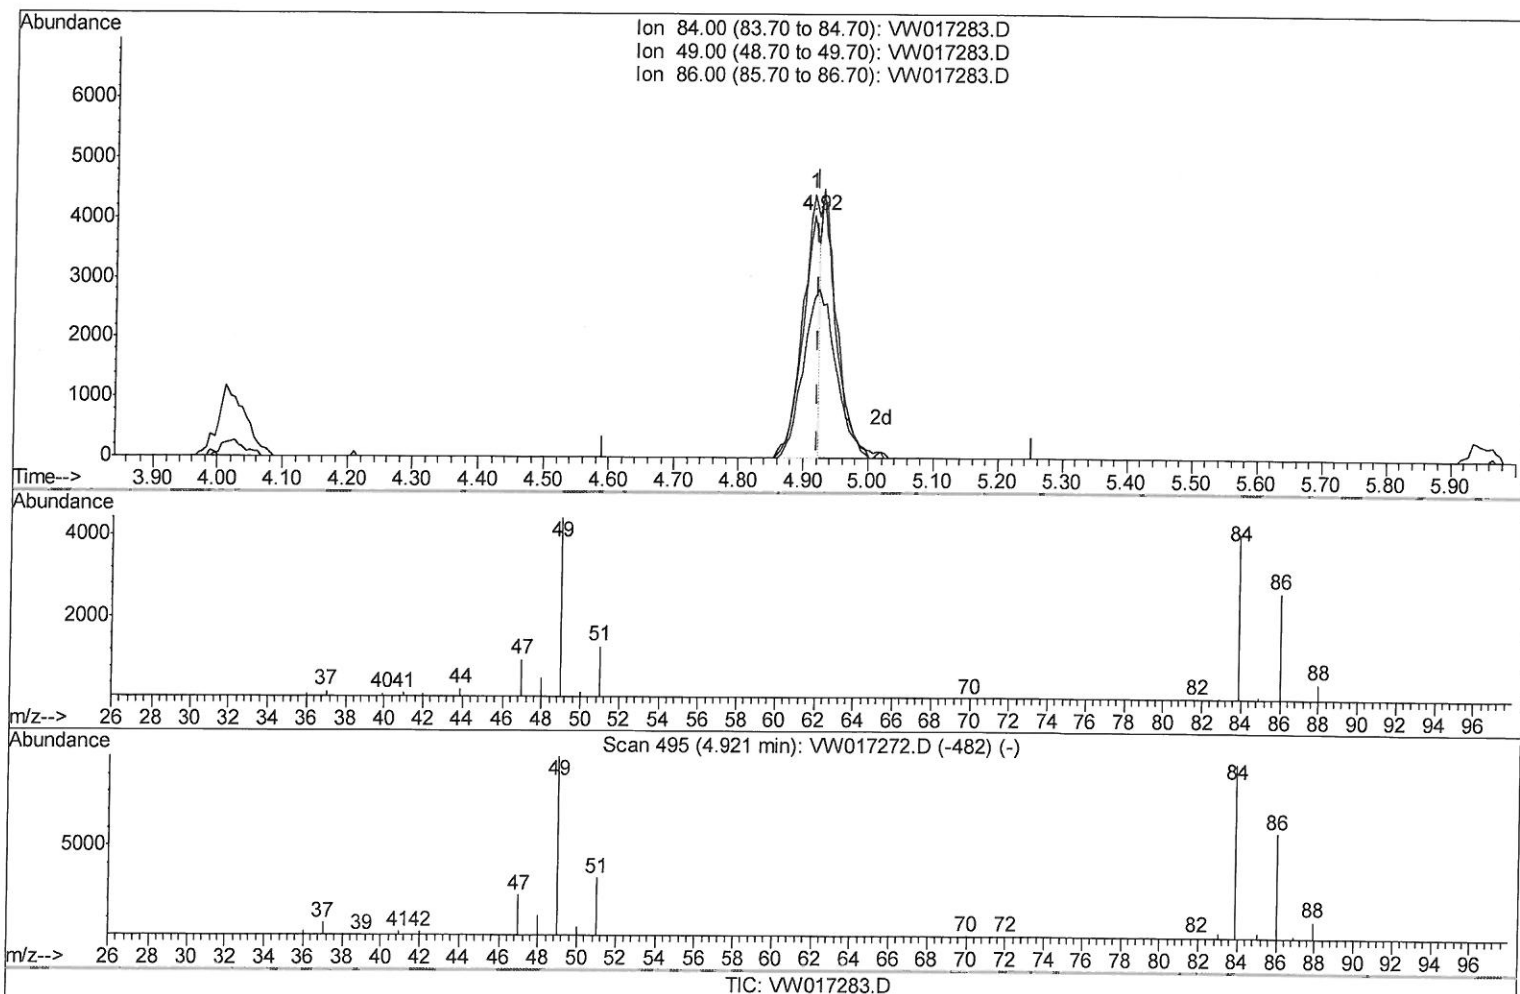

(16) Methylene chloride (T)

4.916min (-0.006) 1.50ug/L

response 7219

Ion	Exp%	Act%
84.00	100	100
49.00	103.30	108.35
86.00	64.40	65.72
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111720\
 Data File : VW017283.D
 Acq On : 17 Nov 2020 14:00
 Operator : SY/VA
 Sample : L4710-21RE
 Misc : 4.46G/10ML/MSVOA W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AY5RE

Manual Integrations
 APPROVED

MMDadoda
 11/19/2020 11:09:21 AM

Quant Time: Nov 18 02:16:38 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 18 02:13:37 2020
 Response via : Initial Calibration

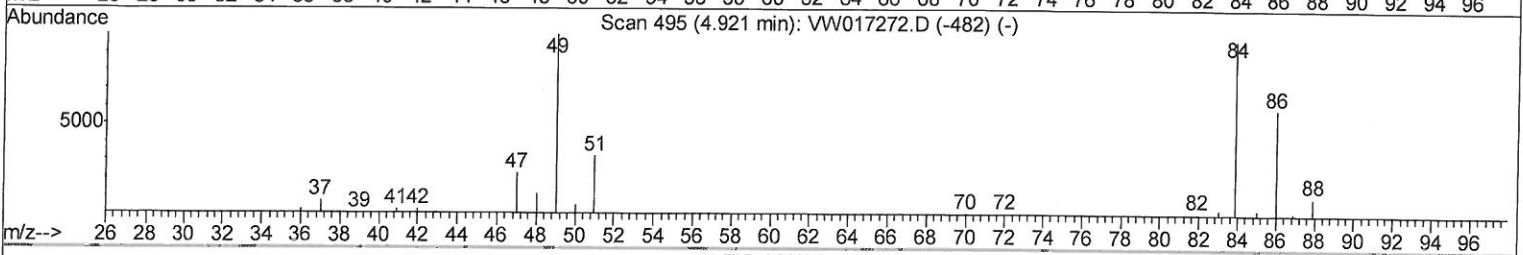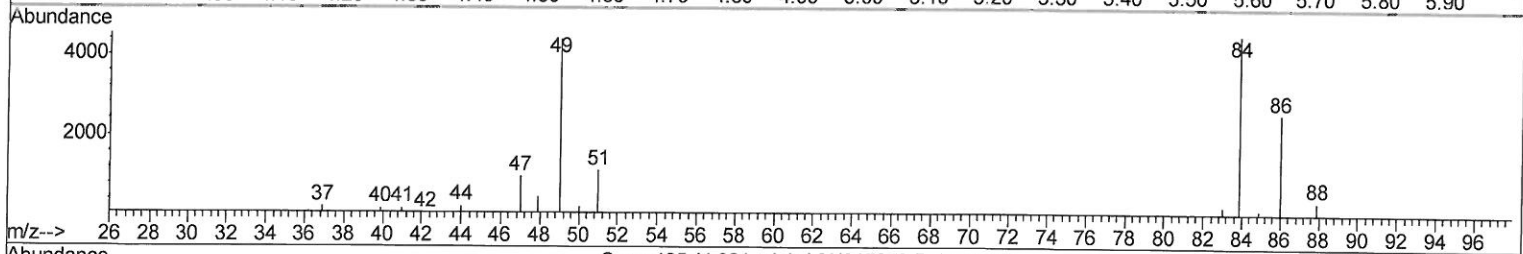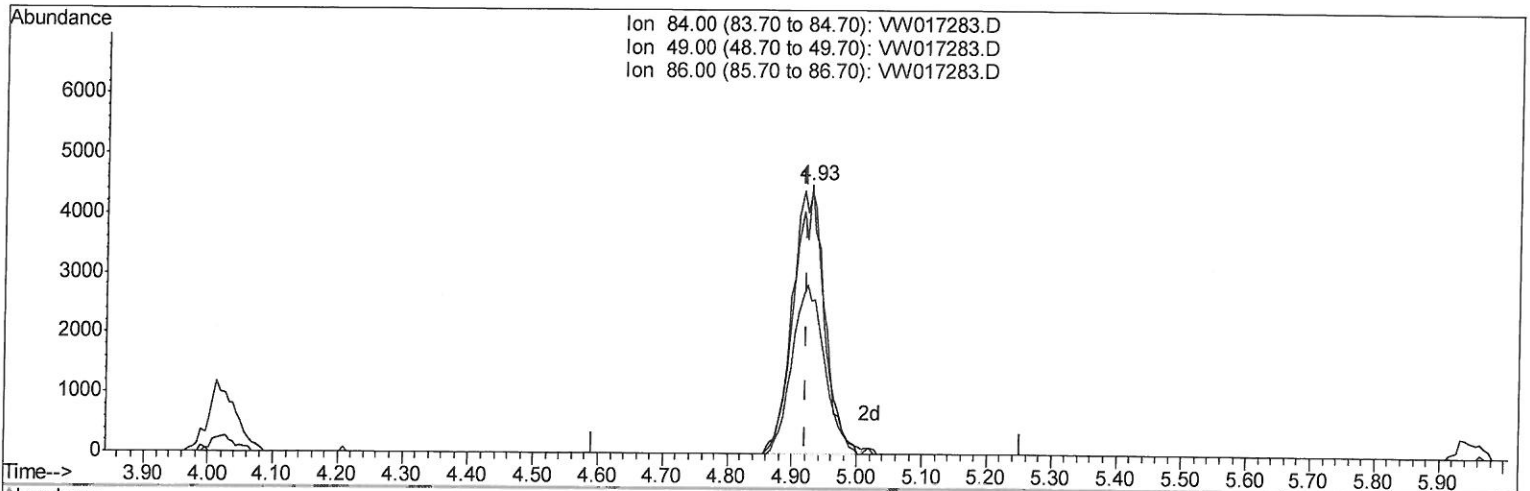

TIC: VW017283.D

(16) Methylene chloride (T)

4.928min (+0.006) 2.99ug/L m

response 14447

Ion	Exp%	Act%
84.00	100	100
49.00	103.30	97.12
86.00	64.40	56.78
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111720\
 Data File : VW017283.D
 Acq On : 17 Nov 2020 14:00
 Operator : SY/VA
 Sample : L4710-21RE
 Misc : 4.46G/10ML/MSVOA W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AY5RE

Manual Integrations
 APPROVED

MMDadoda
 11/19/2020 11:09:21 AM

Quant Time: Nov 18 03:59:35 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 18 02:13:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	357963	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	271562	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	88761	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	74791	16.59	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.36%
7) Chloroethane-d5	2.90	69	67217	19.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.40%
10) 1,1-Dichloroethene-d2	4.03	63	112367	13.93	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.72%
20) 2-Butanone-d5	7.08	46	28915	28.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	57.36%
24) Chloroform-d	7.65	84	170658	20.42	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.68%
26) 1,2-Dichloroethane-d4	8.31	65	91069	21.92	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.68%
29) Benzene-d6	8.27	84	316119	22.86	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.44%
33) 1,2-Dichloropropane-d6	9.27	67	90240	23.59	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.36%
37) Toluene-d8	10.33	98	277227	21.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.04%
38) trans-1,3-Dichloropropene-	10.58	79	32311	18.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.96%
39) 2-Hexanone-d5	10.93	63	21496	32.20	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.40%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	60556	18.17	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	72.68%
61) 1,2-Dichlorobenzene-d4	13.86	152	61332	19.61	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.44%

Target Compounds

				Ovalue
13) Acetone	4.14	43	1384m	2.050 ug/L
16) Methylene chloride	4.93	84	14447m	2.994 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

11/25/20 sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111720\
Data File : VW017283.D
Acq On : 17 Nov 2020 14:00
Operator : SY/VA
Sample : L4710-21RE
Misc : 4.46G/10ML/MSVOA W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AY5RE

Manual Integrations
APPROVED

MMDadoda
11/19/2020 11:09:21 AM

Quant Time: Nov 18 03:59:35 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 18 02:13:37 2020
Response via : Initial Calibration

