

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111720\
 Data File : VW017288.D
 Acq On : 17 Nov 2020 15:57
 Operator : SY/VA
 Sample : L4711-21
 Misc : 5.06G/10ML/MSVOA W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B07

Quant Time: Nov 18 04:19:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 18 02:13:37 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	377005	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	296093	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	86439	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	100955	21.26	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.04%
7) Chloroethane-d5	2.89	69	88982	24.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.28%
10) 1,1-Dichloroethene-d2	4.02	63	145686	17.15	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.60%
20) 2-Butanone-d5	7.09	46	24876	23.43	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	46.86%
24) Chloroform-d	7.65	84	226180	25.70	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.80%
26) 1,2-Dichloroethane-d4	8.31	65	112627	25.74	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.96%
29) Benzene-d6	8.28	84	411738	27.31	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	109.24%
33) 1,2-Dichloropropane-d6	9.27	67	120134	28.80	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	115.20%
37) Toluene-d8	10.33	98	358883	25.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.96%
38) trans-1,3-Dichloropropene-	10.58	79	34110	18.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.56%
39) 2-Hexanone-d5	10.93	63	19542	26.85	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	53.70%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	80000	22.02	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.08%
61) 1,2-Dichlorobenzene-d4	13.86	152	80105	26.30	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.20%


Target Compounds					Ovalue
16) Methylene chloride	4.92	84	12151	2.391 ug/L	93




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW111720\
Data File : VW017288.D
Acq On : 17 Nov 2020 15:57
Operator : SY/VA
Sample : L4711-21
Misc : 5.06G/10ML/MSVOA W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0B07

Quant Time: Nov 18 04:19:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM110420S.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 18 02:13:37 2020
Response via : Initial Calibration

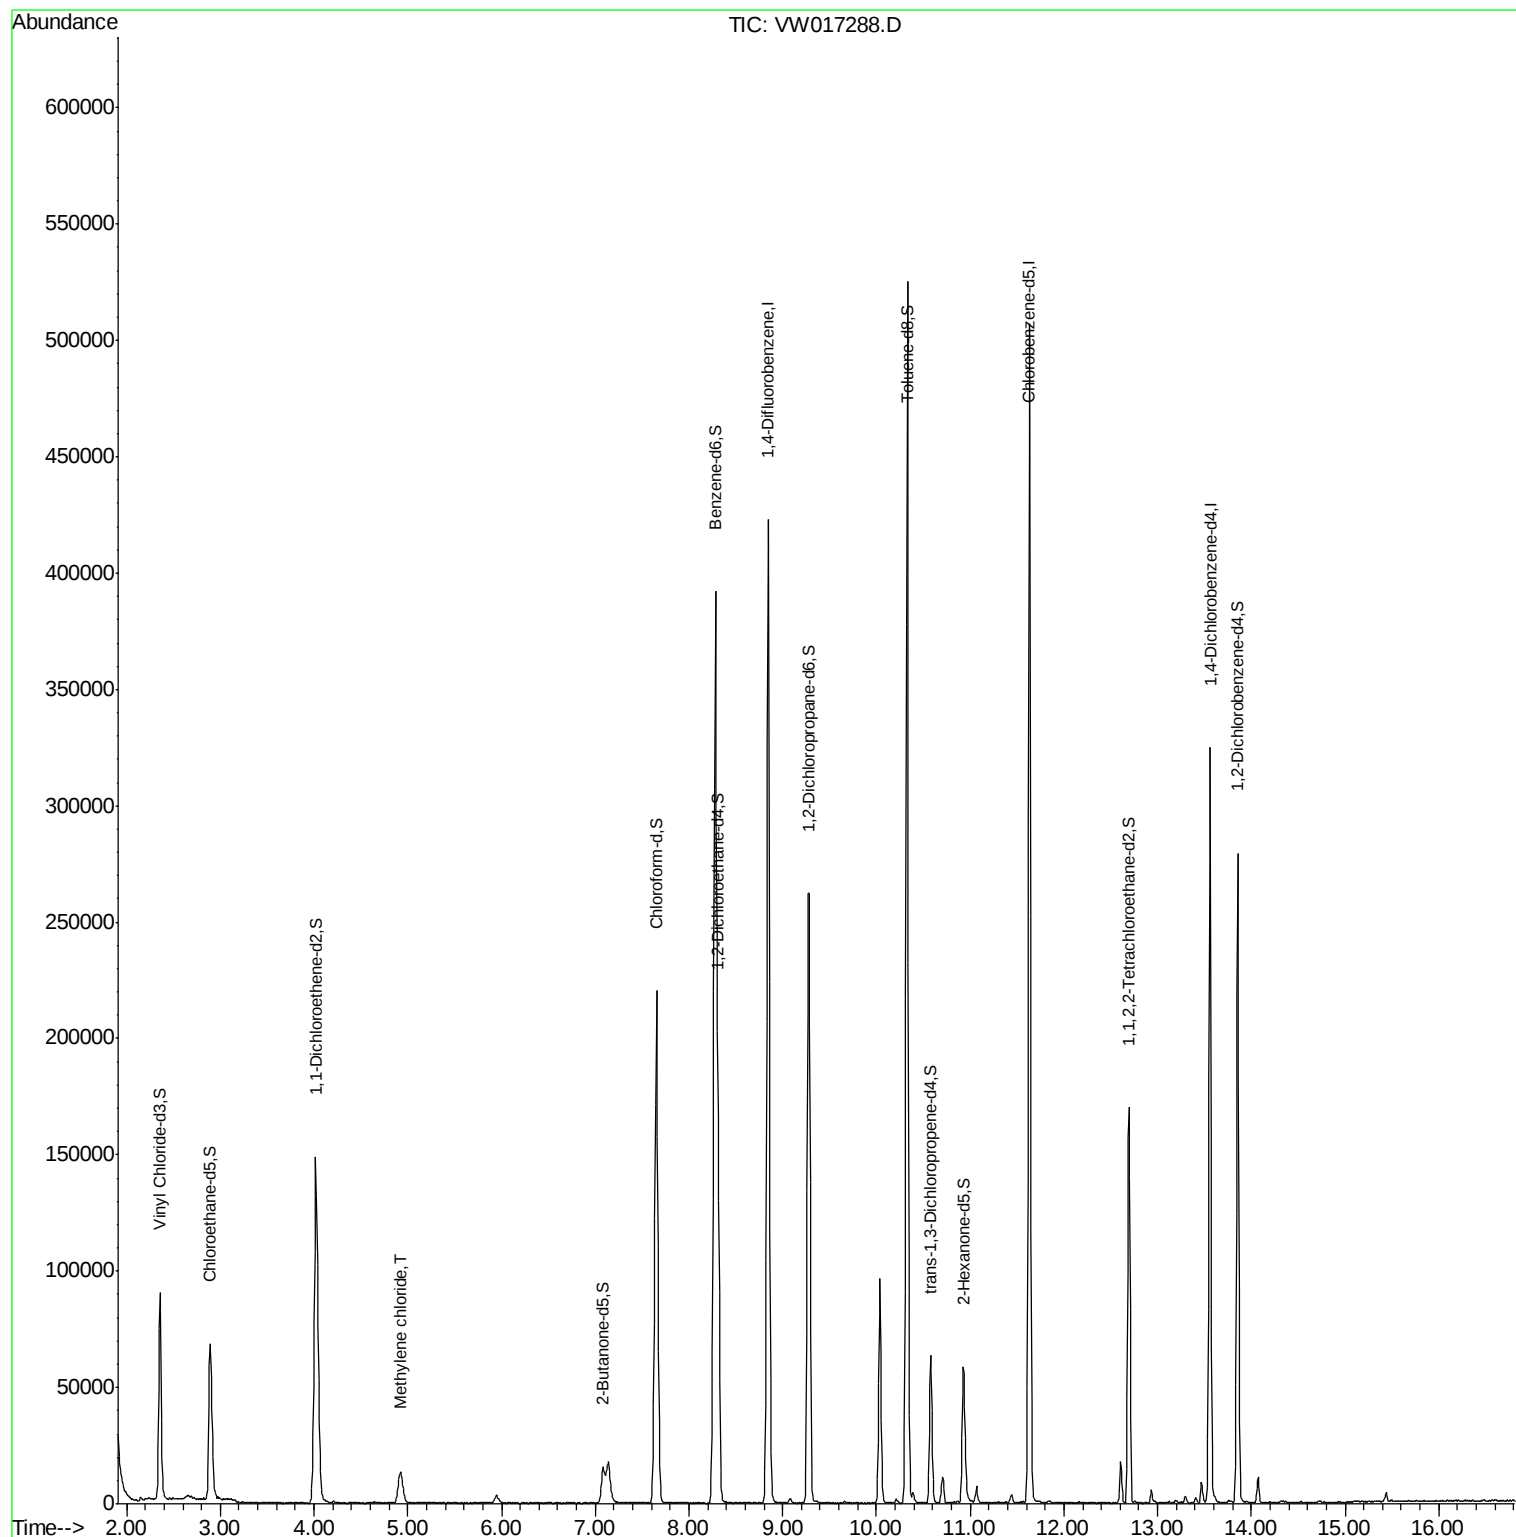

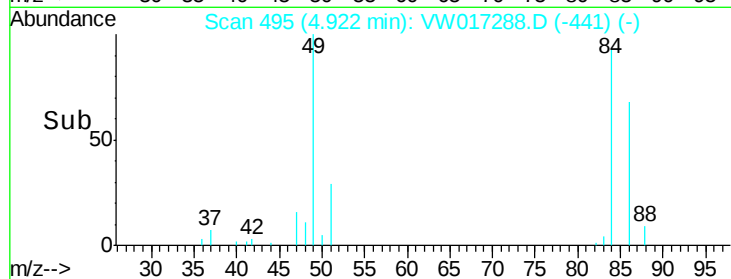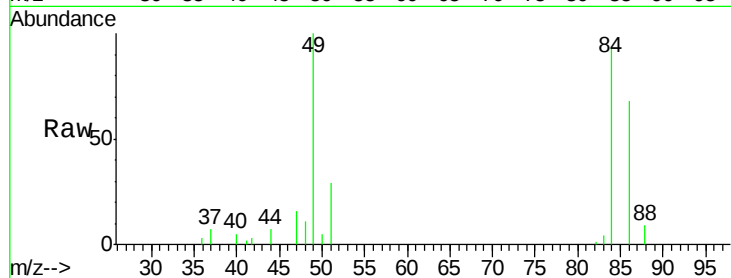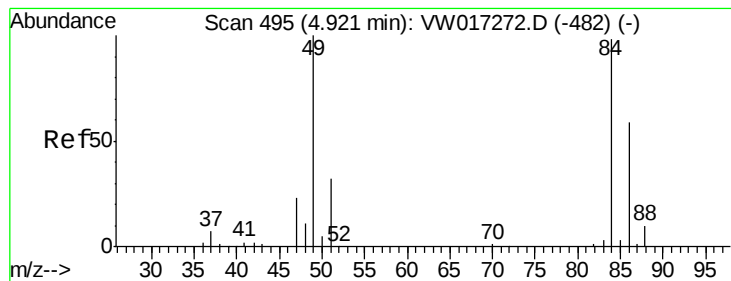

#16
 Methvlene chloride
 Concen: 2.391 ug/L
 RT: 4.92 min Scan# 495
 Delta R.T. 0.00 min
 Lab File: VW017288.D
 Acq: 17 Nov 2020 15:57

Instrument :
 MSVOA_W
 ClientSampleId :
 C0B07

Tot Ion: 84 Resp: 12151
 Ion Ratio Lower Upper
 84 100
 49 107.8 72.3 134.3
 86 72.8 45.1 83.7

