

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW111920\
Quantitation Report (Qedit)


Data File : VW017369.D
Acq On : 19 Nov 2020 14:12
Operator : SY/VA
Sample : L4793-03
Misc : 6.06G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BA3

Manual Integrations
APPROVED

MMDadoda
11/23/2020 1:43:44 PM

Quant Time: Nov 20 01:20:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 20 01:18:11 2020
Response via : Initial Calibration

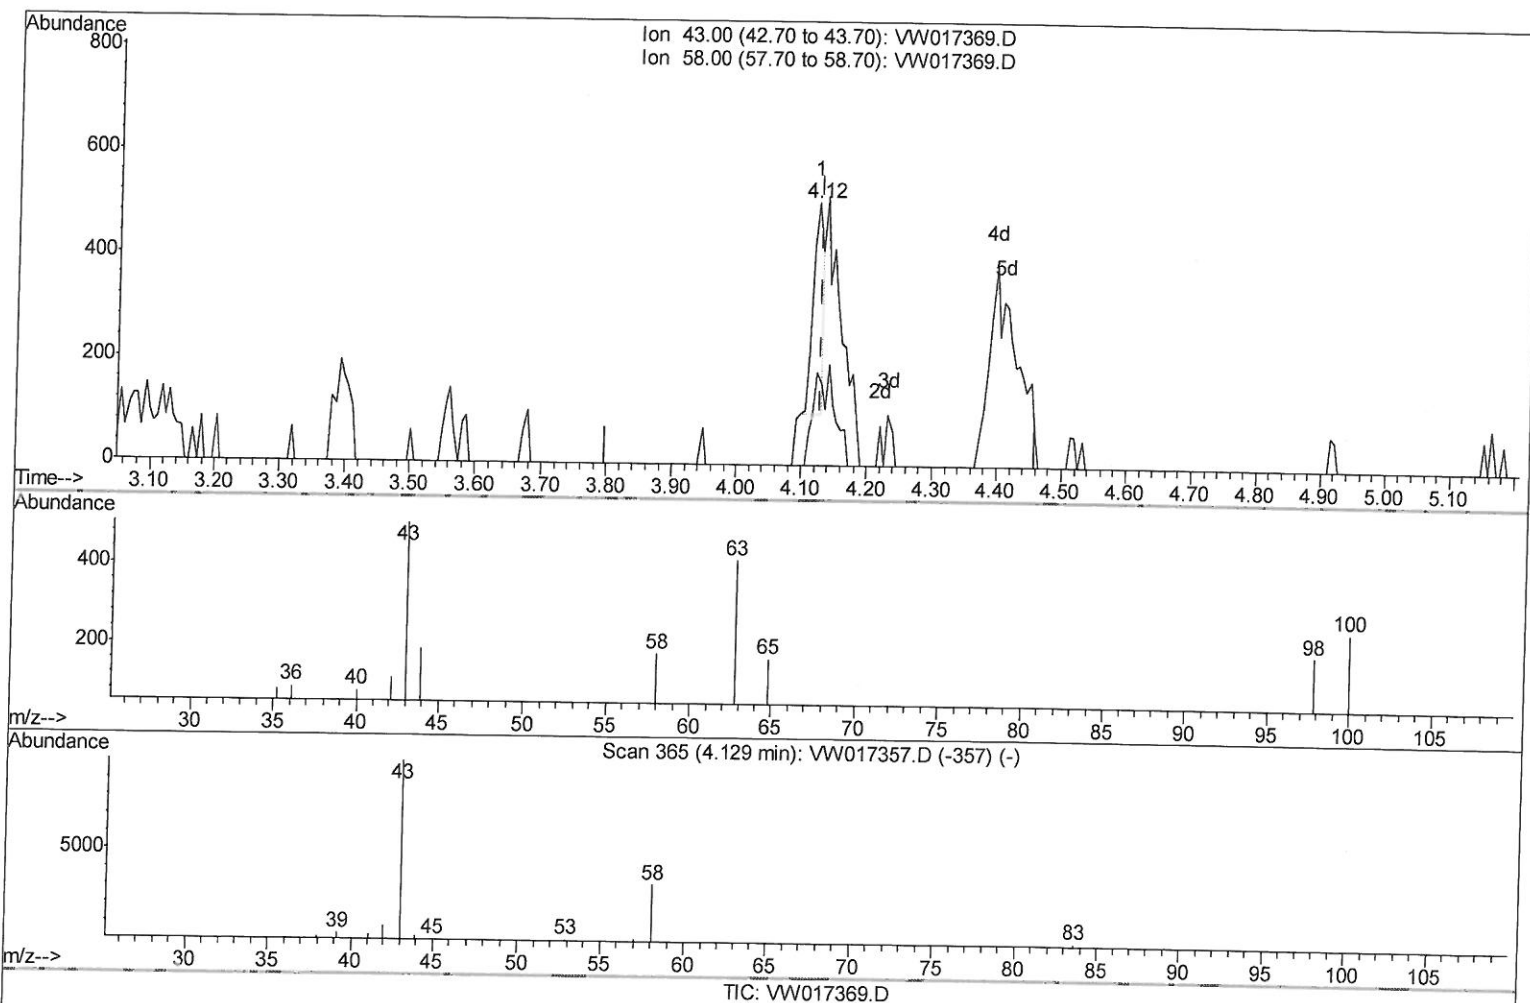

(13) Acetone (T)

4.123min (-0.006) 0.61ug/L

response 428

Ion	Exp%	Act%
43.00	100	100
58.00	33.50	51.87
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW111920\
Quantitation Report (Qedit)


Data File : VW017369.D
Acq On : 19 Nov 2020 14:12
Operator : SY/VA
Sample : L4793-03
Misc : 6.06G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BA3

Manual Integrations
APPROVED

MMDadoda
11/23/2020 1:43:44 PM

Quant Time: Nov 20 01:20:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 20 01:18:11 2020
Response via : Initial Calibration

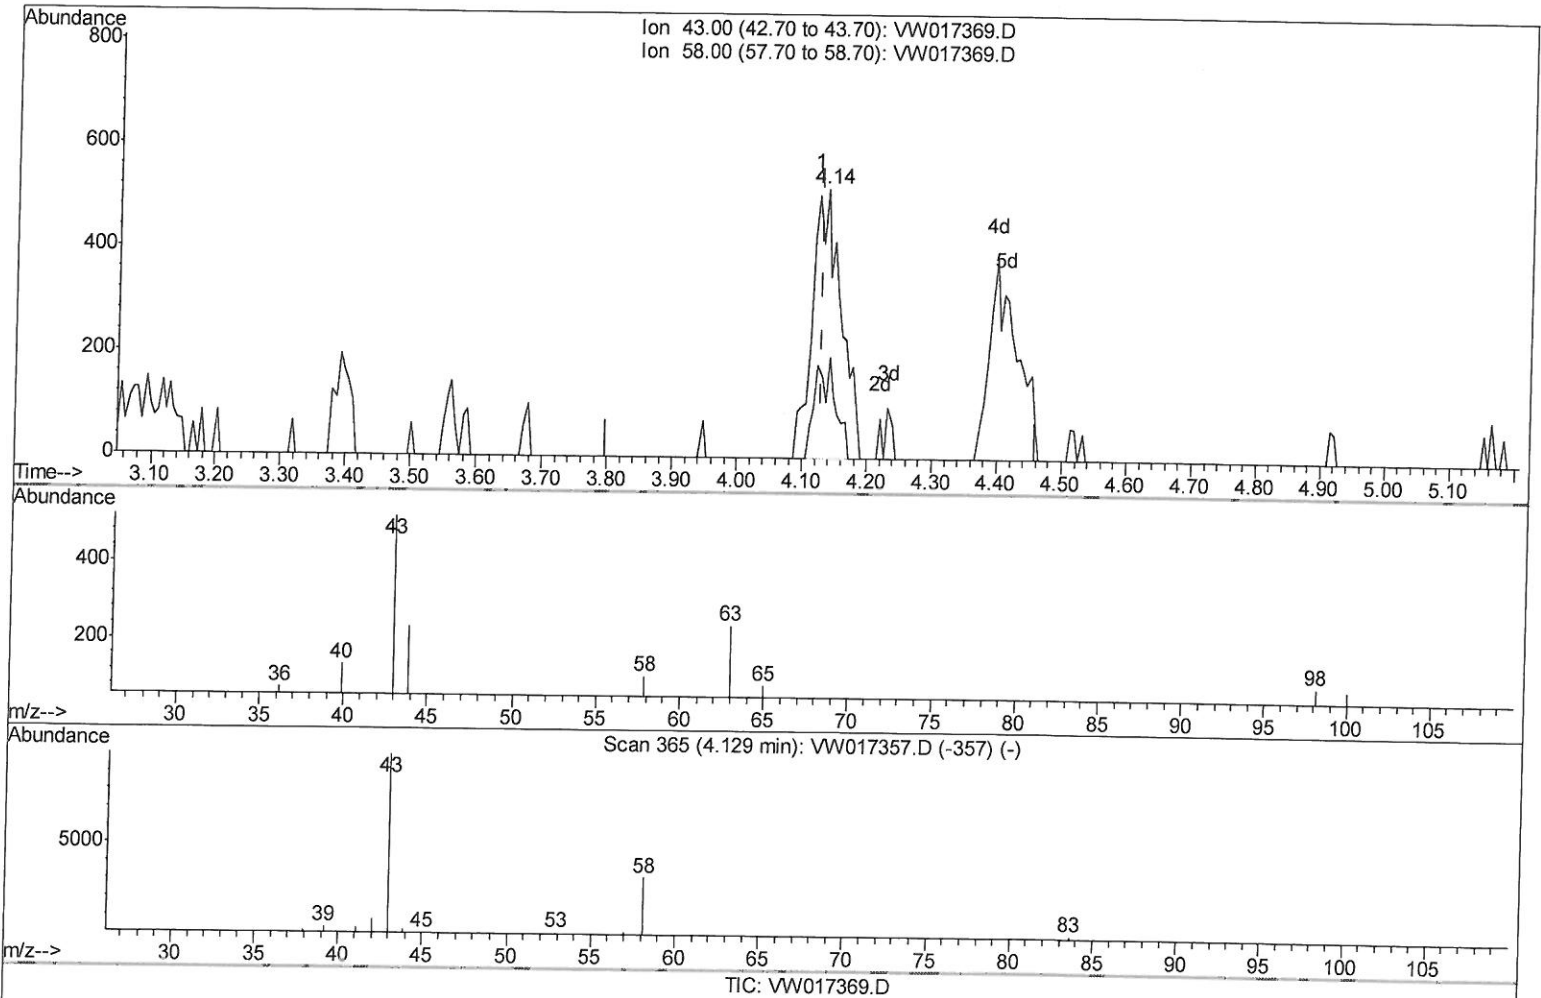

(13) Acetone (T)

4.135min (+0.006) 2.25ug/L m

11/25/20 SY

response 1589

Ion	Exp%	Act%
43.00	100	100
58.00	33.50	13.97
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW111920\
Quantitation Report (QT Reviewed)

Data File : VW017369.D
Acq On : 19 Nov 2020 14:12
Operator : SY/VA
Sample : L4793-03
Misc : 6.06G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BA3

Manual Integrations
APPROVED

MMDadoda
11/23/2020 1:43:44 PM

Quant Time: Nov 20 03:39:07 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 20 01:18:11 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	398095	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	361260	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	160200	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	129803	22.02	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.08%		
7) Chloroethane-d5	2.89	69	102260	21.84	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.36%		
10) 1,1-Dichloroethene-d2	4.02	63	164595	15.96	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	63.84%		
20) 2-Butanone-d5	7.08	46	33315	34.42	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	68.84%		
24) Chloroform-d	7.65	84	219169	20.96	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	83.84%		
26) 1,2-Dichloroethane-d4	8.31	65	101974	20.18	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	80.72%		
29) Benzene-d6	8.27	84	433804	21.30	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	85.20%		
33) 1,2-Dichloropropane-d6	9.27	67	116572	21.49	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	85.96%		
37) Toluene-d8	10.32	98	405241	21.14	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.56%		
38) trans-1,3-Dichloropropene-	10.58	79	45212	19.14	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	76.56%		
39) 2-Hexanone-d5	10.93	63	25426	34.95	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	69.90%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	78867	19.18	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	76.72%		
61) 1,2-Dichlorobenzene-d4	13.85	152	130030	21.99	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	87.96%		

Target Compounds

13) Acetone	4.14	43	1589m	2.250	ug/L	Qvalue
16) Methylene chloride	4.92	84	17716	2.602	ug/L	(11/25/2020) 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW111920\
Quantitation Report (QT Reviewed)

Data File : VW017369.D
Acq On : 19 Nov 2020 14:12
Operator : SY/VA
Sample : L4793-03
Misc : 6.06G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
C0BA3

Manual Integrations
APPROVED

MMDadoda
11/23/2020 1:43:44 PM

Quant Time: Nov 20 03:39:07 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 20 01:18:11 2020
Response via : Initial Calibration

