

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW111920\
Quantitation Report (Qedit)




Data File : VW017400.D
Acq On : 20 Nov 2020 03:28
Operator : SY/VA
Sample : L4794-20
Misc : 5.50G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BH3

Manual Integrations
APPROVED

MMDadoda
11/23/2020 1:44:44 PM

Quant Time: Nov 20 04:40:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 20 04:37:10 2020
Response via : Initial Calibration

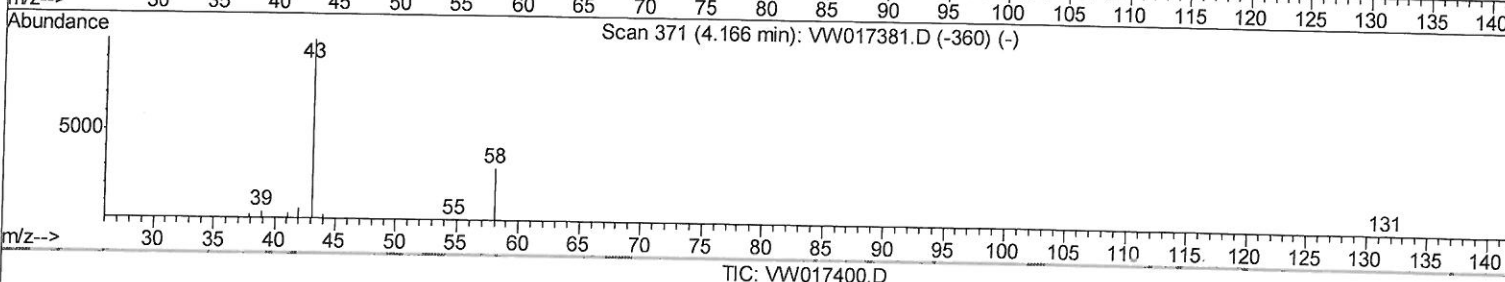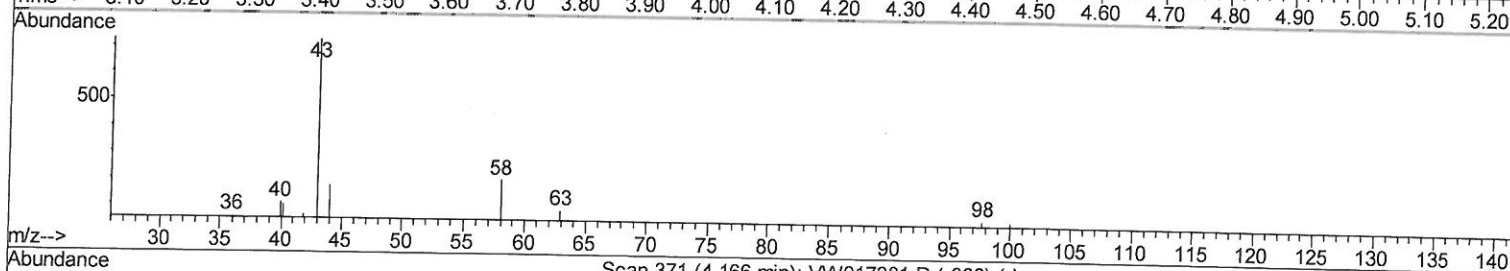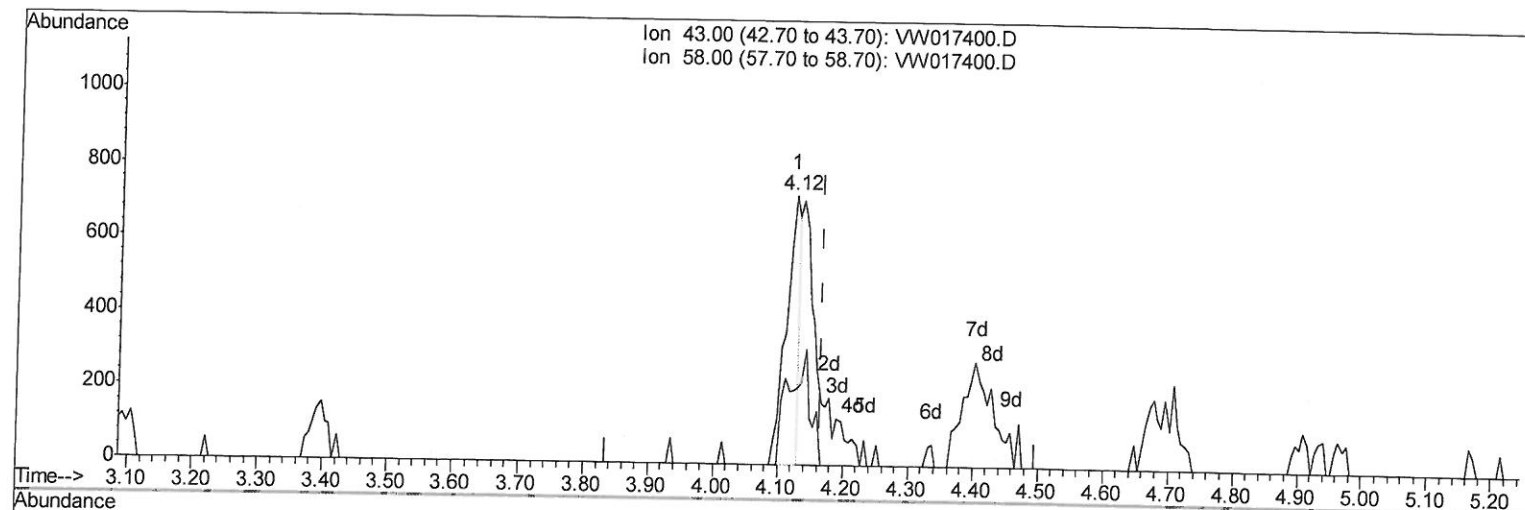

TIC: VW017400.D

(13) Acetone (T)

4.123min (-0.043) 1.61ug/L

response 1042

Ion	Exp%	Act%
43.00	100	100
58.00	33.50	21.31
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW111920\
Quantitation Report (Qedit)


Data File : VW017400.D
Acq On : 20 Nov 2020 03:28
Operator : SY/VA
Sample : L4794-20
Misc : 5.50G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BH3

Manual Integrations
APPROVED

MMDadoda
11/23/2020 1:44:44 PM

Quant Time: Nov 20 04:40:46 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 20 04:37:10 2020
Response via : Initial Calibration

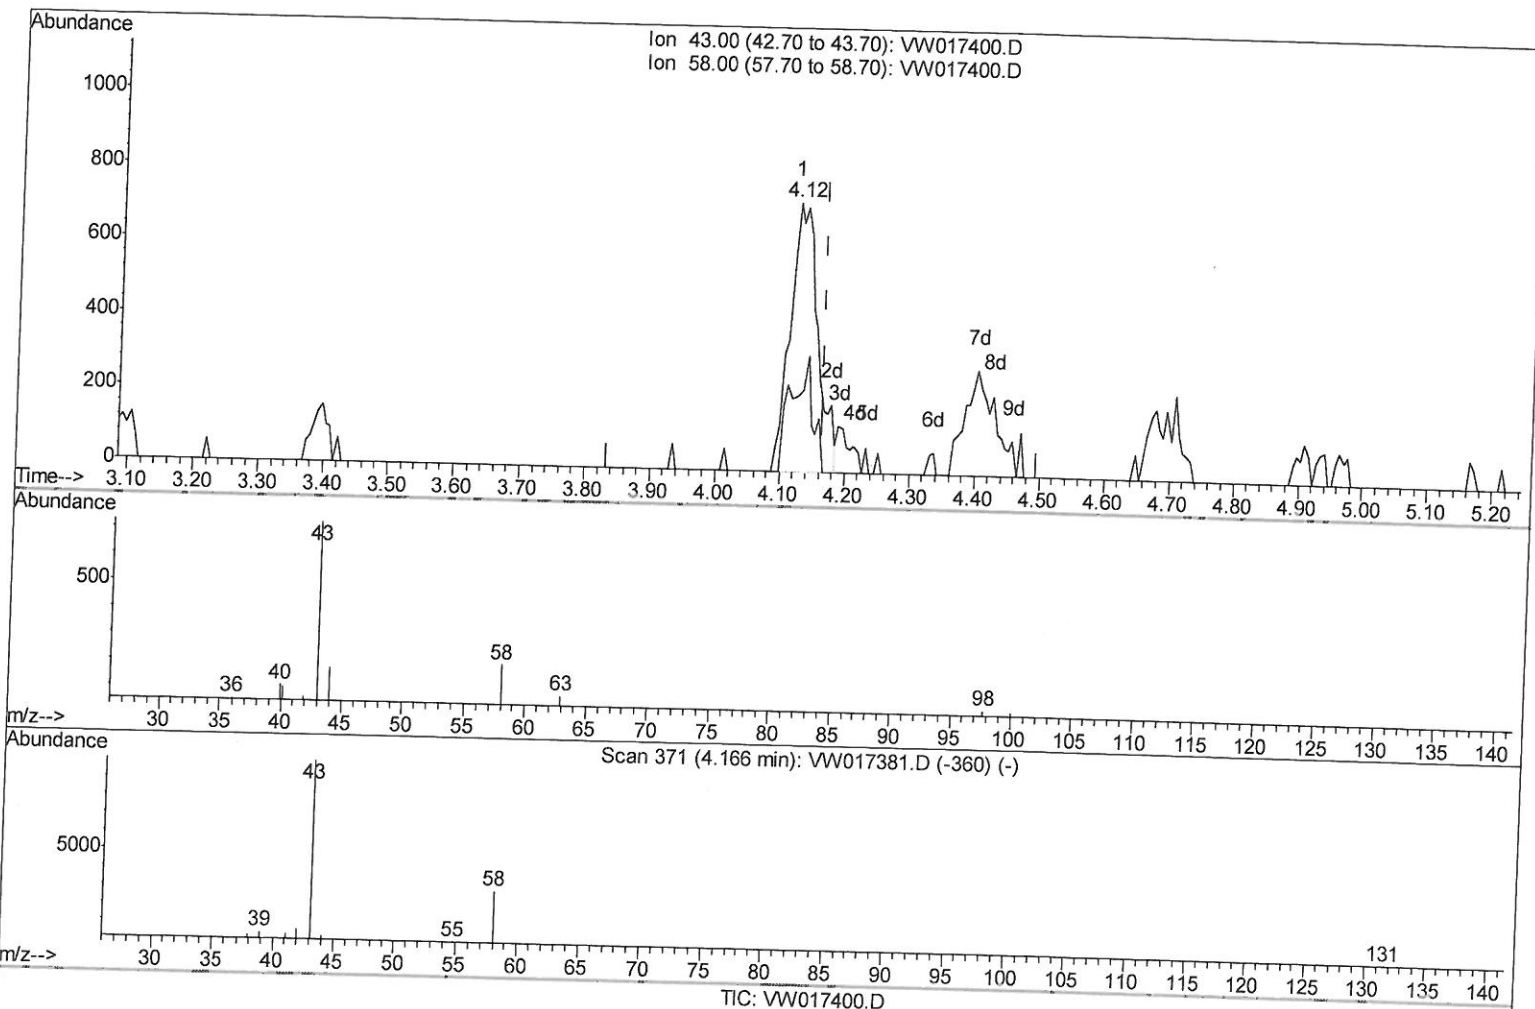

(13) Acetone (T)

4.123min (-0.043) 3.30ug/L m

response 2139

Ion	Exp%	Act%
43.00	100	100
58.00	33.50	10.38
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW111920\

Quantitation Report (QT Reviewed)

Data File : VW017400.D

Acq On : 20 Nov 2020 03:28

Operator : SY/VA

Sample : L4794-20

Misc : 5.50G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Instrument :

MSVOA_W

ClientSampleId :

C0BH3

Manual Integrations
APPROVED

MMDadoda

11/23/2020 1:44:44 PM

Quant Time: Nov 20 06:12:51 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M

Quant Title : VOC Analysis

QLast Update : Fri Nov 20 04:37:10 2020

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	365830	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	338591	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	153879	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	105483	19.48	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.92%		
7) Chloroethane-d5	2.89	69	91588	21.29	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.16%		
10) 1,1-Dichloroethene-d2	4.02	63	146737	15.49	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	61.96%		
20) 2-Butanone-d5	7.08	46	39530	44.44	ug/L	-0.01
Spiked Amount 50.000	Range 20 - 135		Recovery =	88.88%		
24) Chloroform-d	7.65	84	226704	23.59	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	94.36%		
26) 1,2-Dichloroethane-d4	8.31	65	115196	24.81	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	99.24%		
29) Benzene-d6	8.28	84	442224	23.17	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	92.68%		
33) 1,2-Dichloropropane-d6	9.27	67	124193	24.42	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	97.68%		
37) Toluene-d8	10.33	98	418923	23.31	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	93.24%		
38) trans-1,3-Dichloropropene-	10.58	79	48291	21.81	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	87.24%		
39) 2-Hexanone-d5	10.93	63	30637	44.93	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	89.86%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	95335	24.74	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	98.96%		
61) 1,2-Dichlorobenzene-d4	13.85	152	142145	25.02	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	100.08%		

Target Compounds

13) Acetone	4.12	43	2139m	3.296	ug/L	Qvalue
16) Methylene chloride	4.92	84	29570	4.726	ug/L	11/25/2014 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW111920\
Quantitation Report (QT Reviewed)

Data File : VW017400.D
Acq On : 20 Nov 2020 03:28
Operator : SY/VA
Sample : L4794-20
Misc : 5.50G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BH3

Manual Integrations
APPROVED

MMDadoda
11/23/2020 1:44:44 PM

Quant Time: Nov 20 06:12:51 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 20 04:37:10 2020
Response via : Initial Calibration

