

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW111920\
 Data File : VW017384.D
 Acq On : 19 Nov 2020 21:12
 Operator : SY/VA
 Sample : L4751-22
 Misc : 4.75G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AY2

Manual Integrations
 APPROVED

MMDadoda
 11/23/2020 1:44:05 PM

Quant Time: Nov 20 04:53:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 20 04:37:10 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	376868	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	321585	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	125405	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	111839	20.04	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.16%
7) Chloroethane-d5	2.89	69	92051	20.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.08%
10) 1,1-Dichloroethene-d2	4.03	63	143645	14.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.88%
20) 2-Butanone-d5	7.08	46	25010	27.30	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	54.60%
24) Chloroform-d	7.65	84	200821	20.28	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.12%
26) 1,2-Dichloroethane-d4	8.31	65	97419	20.36	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.44%
29) Benzene-d6	8.28	84	391707	21.61	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.44%
33) 1,2-Dichloropropane-d6	9.27	67	106994	22.15	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.60%
37) Toluene-d8	10.33	98	350278	20.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.08%
38) trans-1,3-Dichloropropene-	10.58	79	33854	16.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	64.40%
39) 2-Hexanone-d5	10.93	63	17755	27.42	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	54.84%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	70289	19.21	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.84%
61) 1,2-Dichlorobenzene-d4	13.86	152	93986	20.30	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.20%

Target Compounds				Ovalue
13) Acetone	4.13	43	2435m	3.642 ug/L
15) Methyl Acetate	4.67	43	4604	3.145 ug/L # 76
16) Methylene chloride	4.93	84	19477	3.021 ug/L 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW111920\
Data File : VW017384.D
Acq On : 19 Nov 2020 21:12
Operator : SY/VA
Sample : L4751-22
Misc : 4.75G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0AY2

Manual Integrations
APPROVED

MMDadoda
11/23/2020 1:44:05 PM

Quant Time: Nov 20 04:53:45 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111820S.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 20 04:37:10 2020
Response via : Initial Calibration

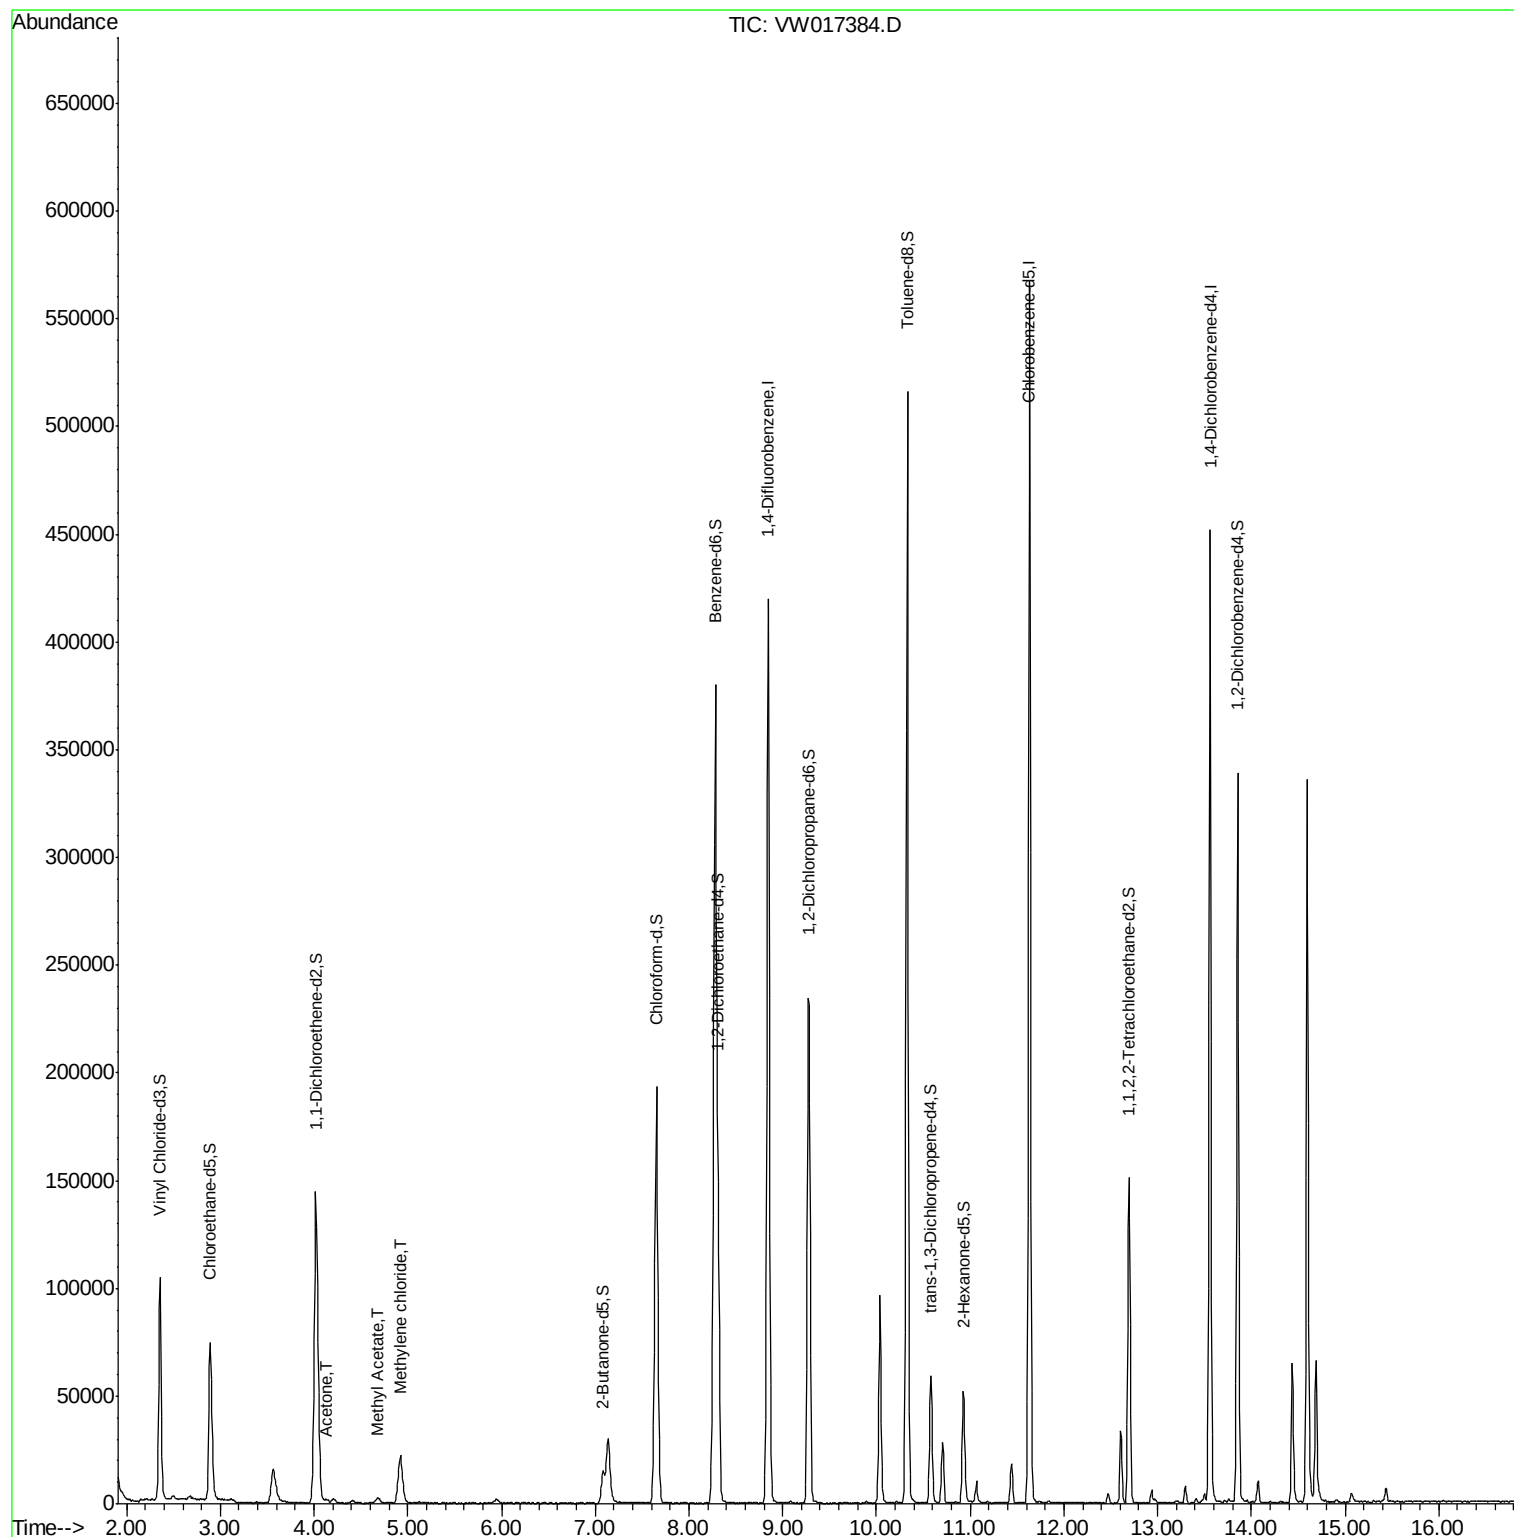

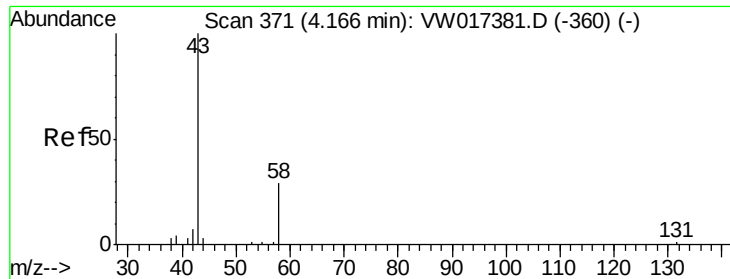

#13

Acetone

Concen: 3.642 ug/L m

RT: 4.13 min Scan# 365

Delta R.T. -0.04 min

Lab File: VW017384.D

Acq: 19 Nov 2020 21:12

Instrument :

MSVOA_W

ClientSampled :

C0AY2

Tot Ion: 43 Resp: 2435

Ion Ratio Lower Upper

43 100


58 31.9 0.0 67.0

Manual Integrations

APPROVED

MMDadoda

11/23/2020 1:44:05 PM

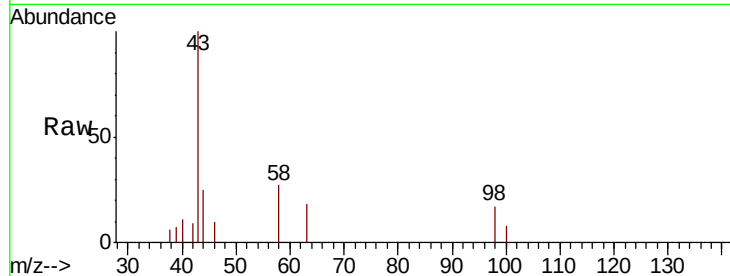

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

4.13

1000

800



600

400

200

0

Time-->

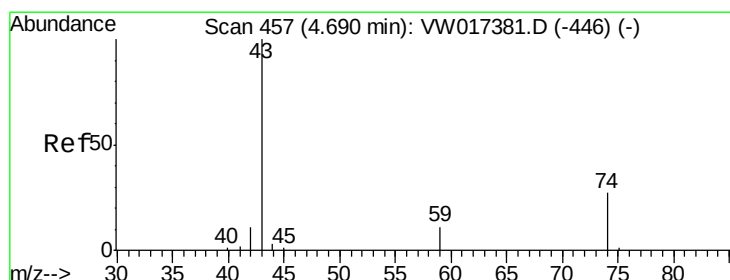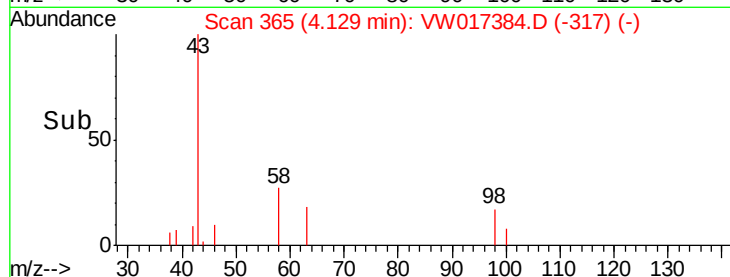

#15

Methyl Acetate

Concen: 3.145 ug/L

RT: 4.67 min Scan# 454

Delta R.T. -0.02 min

Lab File: VW017384.D


Acq: 19 Nov 2020 21:12

Tgt Ion: 43 Resp: 4604

Ion Ratio Lower Upper

43 100

74 16.5 23.7 35.5#

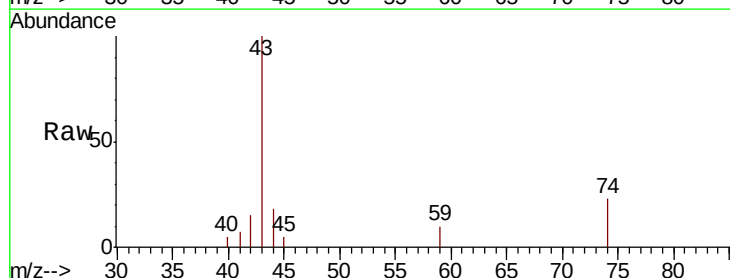

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 74.00 (73.70 to 74.70): VW

4.67


1500


1000

500

0

Time-->

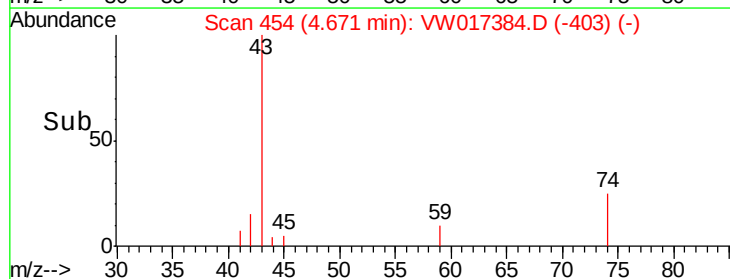

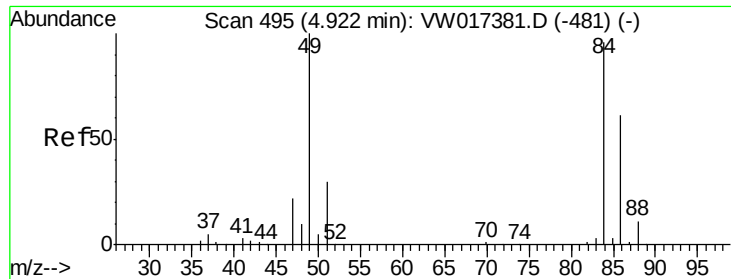

#16
 Methvlene chloride
 Concen: 3.021 ug/L
 RT: 4.93 min Scan# 496
 Delta R.T. 0.01 min
 Lab File: VW017384.D
 Acq: 19 Nov 2020 21:12

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AY2

Tot Ion:	84	Resp:	19477
Ion Ratio	Lower	Upper	
84	100		
49	96.9	71.5	132.9
86	65.2	42.8	79.4

Manual Integrations
 APPROVED

MMDadoda
 11/23/2020 1:44:05 PM

