

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120720\
 Data File : VW017579.D
 Acq On : 07 Dec 2020 15:05
 Operator : SY/VA
 Sample : L4955-09
 Misc : 5.63G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4K4

Manual Integrations
 APPROVED

MMDadoda
 12/21/2020 9:27:45 AM

Quant Time: Dec 20 03:56:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Dec 20 03:53:49 2020
 Response via : Initial Calibration

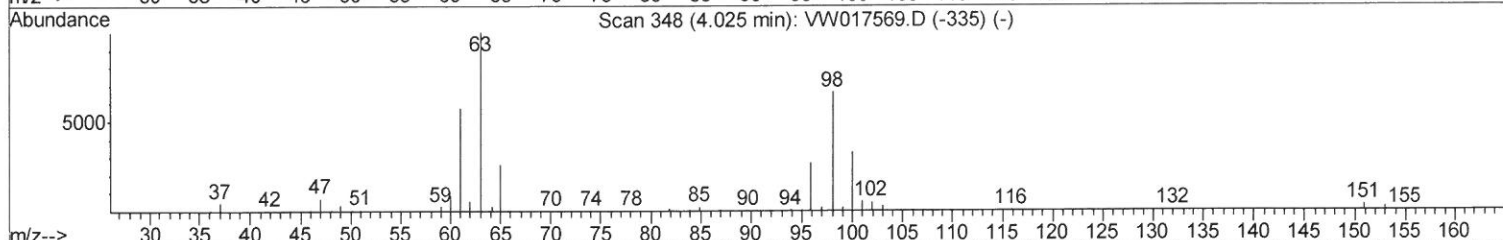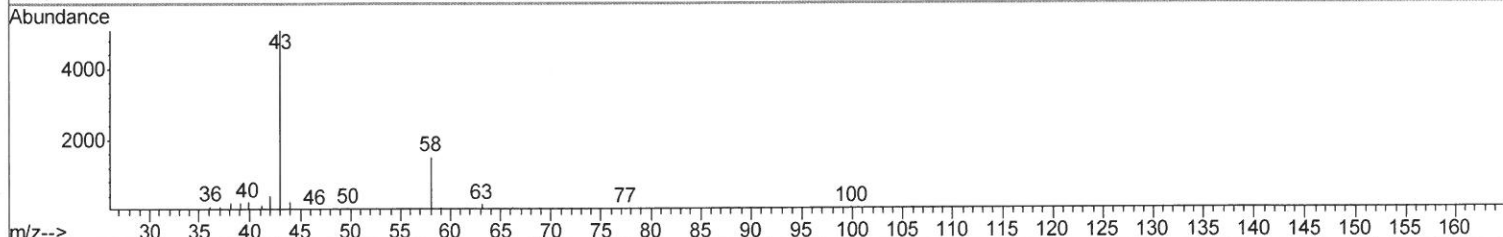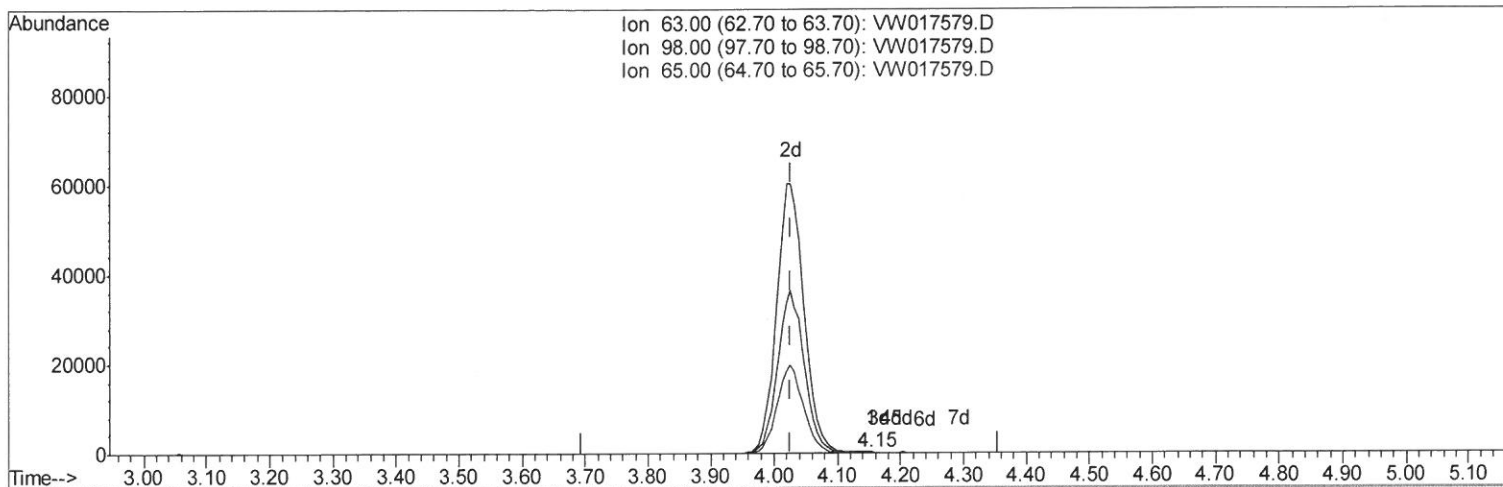

TIC: VW017579.D

(10) 1,1-Dichloroethene-d2 (S)

4.154min (+0.128) 0.01ug/L

response 125

Ion	Exp%	Act%
63.00	100	100
98.00	76.30	82.40
65.00	23.70	27.20
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120720\
Data File : VW017579.D
Acq On : 07 Dec 2020 15:05
Operator : SY/VA
Sample : L4955-09
Misc : 5.63G/10ML/MSVOA W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG4K4

Manual Integrations
APPROVED

MMDadoda
12/21/2020 9:27:45 AM

Quant Time: Dec 20 03:56:24 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
Quant Title : VOC Analysis
QLast Update : Sun Dec 20 03:53:49 2020
Response via : Initial Calibration

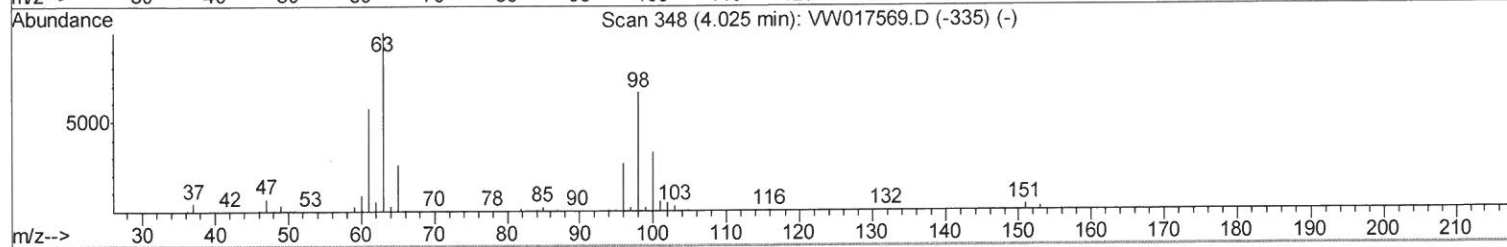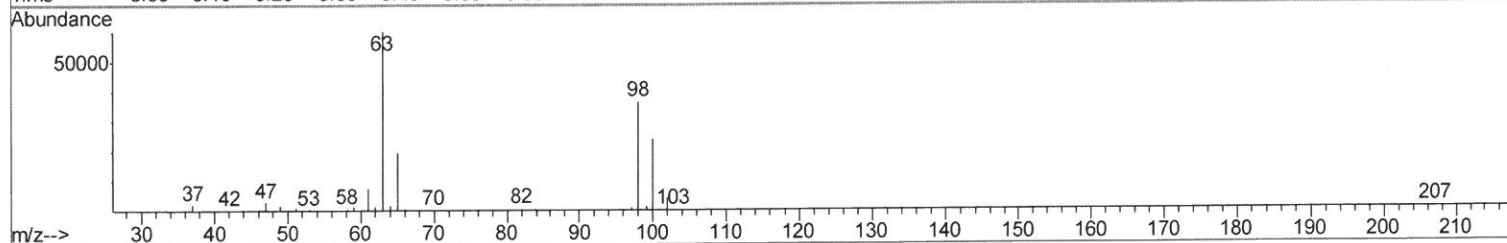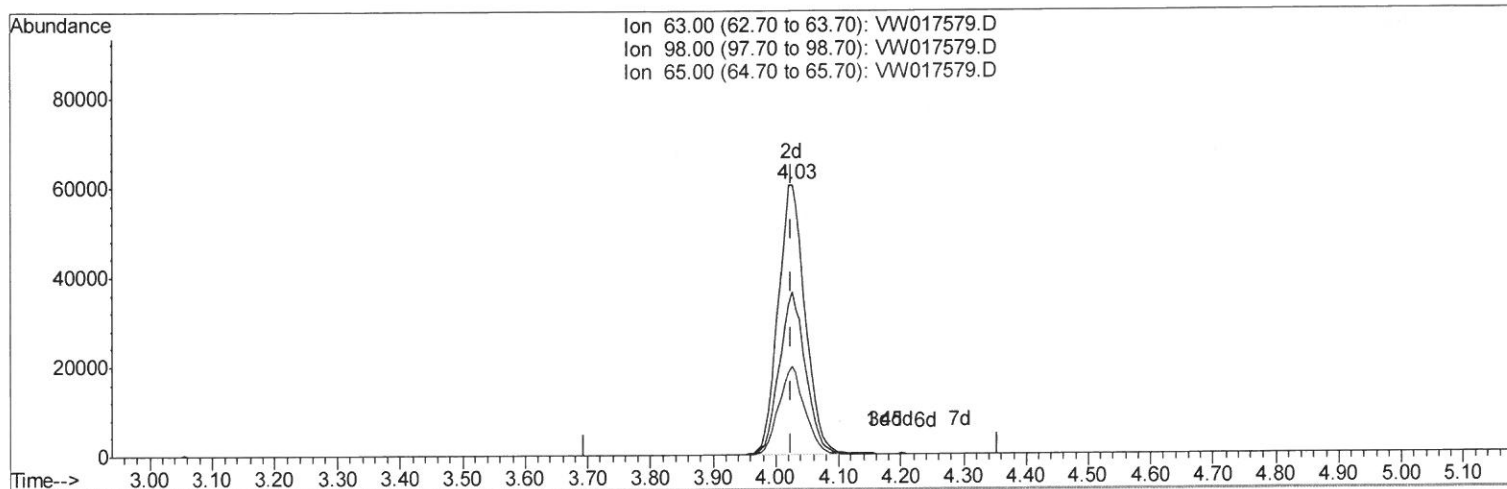

TIC: VW017579.D

(10) 1,1-Dichloroethene-d2 (S)

4.026min (+0.000) 14.31ug/L m

response 180849

Ion	Exp%	Act%
63.00	100	100
98.00	76.30	0.06#
65.00	23.70	0.02#
0.00	0.00	0.00

> 14/21/2020

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120720\
 Data File : VW017579.D
 Acq On : 07 Dec 2020 15:05
 Operator : SY/VA
 Sample : L4955-09
 Misc : 5.63G/10ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4K4

Manual Integrations
 APPROVED

MMDadoda
 12/21/2020 9:27:45 AM

Quant Time: Dec 20 04:20:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Dec 20 03:53:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	431368	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	393742	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	167874	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	99691	17.57	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.28%		
7) Chloroethane-d5	2.89	69	89124	18.61	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.44%		
10) 1,1-Dichloroethene-d2	4.03	63	180849m	14.31	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	57.24%		
20) 2-Butanone-d5	7.09	46	61012	50.99	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.98%		
24) Chloroform-d	7.65	84	267744	21.85	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.40%		
26) 1,2-Dichloroethane-d4	8.31	65	143167	23.81	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	95.24%		
29) Benzene-d6	8.27	84	507836	20.97	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	83.88%		
33) 1,2-Dichloropropane-d6	9.27	67	152324	22.74	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	90.96%		
37) Toluene-d8	10.32	98	454067	20.59	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	82.36%		
38) trans-1,3-Dichloropropene-	10.58	79	61370	20.50	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	82.00%		
39) 2-Hexanone-d5	10.93	63	42200	50.89	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.78%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	114026	23.65	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.60%		
61) 1,2-Dichlorobenzene-d4	13.86	152	144236	23.21	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	92.84%		

Target Compounds

					Ovalue
13) Acetone	4.14	43	20859	18.115	ug/L 94
14) Carbon disulfide	4.39	76	19383	1.133	ug/L # 92
16) Methylene chloride	4.92	84	30716	4.743	ug/L 92
35) Trichloroethene	9.09	95	96885	14.767	ug/L 98
47) Tetrachloroethene	10.87	164	1696194	303.438	ug/L 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120720\
Data File : VW017579.D
Acq On : 07 Dec 2020 15:05
Operator : SY/VA
Sample : L4955-09
Misc : 5.63G/10ML/MSVOA W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG4K4

Manual Integrations
APPROVED

MMDadoda
12/21/2020 9:27:45 AM

Quant Time: Dec 20 04:20:00 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
Quant Title : VOC Analysis
QLast Update : Sun Dec 20 03:53:49 2020
Response via : Initial Calibration

