


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121620\
 Data File : VW017649.D
 Acq On : 16 Dec 2020 08:51
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W121420S.M
 Title : SW846 8260
 Last Update : Mon Dec 14 12:39:23 2020

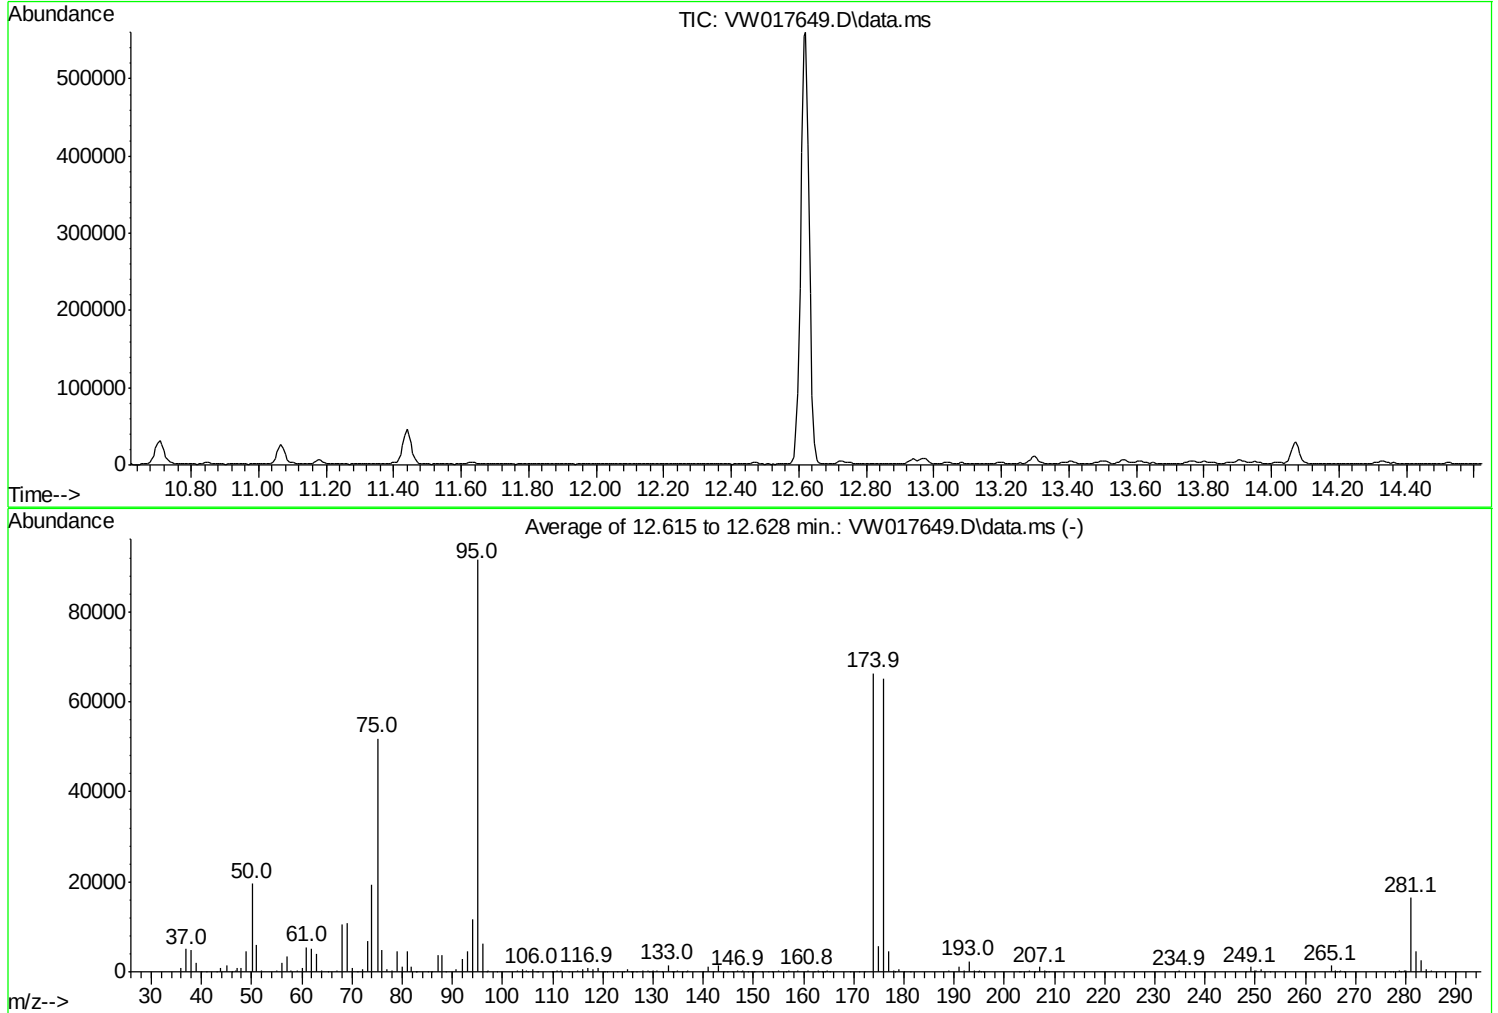

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	19519	PASS
75	95	30	60	56.6	51837	PASS
95	95	100	100	100.0	91557	PASS
96	95	5	9	7.0	6378	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.5	66363	PASS
175	174	5	9	8.5	5638	PASS
176	174	95	101	98.3	65251	PASS
177	176	5	9	7.0	4582	PASS