




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122021\
Data File : VW021502.D
Acq On : 20 Dec 2021 16:48
Operator : SY/VA
Sample : M5171-13
Misc : 6.35g/10.0mL/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLA9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2021
Supervised By :Amit Patel 12/24/2021

Quant Time: Dec 20 18:54:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 18 00:55:20 2021
Response via : Initial Calibration

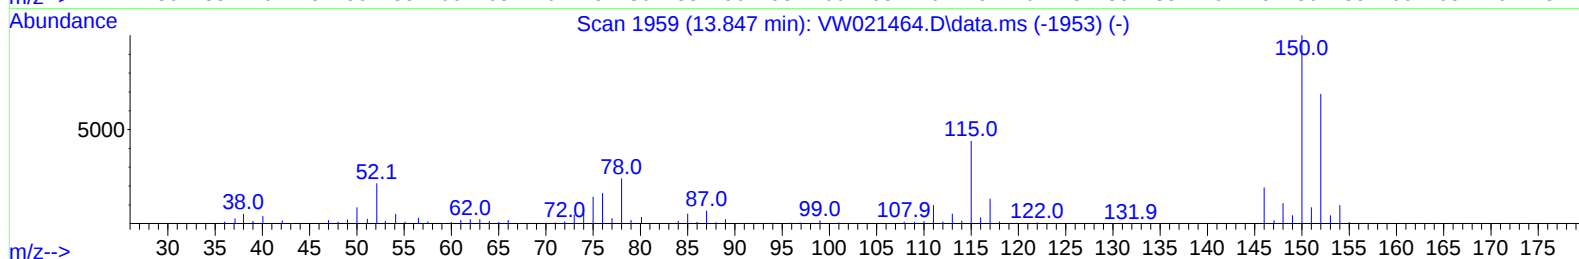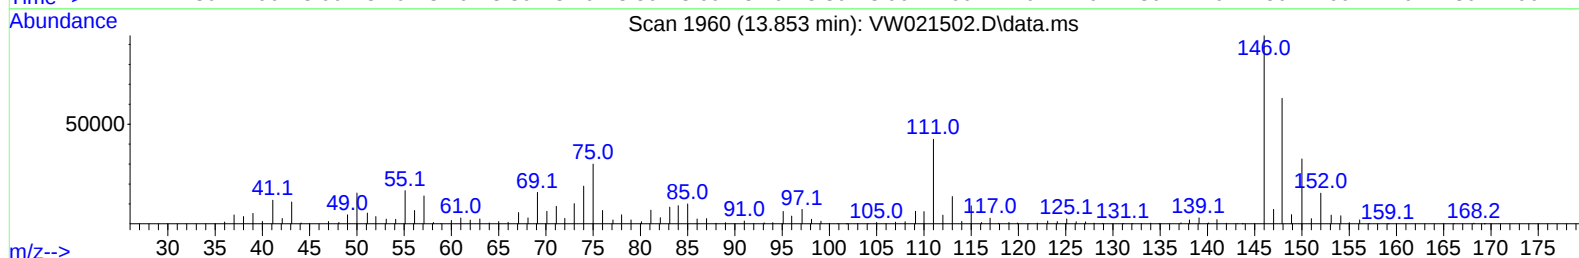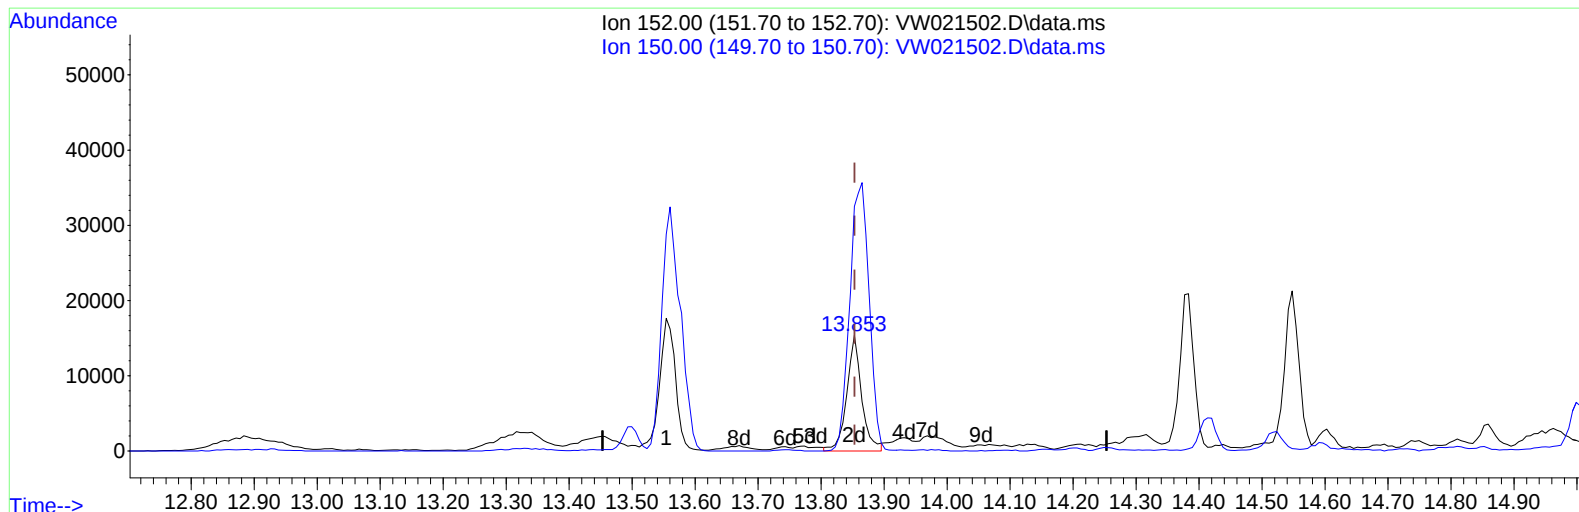

TIC: VW021502.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

13.853min (-0.000) 21.33 ug/L m

response 25361

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	1	




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122021\
Data File : VW021502.D
Acq On : 20 Dec 2021 16:48
Operator : SY/VA
Sample : M5171-13
Misc : 6.35g/10.0mL/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLA9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2021
Supervised By :Amit Patel 12/24/2021

Quant Time: Dec 20 18:54:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 18 00:55:20 2021
Response via : Initial Calibration

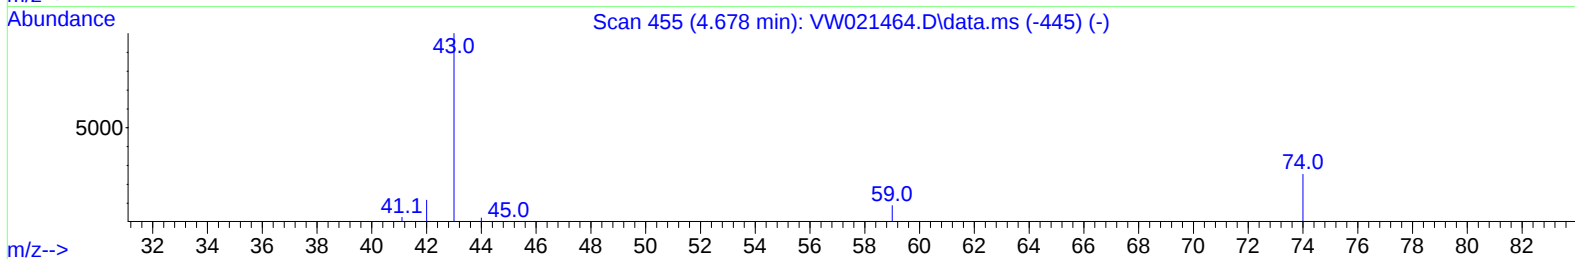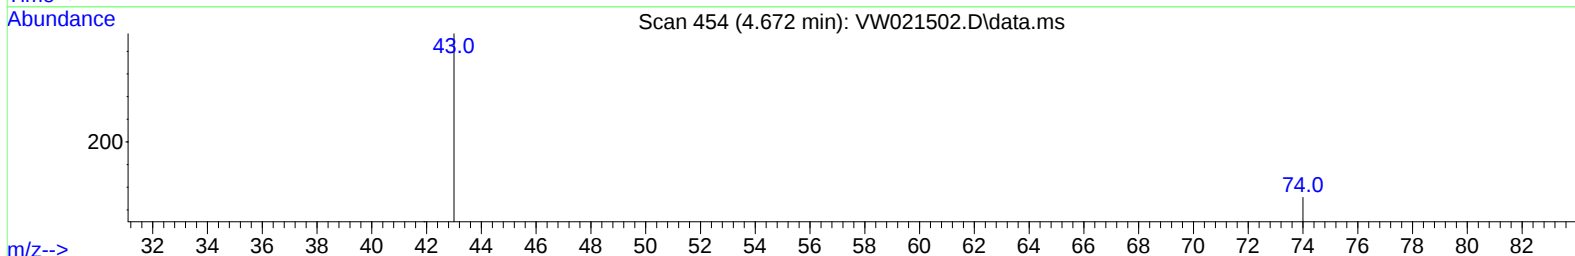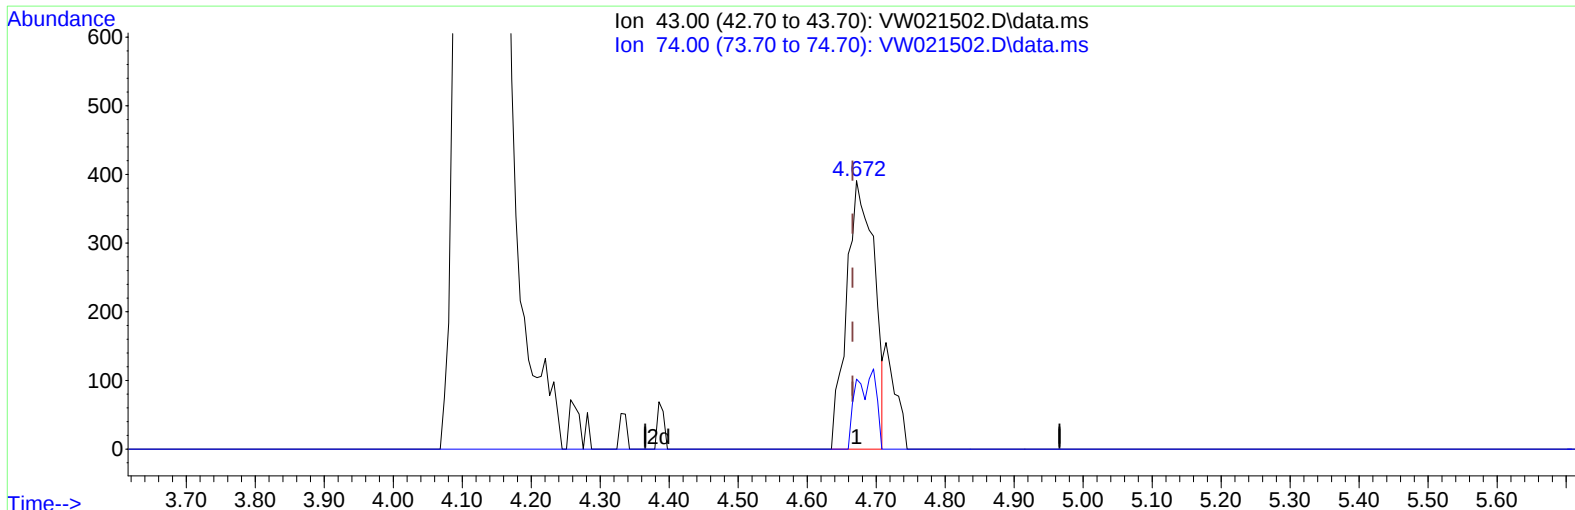

TIC: VW021502.D\data.ms

(15) Methyl Acetate (T)

4.672min (+ 0.006) 2.14 ug/L

response 1086

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	20.50	11.33#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122021\
Data File : VW021502.D
Acq On : 20 Dec 2021 16:48
Operator : SY/VA
Sample : M5171-13
Misc : 6.35g/10.0mL/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLA9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2021
Supervised By :Amit Patel 12/24/2021

Quant Time: Dec 20 18:54:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 18 00:55:20 2021
Response via : Initial Calibration

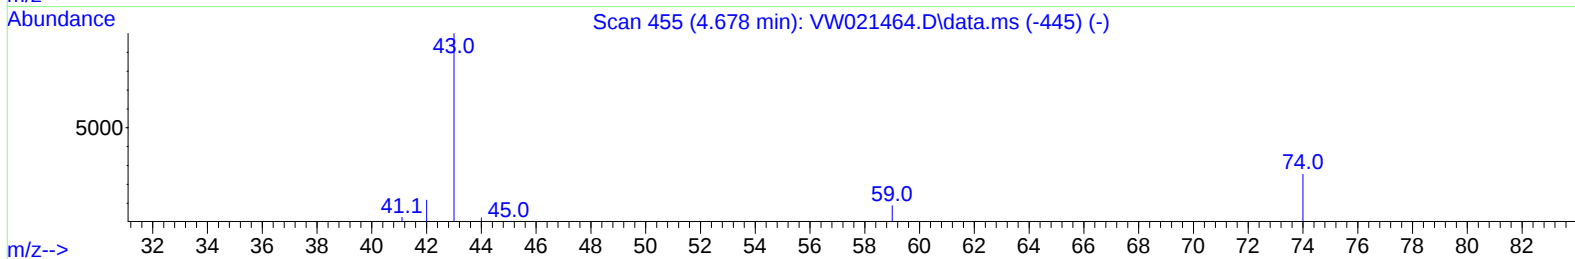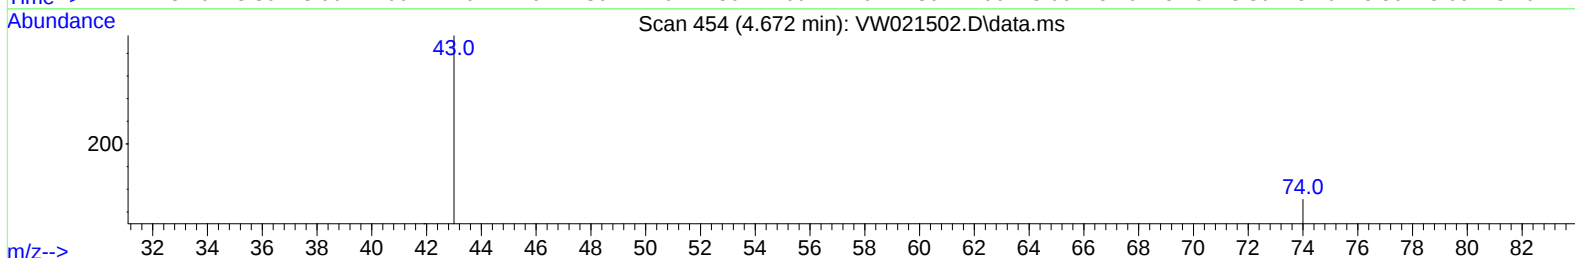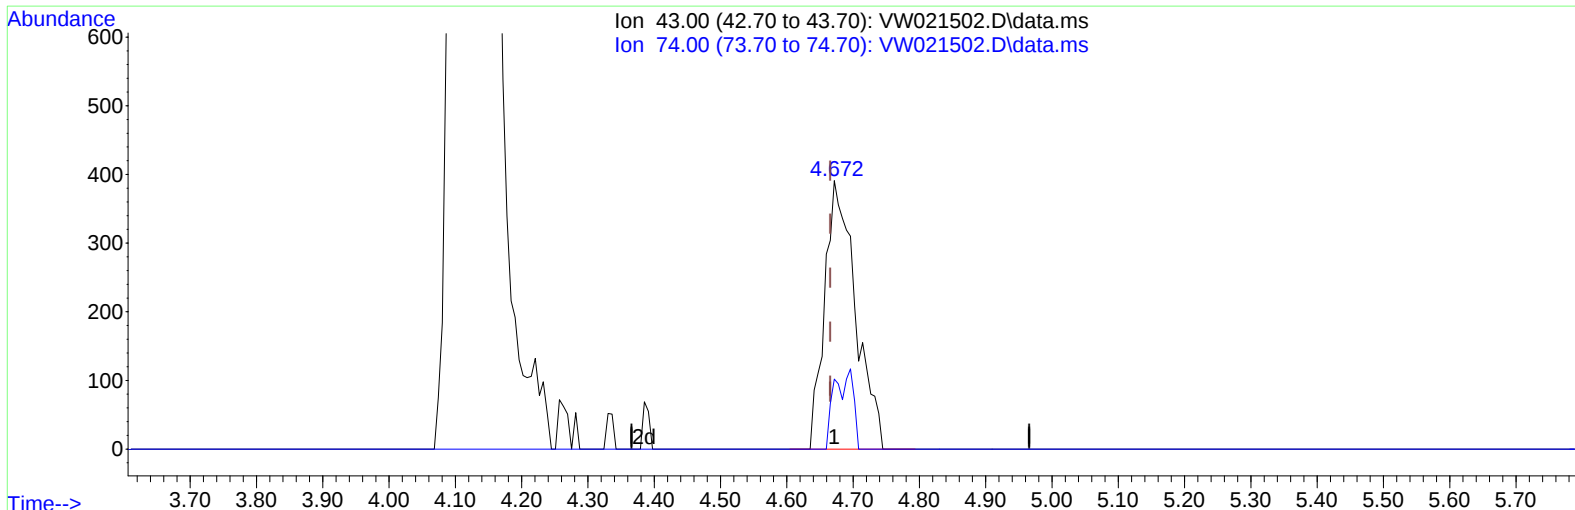

TIC: VW021502.D\data.ms

(15) Methyl Acetate (T)

4.672min (+ 0.006) 2.48 ug/L m

response 1262

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	20.50	9.75#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122021\
Data File : VW021502.D
Acq On : 20 Dec 2021 16:48
Operator : SY/VA
Sample : M5171-13
Misc : 6.35g/10.0mL/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLA9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2021
Supervised By :Amit Patel 12/24/2021

Quant Time: Dec 20 18:54:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 18 00:55:20 2021
Response via : Initial Calibration

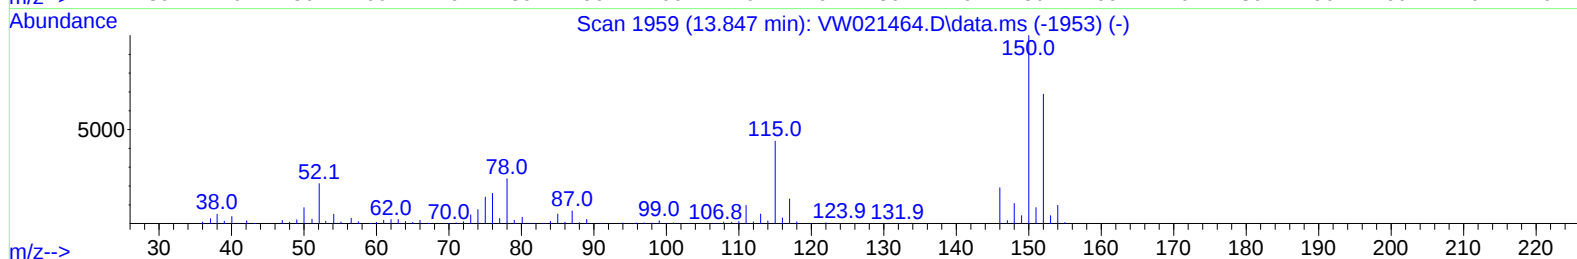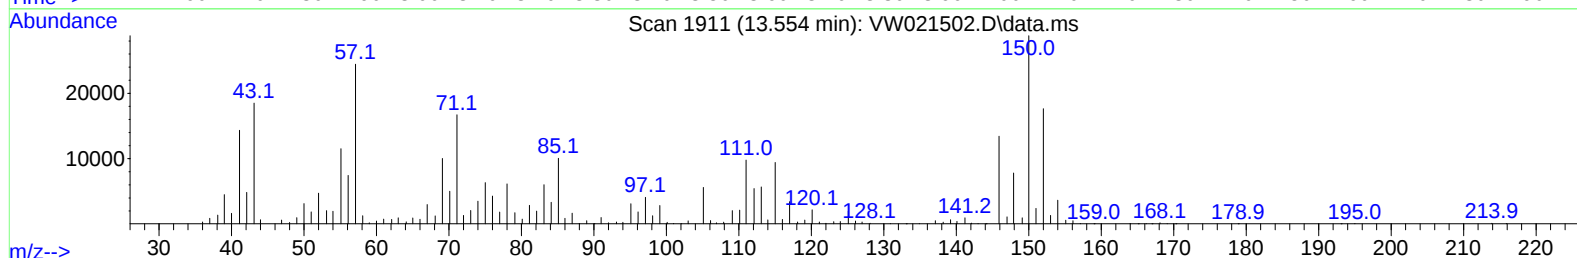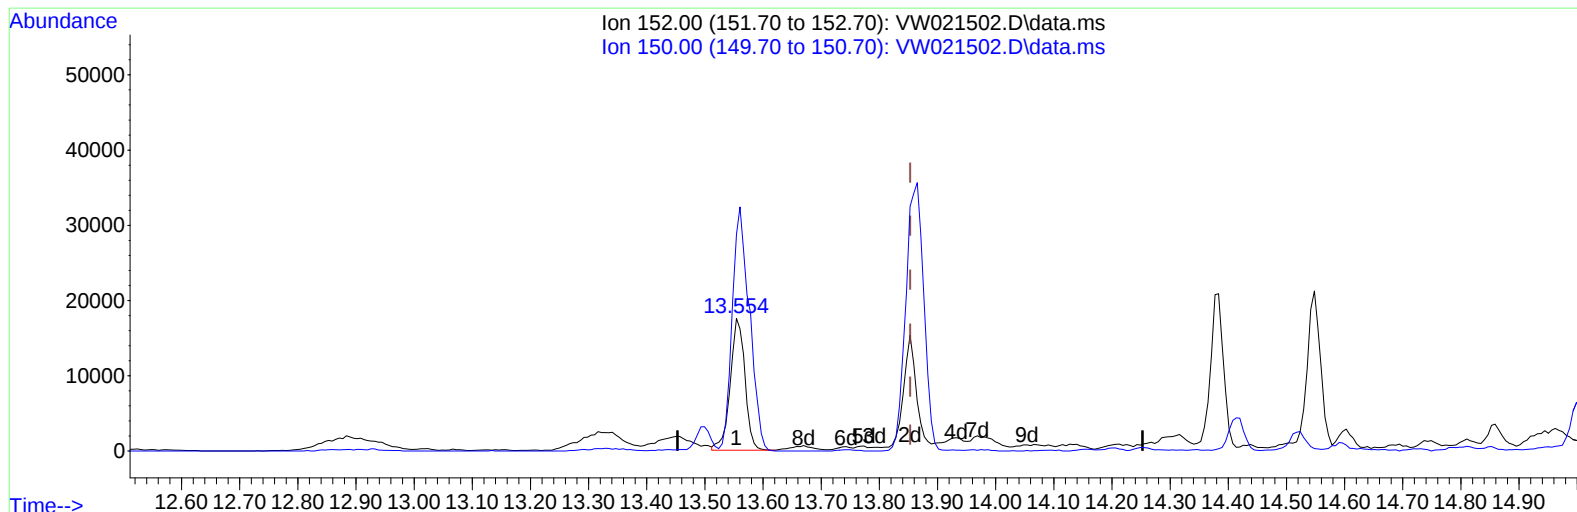

TIC: VW021502.D\data.ms

(66) 1,2-Dichlorobenzene-d4 (S)

13.554min (-0.299) 25.80 ug/L

response 30685

Ion	Exp%	Act%
152.00	100.00	100.00
150.00	172.50	217.70
0.00		

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122021\
 Data File : VW021502.D
 Acq On : 20 Dec 2021 16:48
 Operator : SY/VA
 Sample : M5171-13
 Misc : 6.35g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLA9

Manual IntegrationsAPPROVED

Quant Time: Dec 20 18:54:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 18 00:55:20 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/20/2021
 Supervised By :Amit Patel 12/24/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	128044	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	94274	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	30685	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	21395	9.174	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	36.680%
7) Chloroethane-d5	2.885	69	19412	12.592	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	50.360%
11) 1,1-Dichloroethene-d2	4.019	63	37370	12.020	ug/L	0.00
Spiked Amount	25.000					

Instrument :

MSVOA_W

ClientSampleId :

BGLA9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2021

Supervised By :Amit Patel 12/24/2021

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122021\
Data File : VW021502.D
Acq On : 20 Dec 2021 16:48
Operator : SY/VA
Sample : M5171-13
Misc : 6.35g/10.0mL/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLA9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/20/2021
Supervised By :Amit Patel 12/24/2021

Quant Time: Dec 20 18:54:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 18 00:55:20 2021
Response via : Initial Calibration

