

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122021\
 Data File : VW021508.D
 Acq On : 20 Dec 2021 19:16
 Operator : SY/VA
 Sample : M5125-01
 Misc : 6.190g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0AN4

Quant Time: Dec 20 21:32:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 18 00:55:20 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	167170	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	156969	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	80824	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	39179	12.868	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	51.480%
7) Chloroethane-d5	2.879	69	25747	12.792	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	51.160%
11) 1,1-Dichloroethene-d2	4.013	63	58113	14.317	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.280%
21) 2-Butanone-d5	7.092	46	19473	45.374	ug/L	0.02
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.740%
24) Chloroform-d	7.647	84	84062	18.044	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	72.160%
26) 1,2-Dichloroethane-d4	8.305	65	47333	19.101	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	76.400%
32) Benzene-d6	8.275	84	171169	19.894	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.560%
36) 1,2-Dichloropropane-d6	9.275	67	47073	20.400	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.600%
41) Toluene-d8	10.323	98	167218	19.021	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.080%
43) trans-1,3-Dichloroprop...	10.579	79	20712	19.494	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.960%
47) 2-Hexanone-d5	10.927	63	17504	51.299	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.600%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	40166	20.249	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.000%
66) 1,2-Dichlorobenzene-d4	13.853	152	58864	18.792	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	75.160%
Target Compounds						
63) 1,2,4-Trimethylbenzene	13.249	105	5711	0.619	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW122021\
Data File : VW021508.D
Acq On : 20 Dec 2021 19:16
Operator : SY/VA
Sample : M5125-01
Misc : 6.190g/10.0mL/MSVOA_W/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
H0AN4

Quant Time: Dec 20 21:32:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 18 00:55:20 2021
Response via : Initial Calibration

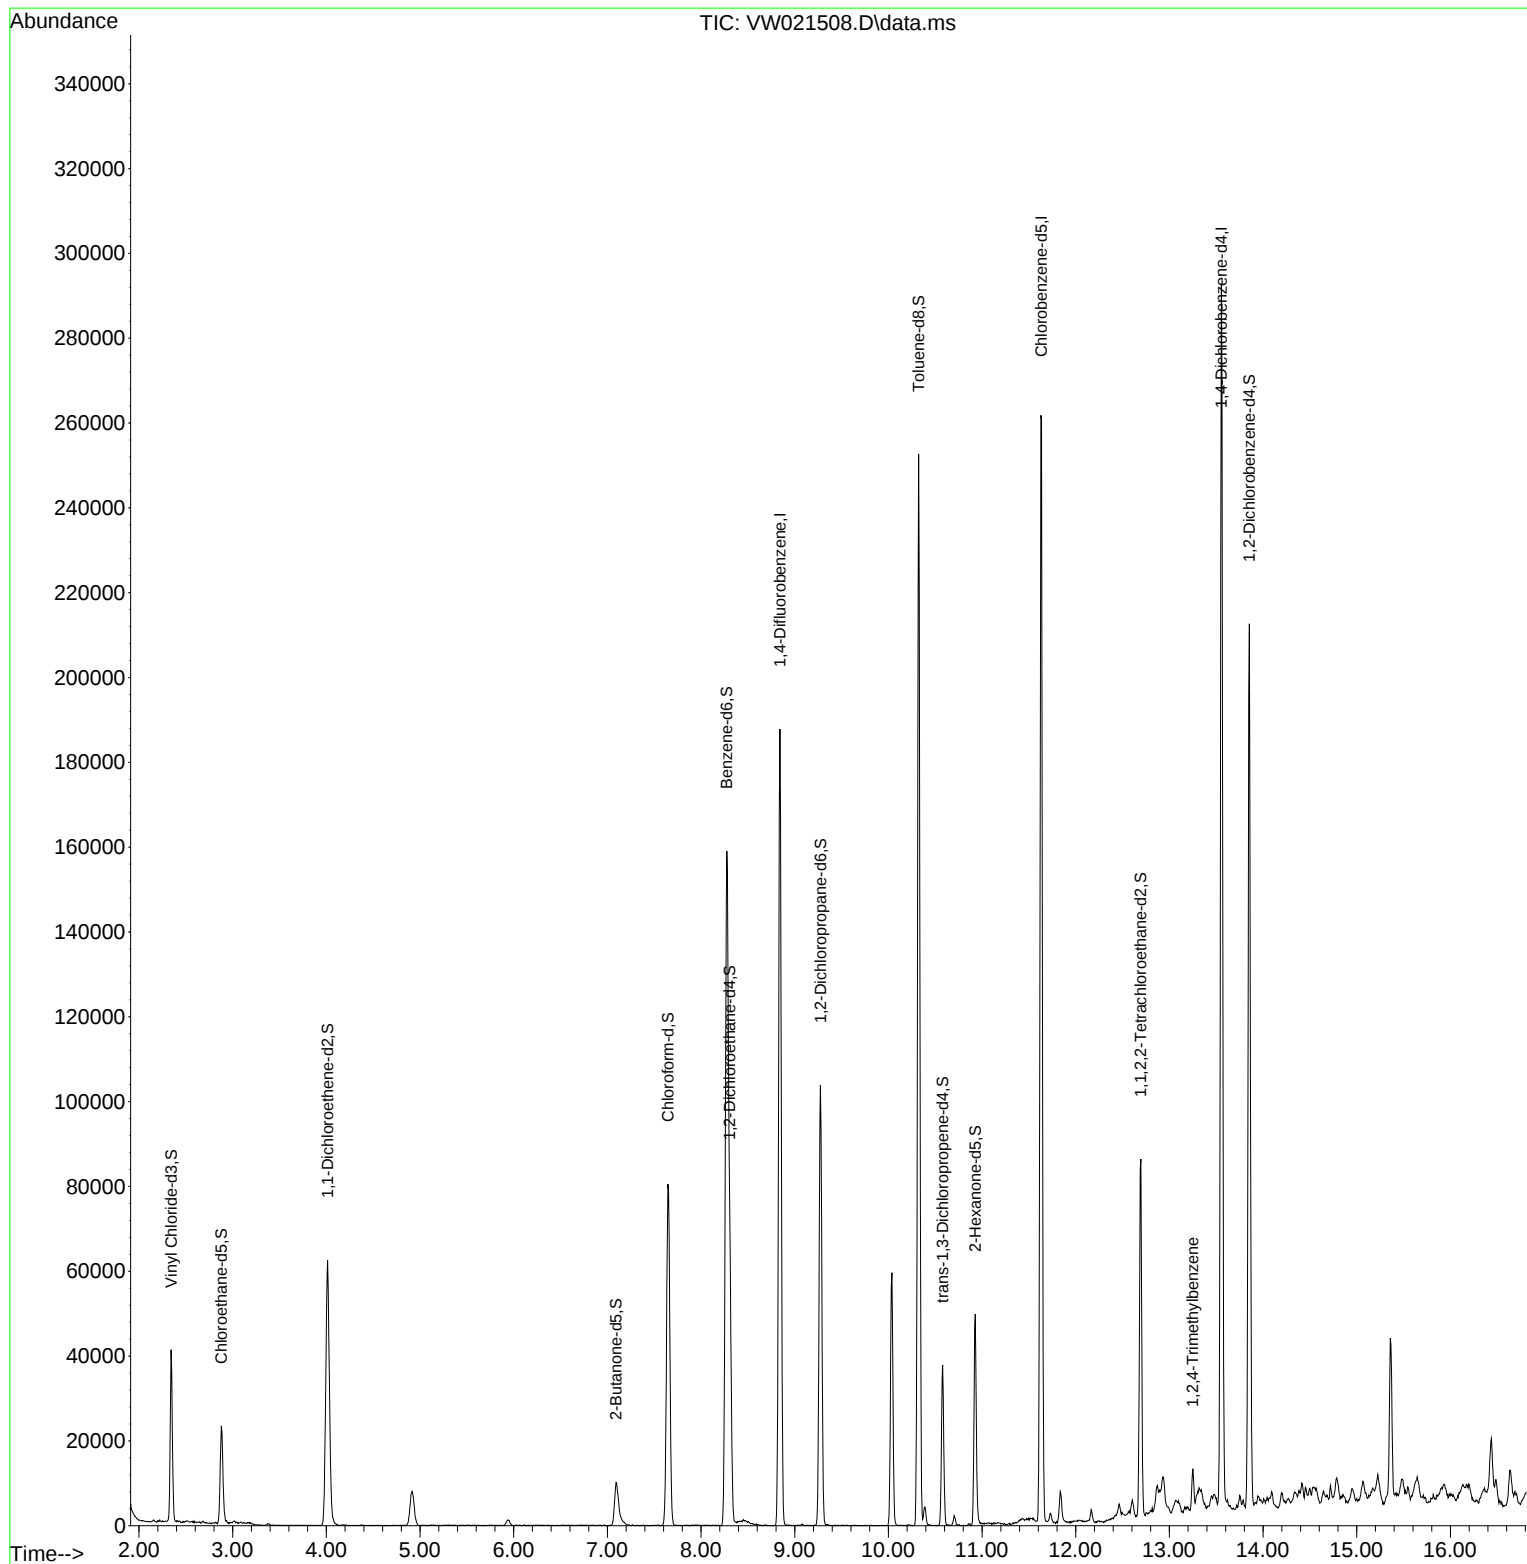

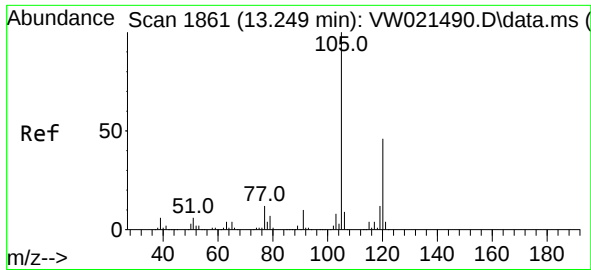

#63
 1,2,4-Trimethylbenzene
 Concen: 0.619 ug/L
 RT: 13.249 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VW021508.D
 Acq: 20 Dec 2021 19:16

Instrument :
 MSVOA_W
 ClientSampleId :
 H0AN4

Tgt Ion:105 Resp: 5711
 Ion Ratio Lower Upper
 105 100
 120 43.7 35.0 52.6

