


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw122120\
Data File : VW017682.D
Acq On : 21 Dec 2020 09:07
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W121420S.M
Title : Sw846 8260
Last Update : Mon Dec 14 12:39:23 2020

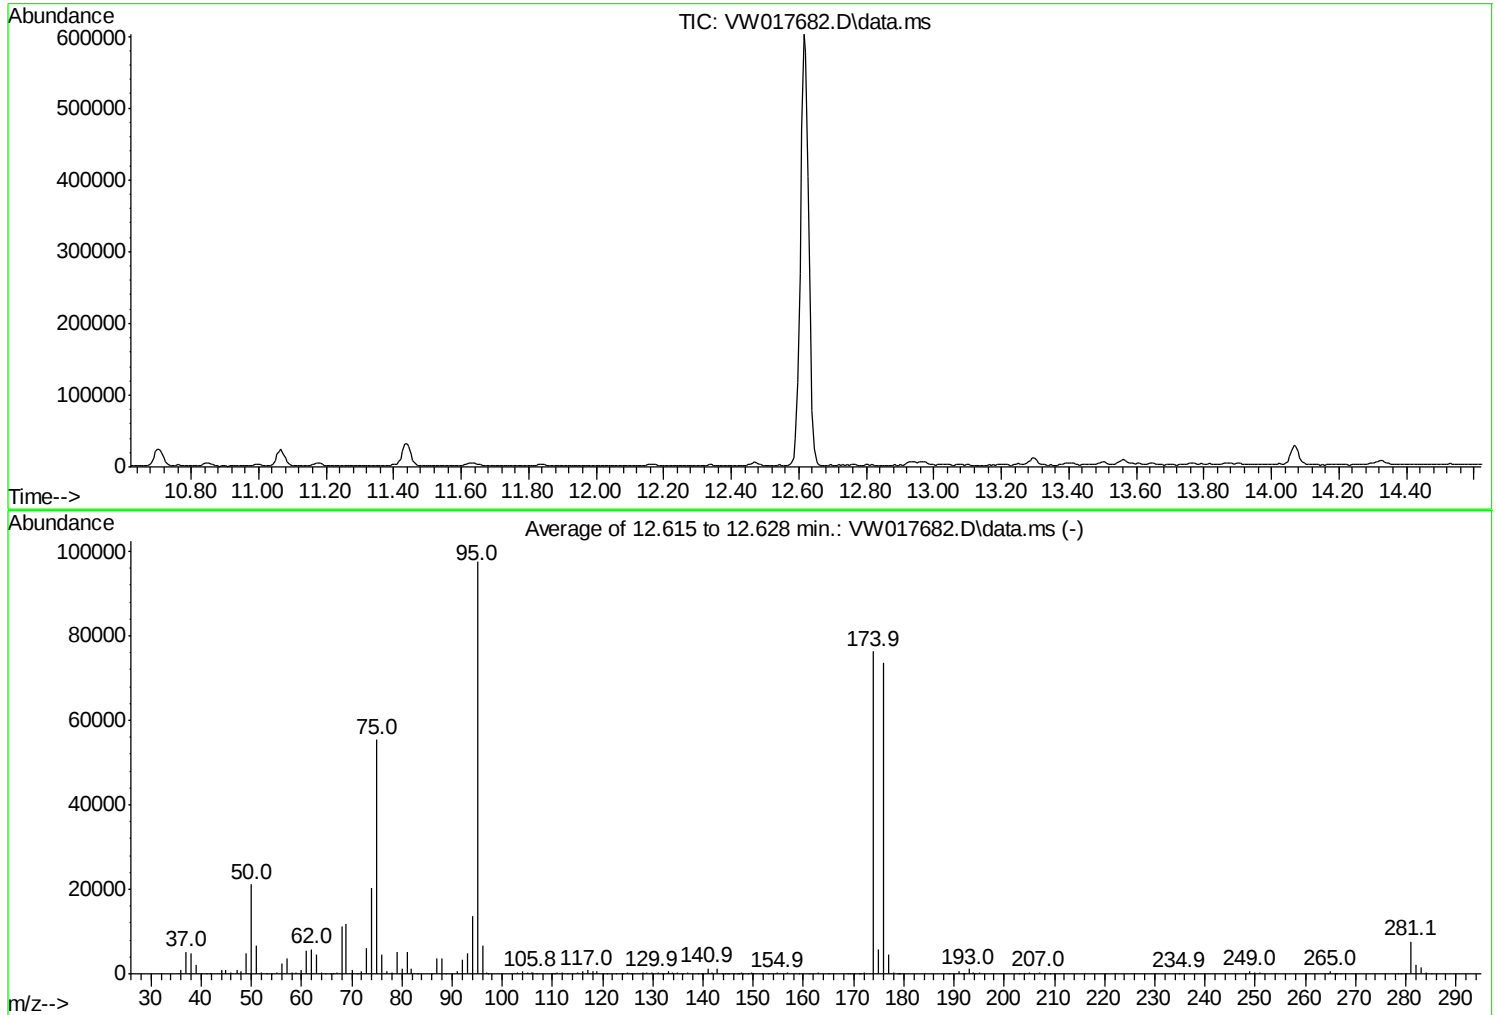

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1746

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.7	21181	PASS
75	95	30	60	56.8	55377	PASS
95	95	100	100	100.0	97568	PASS
96	95	5	9	7.0	6828	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.2	76296	PASS
175	174	5	9	7.7	5874	PASS
176	174	95	101	96.4	73533	PASS
177	176	5	9	6.3	4620	PASS