

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061722\
 Data File : VW023491.D
 Acq On : 17 Jun 2022 14:32
 Operator : SY/VA
 Sample : N3292-04
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 17 23:30:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 17 23:30:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	339291	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	322493	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	144610	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	111508	20.687	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.760%
7) Chloroethane-d5	2.885	69	78590	19.834	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.320%
11) 1,1-Dichloroethene-d2	4.019	63	106609	14.169	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.680%
21) 2-Butanone-d5	7.080	46	55655	50.570	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.140%
24) Chloroform-d	7.647	84	205564	22.009	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.040%
26) 1,2-Dichloroethane-d4	8.305	65	111927	22.251	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.000%
32) Benzene-d6	8.275	84	369560	21.612	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.440%
36) 1,2-Dichloropropane-d6	9.275	67	115676	22.962	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.840%
41) Toluene-d8	10.323	98	341534	20.449	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.800%
43) trans-1,3-Dichloroprop...	10.579	79	47643	20.720	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.880%
47) 2-Hexanone-d5	10.927	63	42045	52.230	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.460%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	108028	22.959	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.840%
66) 1,2-Dichlorobenzene-d4	13.853	152	128907	24.693	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.760%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4598	0.659	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061722\
Data File : VW023491.D
Acq On : 17 Jun 2022 14:32
Operator : SY/VA
Sample : N3292-04
Misc : 5.08g/10mL/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 17 23:30:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 17 23:30:09 2022
Response via : Initial Calibration

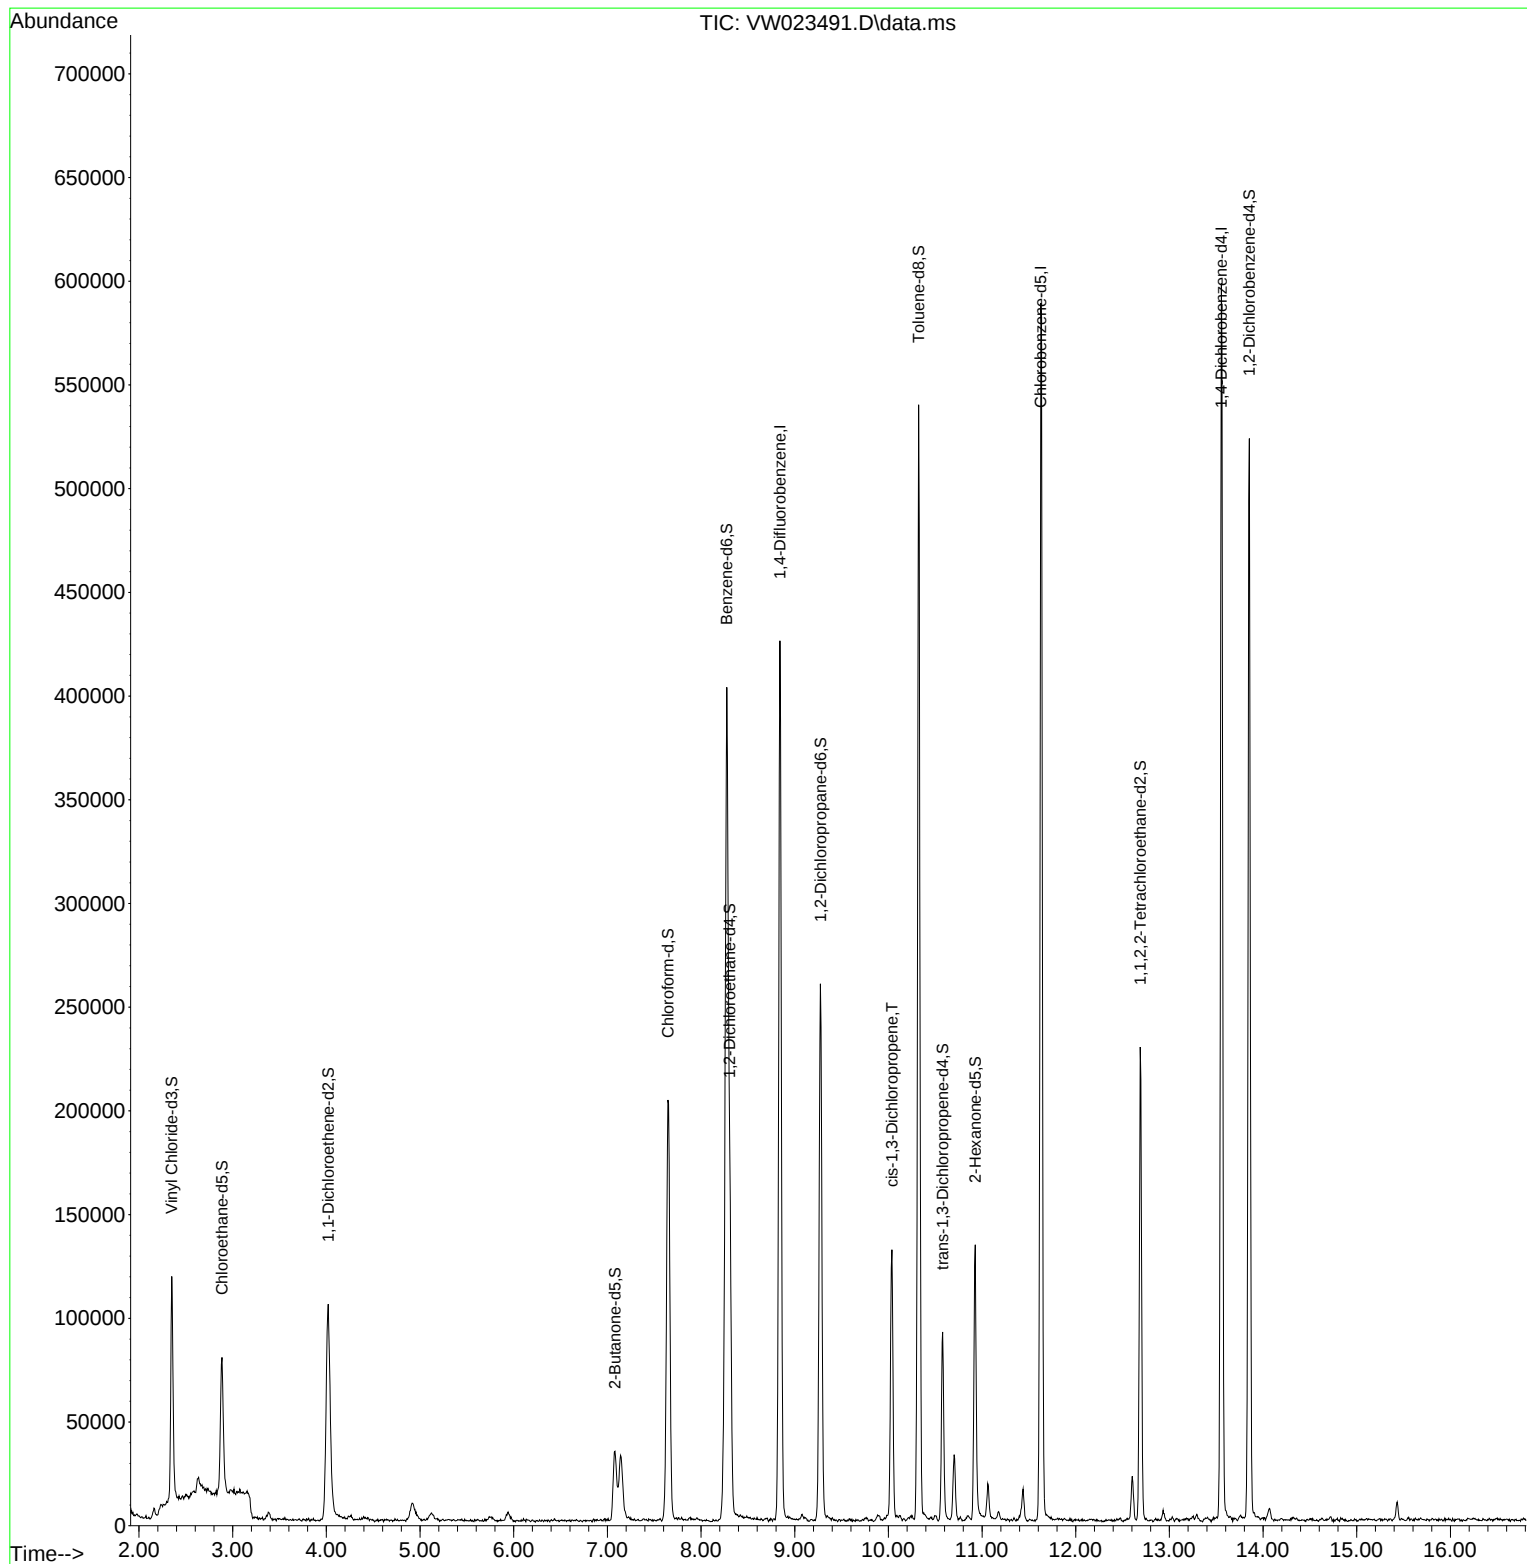

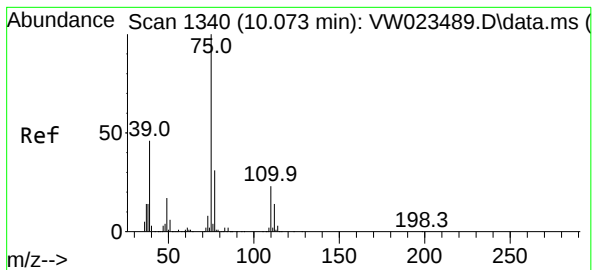

#39
 cis-1,3-Dichloropropene
 Concen: 0.659 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023491.D
 Acq: 17 Jun 2022 14:32

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 4598
 Ion Ratio Lower Upper
 75 100
 77 36.5 22.1 41.1

