


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW102718\
Data File : VW006375.D
Acq On : 25 Oct 2018 21:24
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
Title : SW846 8260
Last Update : Thu Oct 18 17:01:24 2018

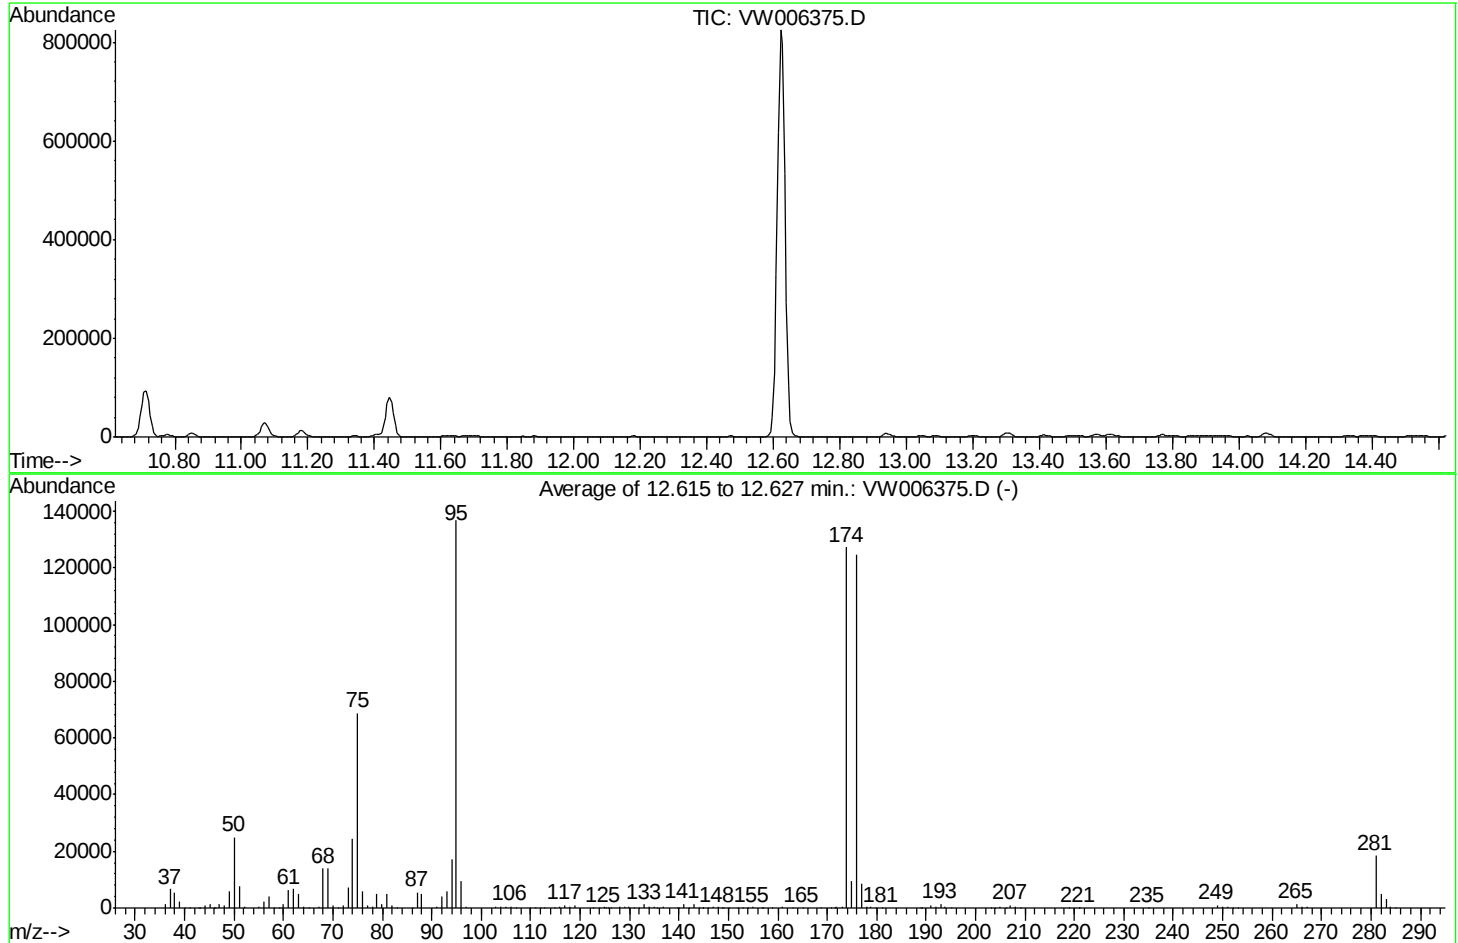

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	24997	PASS
75	95	30	60	50.3	68781	PASS
95	95	100	100	100.0	136800	PASS
96	95	5	9	6.9	9394	PASS
173	174	0.00	2	0.3	336	PASS
174	95	50	100	93.0	127210	PASS
175	174	5	9	7.4	9458	PASS
176	174	95	101	98.0	124720	PASS
177	176	5	9	6.8	8465	PASS