

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120121\
 Data File : VW020999.D
 Acq On : 01 Dec 2021 11:31
 Operator : SY/VA
 Sample : VIBLK496
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK496

Quant Time: Dec 02 01:57:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 02 01:54:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	107870	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	99807	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	55569	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	26087	20.849	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.400%
7) Chloroethane-d5	2.892	69	21172	26.236	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.960%
11) 1,1-Dichloroethene-d2	4.019	63	41010	16.940	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.760%
21) 2-Butanone-d5	7.080	46	14043	44.965	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.940%
24) Chloroform-d	7.653	84	63814	23.479	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.920%
26) 1,2-Dichloroethane-d4	8.311	65	34022	24.661	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.640%
32) Benzene-d6	8.275	84	125944	23.942	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.760%
36) 1,2-Dichloropropane-d6	9.275	67	35983	24.022	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.080%
41) Toluene-d8	10.323	98	126288	24.188	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.760%
43) trans-1,3-Dichloroprop...	10.579	79	14961	21.131	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.520%
47) 2-Hexanone-d5	10.921	63	11324	45.581	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.160%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	27015	23.543	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.160%
66) 1,2-Dichlorobenzene-d4	13.853	152	46390	23.423	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.680%
Target Compounds						
					Qvalue	
53) m,p-Xylene	11.835	106	2293	0.797	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120121\
Data File : VW020999.D
Acq On : 01 Dec 2021 11:31
Operator : SY/VA
Sample : VIBLK496
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK496

Quant Time: Dec 02 01:57:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 02 01:54:41 2021
Response via : Initial Calibration

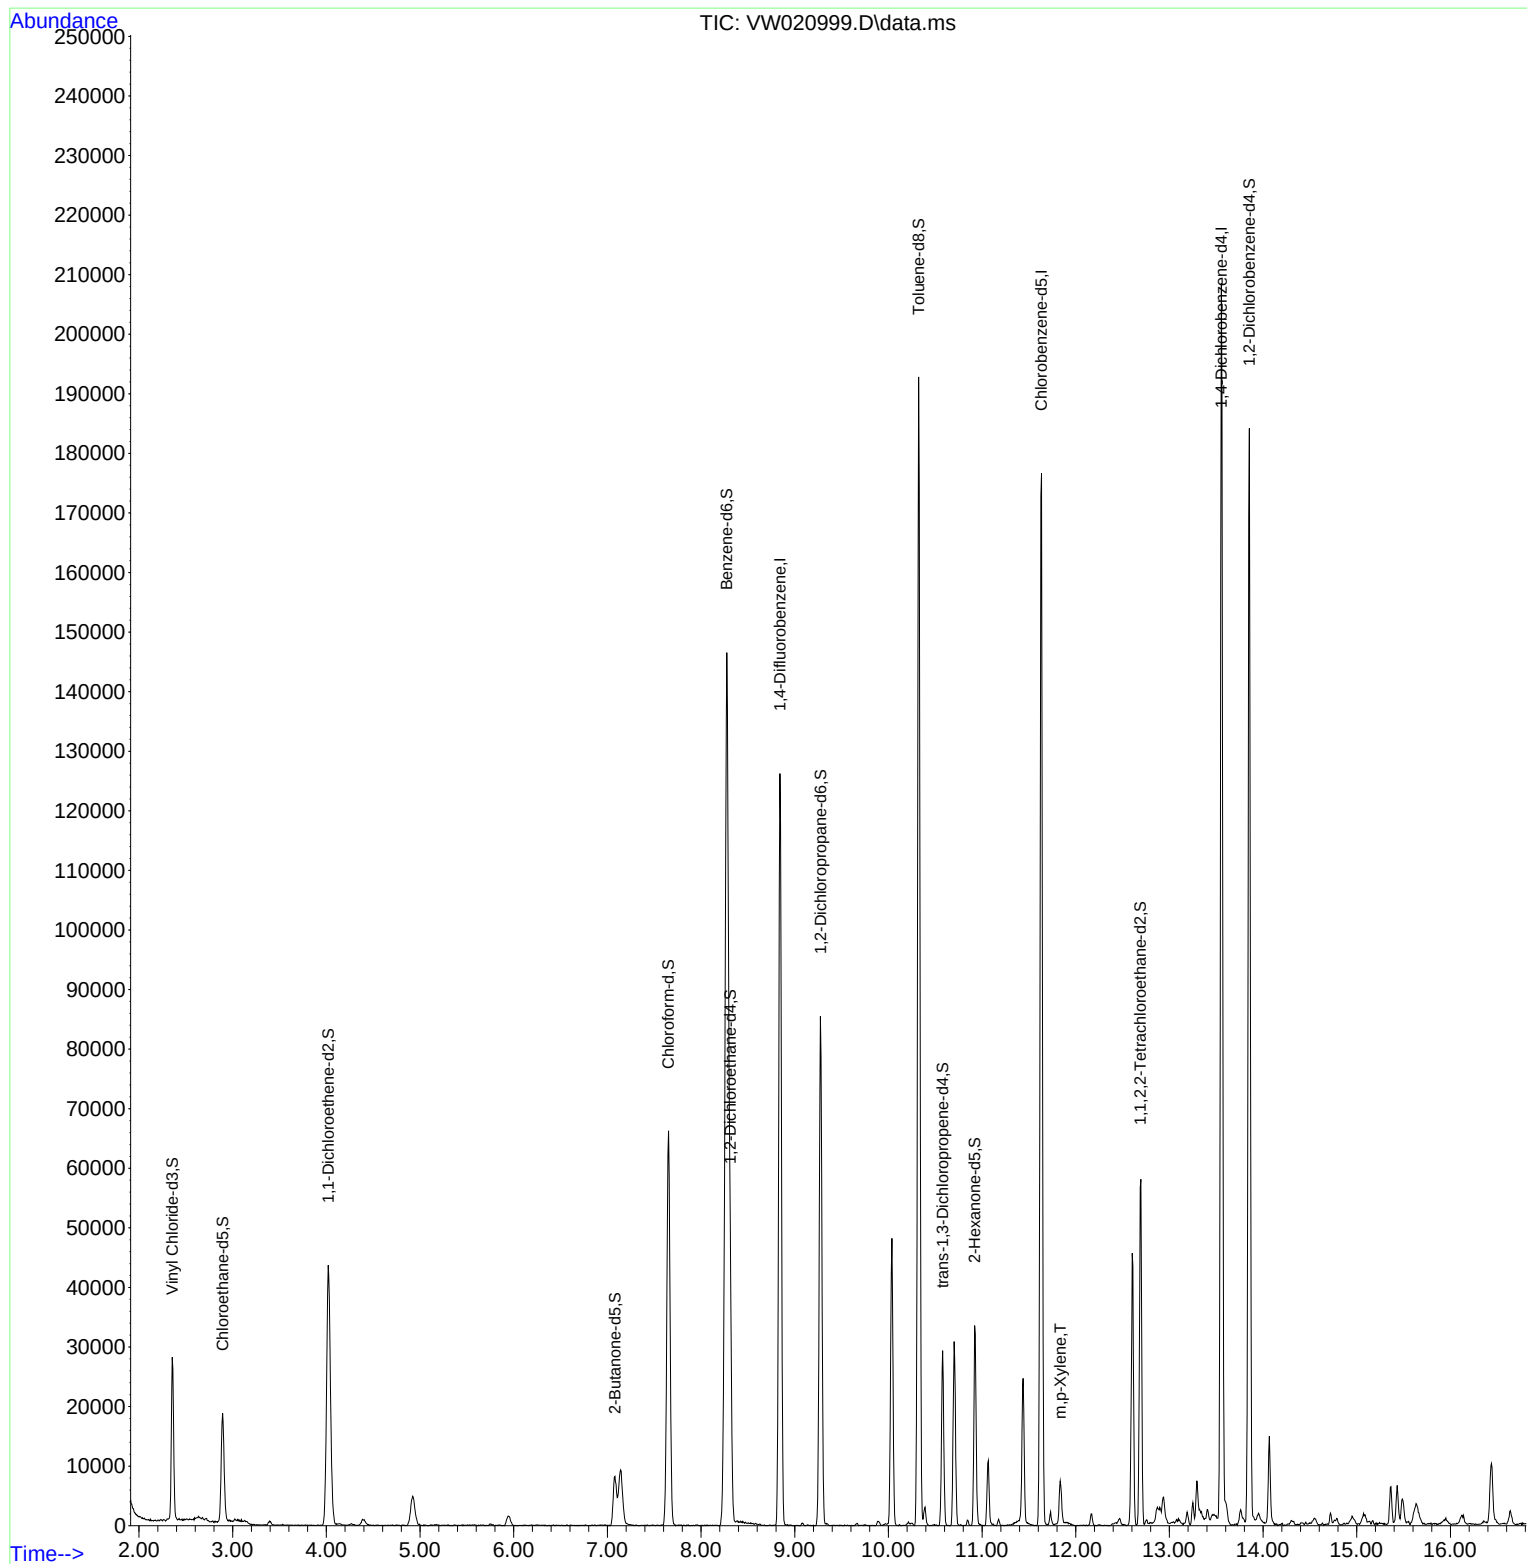

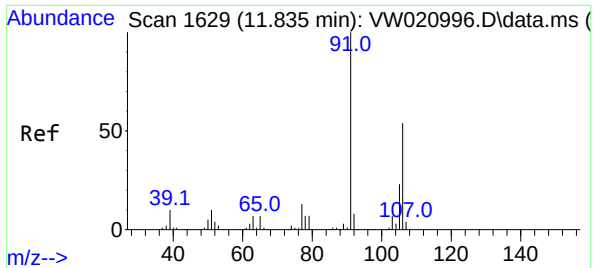

#53
 m,p-Xylene
 Concen: 0.797 ug/L
 RT: 11.835 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VW020999.D
 Acq: 01 Dec 2021 11:31

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK496

Tgt Ion:	106	Resp:	2293
Ion	Ratio	Lower	Upper
106	100		
91	201.7	149.9	278.3

