
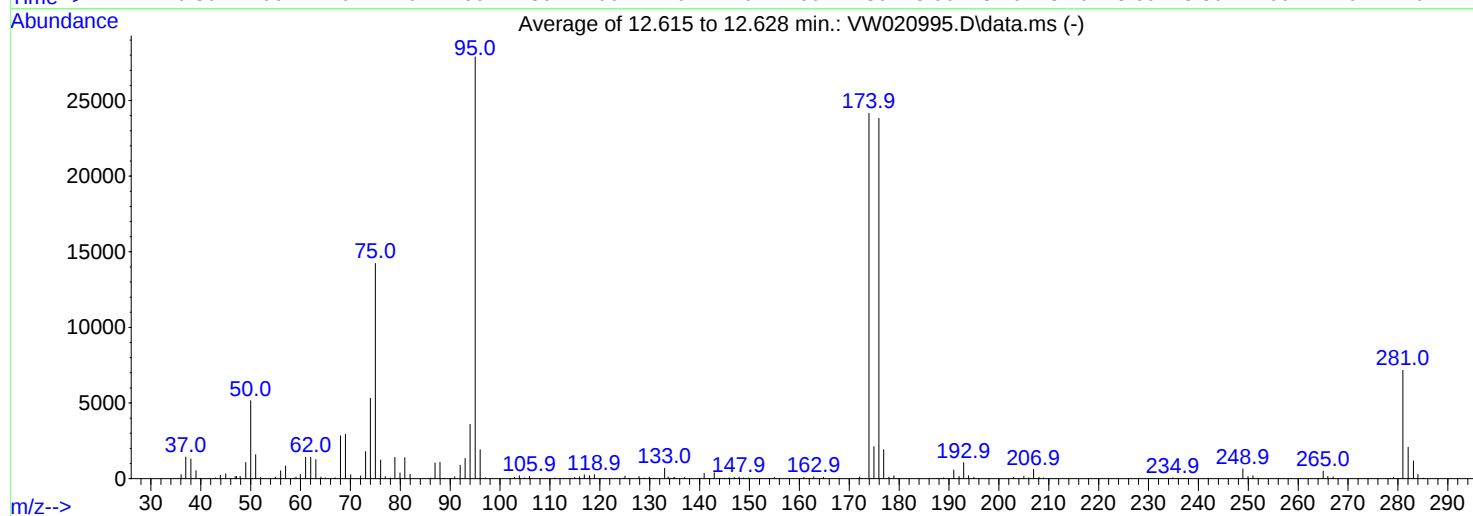


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120121\
 Data File : VW020995.D
 Acq On : 01 Dec 2021 07:18
 Operator : SY/VA
 Sample : BFB468
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB468

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Title : SFAM01.0
 Last Update : Fri Dec 03 01:25:28 2021

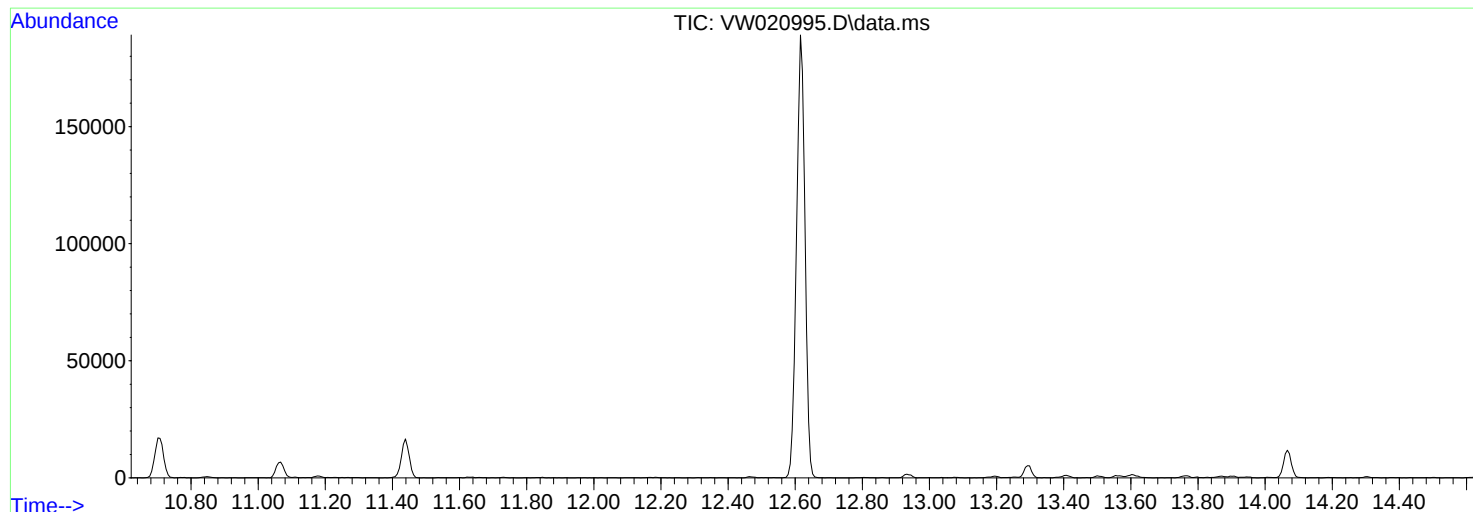

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	5153	PASS
75	95	30	80	51.0	14234	PASS
95	95	100	100	100.0	27888	PASS
96	95	5	9	6.9	1915	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.6	24152	PASS
175	174	5	9	8.8	2115	PASS
176	174	95	105	98.6	23819	PASS
177	176	5	10	8.1	1920	PASS

m/z	Abundance
36.00	197.0
37.00	1114.0
38.00	1043.0
39.00	397.0
39.90	52.0
44.00	292.0
45.00	268.0
47.10	209.0
47.90	110.0
49.00	716.0
50.00	3756.0
51.00	1191.0
55.00	97.0
55.90	383.0
57.00	660.0
59.90	231.0
61.00	1211.0
62.00	1156.0
63.10	981.0
64.20	82.0
66.90	82.0
68.00	2121.0
69.00	2202.0
70.10	223.0
72.00	152.0
73.10	1076.0
74.00	4074.0
75.00	11066.0
76.00	853.0
77.10	89.0
78.00	122.0
78.90	979.0
79.90	282.0
80.90	1026.0
82.00	227.0
86.10	53.0
86.90	876.0
87.90	827.0
90.90	86.0
92.00	717.0
93.00	1048.0
94.00	2897.0
95.00	22856.0
96.00	1618.0
103.80	149.0
105.80	100.0
115.00	64.0
115.80	108.0
116.80	163.0
118.00	100.0
118.80	163.0
124.80	110.0
127.80	84.0
128.80	62.0
129.80	83.0
133.00	225.0
133.90	63.0
135.00	57.0
136.90	59.0
140.90	292.0
142.90	355.0
147.90	96.0
154.90	58.0
160.80	58.0
171.80	65.0
174.00	20600.0
175.00	1716.0
175.90	21448.0
176.90	1688.0
178.00	53.0
179.10	89.0
190.90	158.0
192.10	74.0
192.80	310.0
194.00	97.0
205.10	60.0
207.10	195.0
208.00	61.0
248.90	176.0
250.00	73.0
251.10	86.0
264.90	230.0
265.90	85.0
279.20	59.0
281.00	2957.0
282.00	821.0
283.00	470.0
284.00	140.0

Instrument :
MSVOA_W
ClientSampleId :
BFB468

m/z	Abundance
43.90	70.0
57.10	52.0
281.00	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB468

m/z	Abundance
36.00	305.0
37.00	1687.0
38.00	1572.0
39.10	606.0
42.90	89.0
44.00	345.0
45.00	423.0
46.90	407.0
47.90	191.0
49.00	1303.0
50.00	6044.0
51.00	1945.0
52.00	90.0
54.90	104.0
56.00	635.0
57.00	1077.0
59.10	206.0
60.00	349.0
61.00	1576.0
62.10	1620.0
63.00	1369.0
64.00	150.0
65.00	93.0
66.80	65.0
68.00	3251.0
69.00	3248.0
70.00	331.0
72.10	192.0
73.10	2567.0
74.00	6040.0
75.00	15911.0
76.10	1505.0
76.90	190.0
78.90	1703.0
80.00	430.0
80.90	1614.0
81.90	323.0
86.10	73.0
87.00	1092.0
88.00	1277.0
88.80	106.0
90.90	137.0
92.00	893.0
93.00	1496.0
94.00	4108.0
95.00	29544.0
96.00	2177.0
97.00	86.0
102.90	182.0
103.90	200.0
104.90	88.0
105.90	180.0
110.90	113.0
112.00	54.0
114.90	88.0
115.90	125.0
116.90	294.0
117.90	299.0
118.90	340.0
125.00	368.0
125.80	67.0
127.90	169.0
129.00	71.0
130.00	95.0
130.90	87.0
133.00	1306.0
133.70	347.0
134.80	158.0
137.00	69.0
140.90	348.0
143.00	425.0
145.00	86.0
145.90	70.0
147.00	139.0
148.00	140.0
148.90	77.0
149.90	96.0
155.10	87.0
161.00	99.0
162.90	244.0
164.90	205.0
172.10	158.0
173.90	25640.0
175.00	2314.0
176.00	24368.0
176.90	2049.0
178.00	132.0
178.90	339.0
179.90	76.0
188.90	157.0
190.90	991.0
192.00	269.0

Instrument :
MSVOA_W
ClientSampleId :
BFB468

192.90	1908.0
193.90	335.0
195.00	168.0
195.90	56.0
203.00	124.0
205.00	283.0
206.00	81.0
206.90	962.0
208.10	159.0
209.00	106.0
234.90	149.0
248.90	1215.0
250.00	156.0
251.00	303.0
251.90	60.0
265.00	858.0
265.90	255.0
267.00	223.0
279.10	120.0
281.00	11487.0
282.00	3837.0
283.10	1898.0
284.00	508.0
285.20	102.0

Instrument :
MSVOA_W
ClientSampleId :
BFB468

m/z	Abundance
36.10	283.0
37.00	1490.0
38.00	1292.0
39.00	577.0
39.80	58.0
43.00	59.0
43.90	270.0
45.00	293.0
47.20	228.0
47.90	173.0
49.00	1175.0
50.00	5659.0
51.00	1639.0
52.00	95.0
55.00	123.0
56.00	545.0
57.00	934.0
58.80	98.0
59.10	89.0
59.90	287.0
61.00	1461.0
62.00	1492.0
63.00	1422.0
64.10	93.0
64.90	81.0
67.00	92.0
68.00	3125.0
69.00	3332.0
70.10	255.0
72.10	180.0
73.00	1735.0
74.00	5824.0
75.00	15724.0
76.00	1326.0
77.00	133.0
78.90	1533.0
79.90	419.0
80.90	1507.0
82.00	317.0
87.00	1135.0
88.00	1142.0
90.90	156.0
92.00	1054.0
93.00	1449.0
94.00	3762.0
95.00	31264.0
96.00	1950.0
97.10	65.0
102.90	116.0
103.90	227.0
104.90	66.0
105.90	178.0
111.10	78.0
112.80	58.0
114.90	78.0
116.00	122.0
116.90	290.0
117.90	181.0
119.00	305.0
125.10	142.0
127.80	156.0
129.90	131.0
133.00	544.0
135.00	153.0
136.90	89.0
140.90	441.0
142.90	404.0
145.90	75.0
146.90	113.0
147.80	91.0
148.80	76.0
149.90	59.0
155.00	107.0
160.80	92.0
162.90	103.0
164.80	90.0
172.10	166.0
173.90	26216.0
174.90	2315.0
175.90	25640.0
176.90	2022.0
177.90	131.0
179.00	150.0
189.10	62.0
191.00	555.0
192.00	147.0
193.00	956.0
193.90	157.0
195.00	112.0
202.90	89.0
205.00	136.0
206.00	69.0

Instrument :
MSVOA_W
ClientSampleId :
BFB468

207.00	644.0
208.00	71.0
208.90	54.0
248.90	560.0
249.90	201.0
250.90	170.0
252.00	52.0
265.00	410.0
266.00	115.0
267.00	140.0
278.50	71.0
279.10	103.0
281.00	7216.0
282.10	1575.0
283.10	1162.0
284.00	184.0
284.90	58.0

Instrument :
MSVOA_W
ClientSampleId :
BFB468