

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
 Data File : VW021788.D
 Acq On : 07 Jan 2022 21:06
 Operator : SY/VA
 Sample : N1025-12
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Jan 07 23:04:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 22:46:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	139408	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	138272	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	80088	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	56417	20.525	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.120%		
7) Chloroethane-d5	2.885	69	40576	21.918	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.680%		
11) 1,1-Dichloroethene-d2	4.025	63	73241	18.208	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	72.840%		
21) 2-Butanone-d5	7.226	46	129	0.321	ug/L	0.14
Spiked Amount 50.000	Range 20 - 135		Recovery =	0.640%#		
24) Chloroform-d	7.653	84	110394	25.350	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	101.400%		
26) 1,2-Dichloroethane-d4	8.311	65	57898	25.179	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	100.720%		
32) Benzene-d6	8.275	84	224100	27.295	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	109.200%		
36) 1,2-Dichloropropane-d6	9.275	67	60018	26.947	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	107.800%		
41) Toluene-d8	10.323	98	218249	26.680	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	106.720%		
43) trans-1,3-Dichloroprop...	10.579	79	23995	22.140	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.560%		
47) 2-Hexanone-d5	10.927	63	20020	59.269	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	118.540%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	52575	28.632	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	114.520%		
66) 1,2-Dichlorobenzene-d4	13.853	152	88145	28.781	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	115.120%		
Target Compounds						Qvalue
34) Trichloroethene	8.848	95	3741	1.562	ug/L #	5
39) cis-1,3-Dichloropropene	10.037	75	2099	0.687	ug/L #	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
Data File : VW021788.D
Acq On : 07 Jan 2022 21:06
Operator : SY/VA
Sample : N1025-12
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Jan 07 23:04:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 07 22:46:04 2022
Response via : Initial Calibration




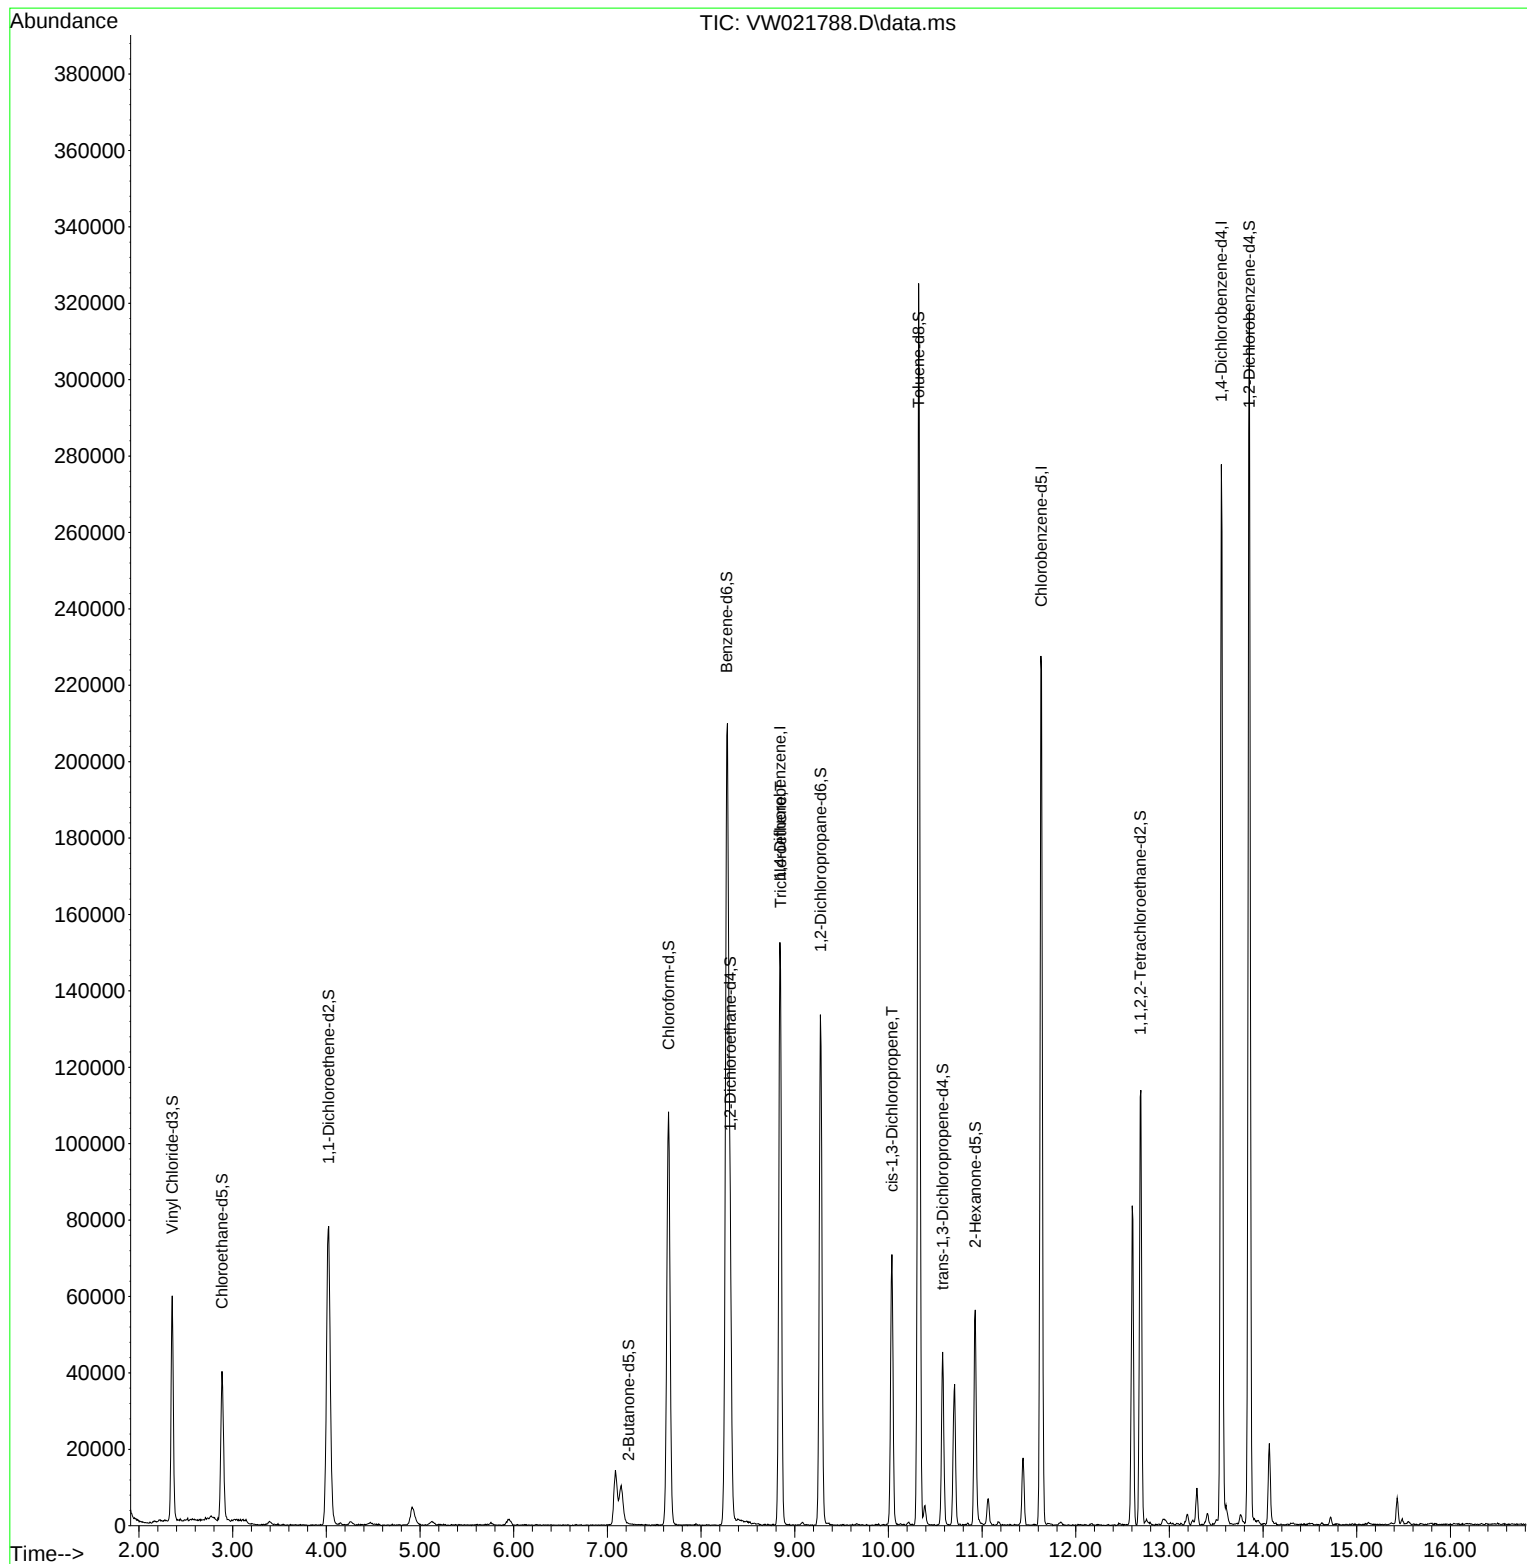


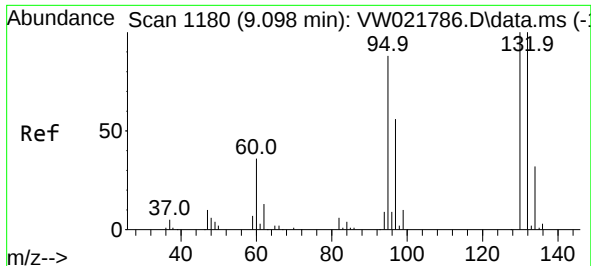

#34
 Trichloroethene
 Concen: 1.562 ug/L
 RT: 8.848 min Scan# 1139
 Delta R.T. -0.250 min
 Lab File: VW021788.D
 Acq: 07 Jan 2022 21:06

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Tgt Ion:	95	Resp:	3741
Ion	Ratio	Lower	Upper
95	100		
97	0.0	47.0	87.2#
132	0.0	65.5	121.6#
130	0.0	69.4	128.8#

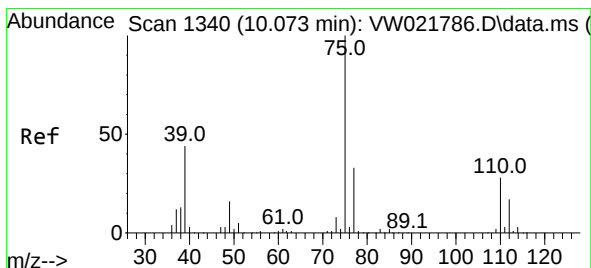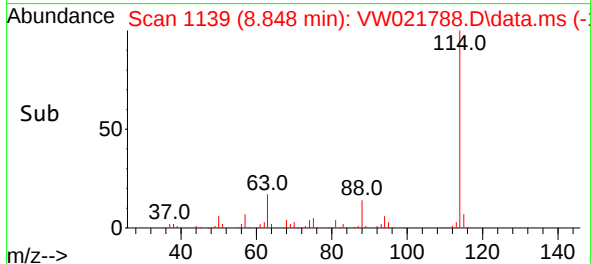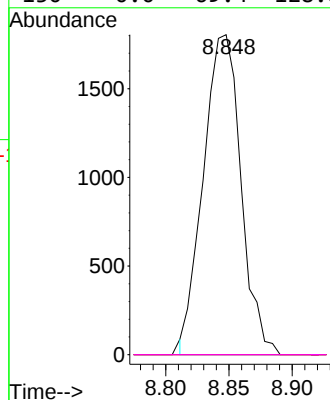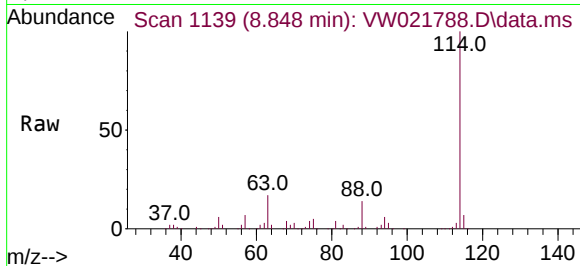

#39
 cis-1,3-Dichloropropene
 Concen: 0.687 ug/L
 RT: 10.037 min Scan# 1334
 Delta R.T. -0.037 min
 Lab File: VW021788.D
 Acq: 07 Jan 2022 21:06

Tgt Ion:	75	Resp:	2099
Ion	Ratio	Lower	Upper
75	100		
77	53.8	21.8	40.6#

