




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
 Data File : VW021776.D
 Acq On : 07 Jan 2022 15:30
 Operator : SY/VA
 Sample : N1053-15
 Misc : 7.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLJ2

Manual IntegrationsAPPROVED

Quant Time: Jan 07 22:02:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 21:59:54 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

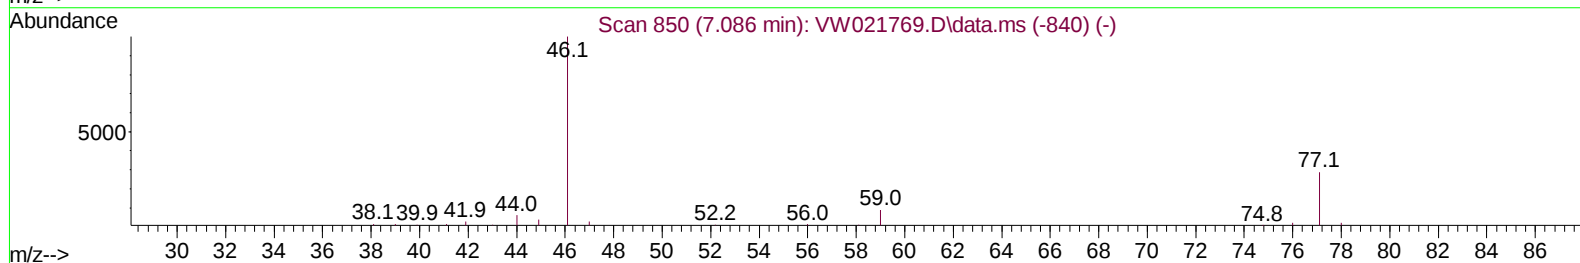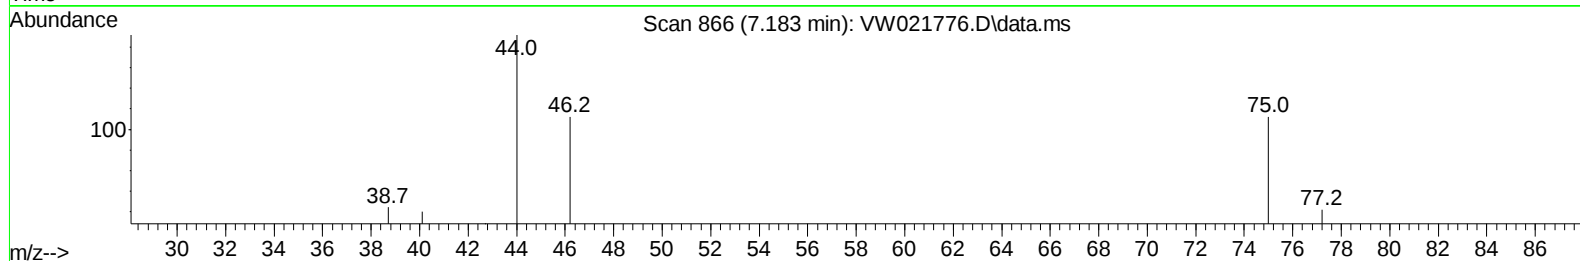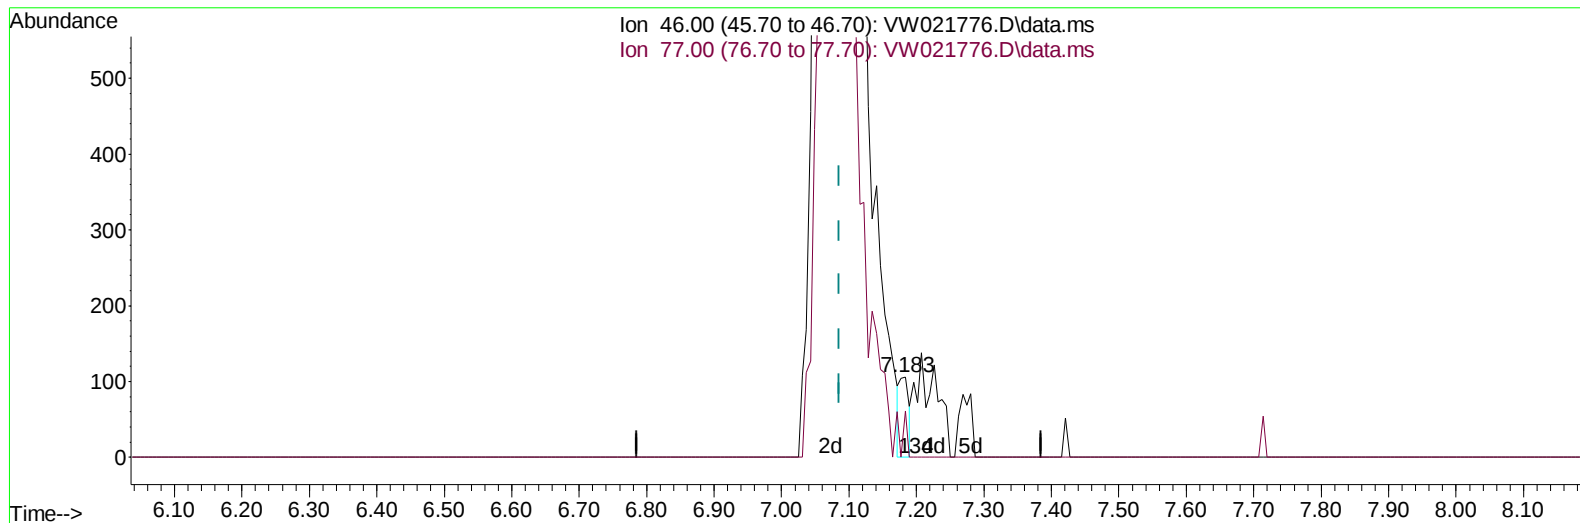

TIC: VW021776.D\data.ms

(21) 2-Butanone-d5 (S)

7.183min (+ 0.098) 0.28 ug/L

response 101

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	21.78
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
 Data File : VW021776.D
 Acq On : 07 Jan 2022 15:30
 Operator : SY/VA
 Sample : N1053-15
 Misc : 7.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLJ2

Manual IntegrationsAPPROVED

Quant Time: Jan 07 22:02:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 21:59:54 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

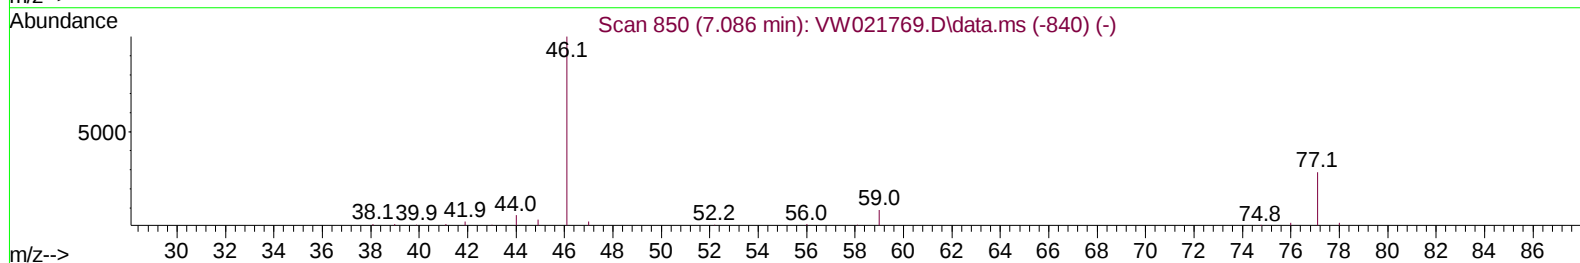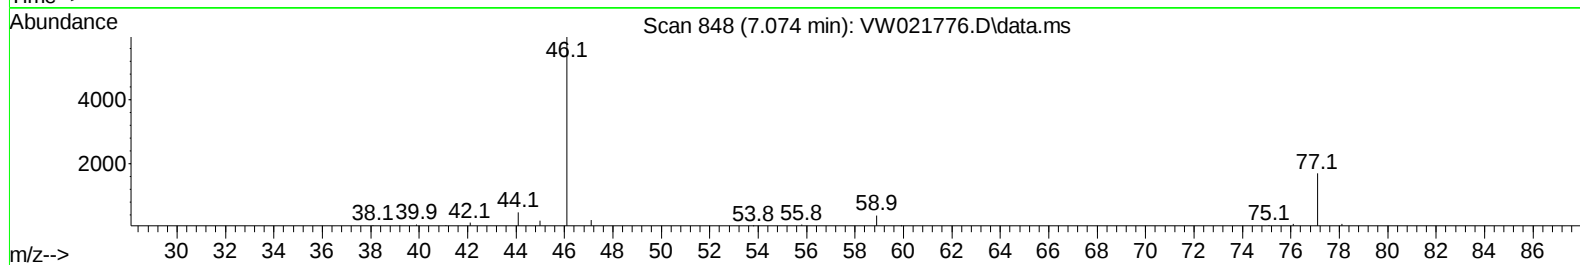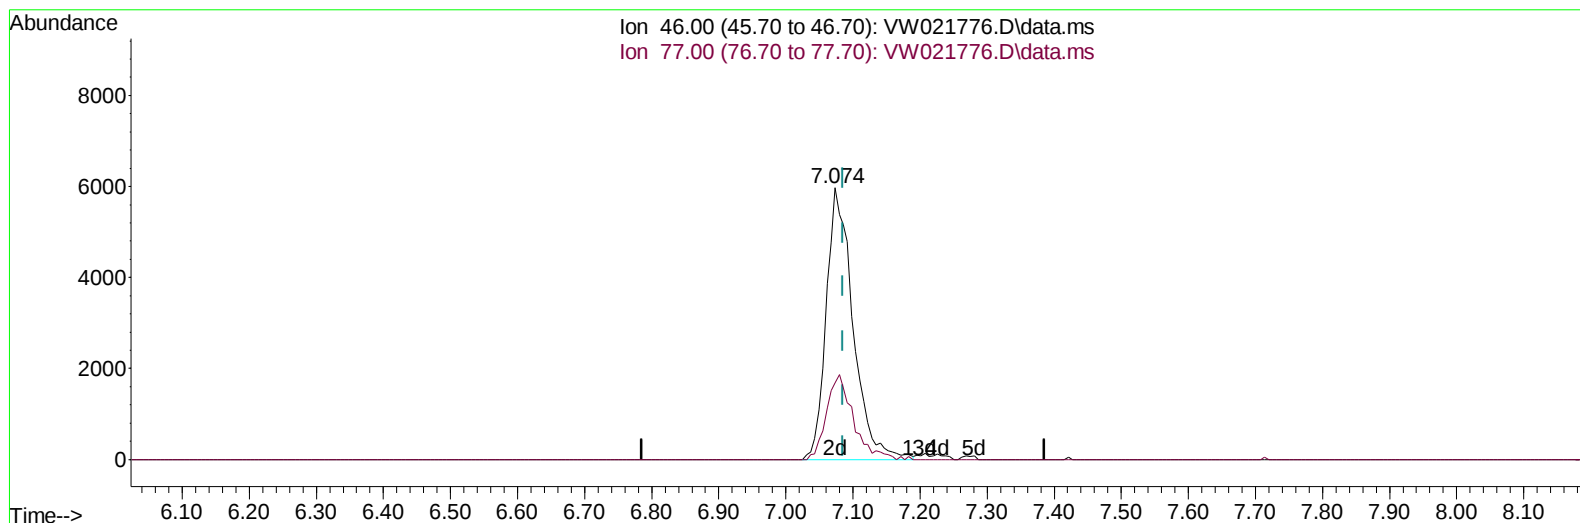

TIC: VW021776.D\data.ms

(21) 2-Butanone-d5 (S)

7.074min (-0.012) 45.35 ug/L m

response 16581

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	0.13#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
 Data File : VW021776.D
 Acq On : 07 Jan 2022 15:30
 Operator : SY/VA
 Sample : N1053-15
 Misc : 7.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLJ2

Manual IntegrationsAPPROVED

Quant Time: Jan 07 22:02:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 21:59:54 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.841	114		126757	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117		125208	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		75088	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		33530	13.416	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	53.680%		
7) Chloroethane-d5	2.885	69		24000	14.258	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	57.040%		
11) 1,1-Dichloroethene-d2	4.019	63		49571	13.554	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	54.200%		
21) 2-Butanone-d5	7.074	46		16581m	45.348	ug/L	-0.01
Spiked Amount 50.000	Range 20	- 135		Recovery =	90.700%		
24) Chloroform-d	7.653	84		76551	19.333	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	77.320%		
26) 1,2-Dichloroethane-d4	8.311	65		41297	19.752	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	79.000%		
32) Benzene-d6	8.275	84		153872	20.697	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	82.800%		
36) 1,2-Dichloropropane-d6	9.274	67		42961	21.301	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	85.200%		
41) Toluene-d8	10.323	98		153545	20.729	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	82.920%		
43) trans-1,3-Dichloroprop...	10.579	79		17603	17.937	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	71.760%		
47) 2-Hexanone-d5	10.920	63		14194	46.405	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	92.820%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		35516	21.360	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	85.440%		
66) 1,2-Dichlorobenzene-d4	13.853	152		63362	22.066	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	88.280%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
Data File : VW021776.D
Acq On : 07 Jan 2022 15:30
Operator : SY/VA
Sample : N1053-15
Misc : 7.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLJ2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/10/2022
Supervised By :Mahesh Dadoda 01/10/2022

Quant Time: Jan 07 22:02:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 07 21:59:54 2022
Response via : Initial Calibration

