




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
 Data File : VW021779.D
 Acq On : 07 Jan 2022 16:42
 Operator : SY/VA
 Sample : N1053-21
 Misc : 6.75g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLJ8

Manual IntegrationsAPPROVED

Quant Time: Jan 07 22:02:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 21:59:54 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

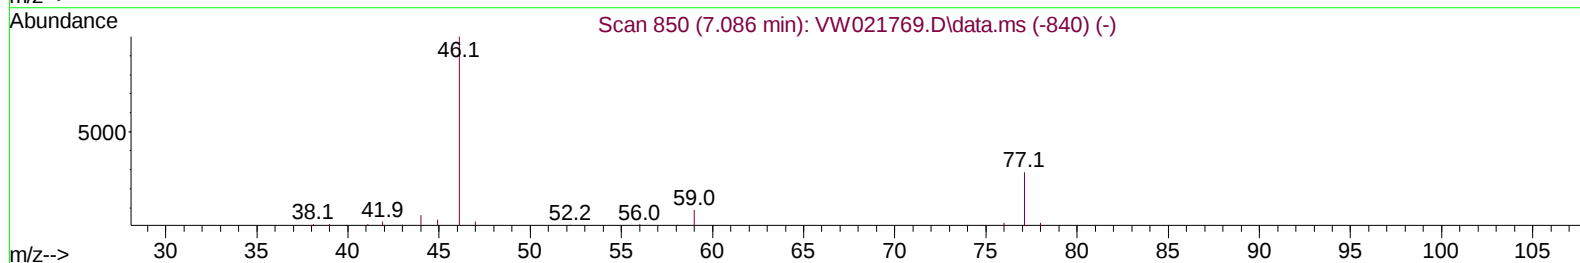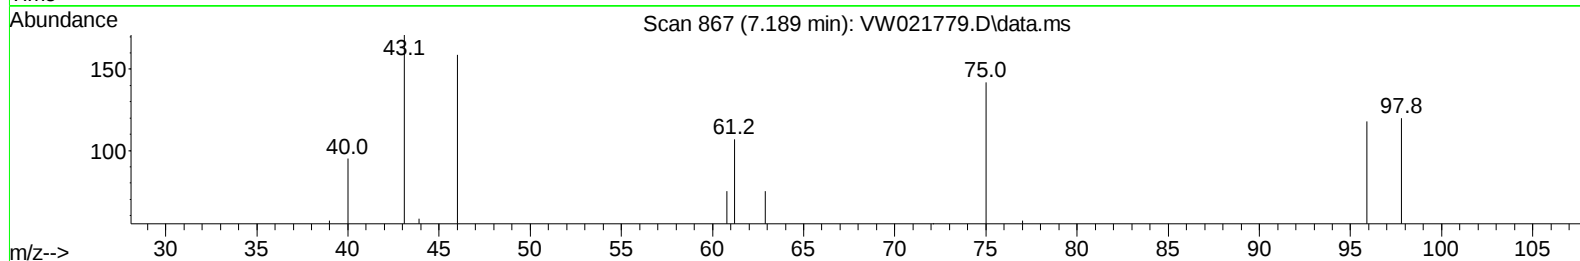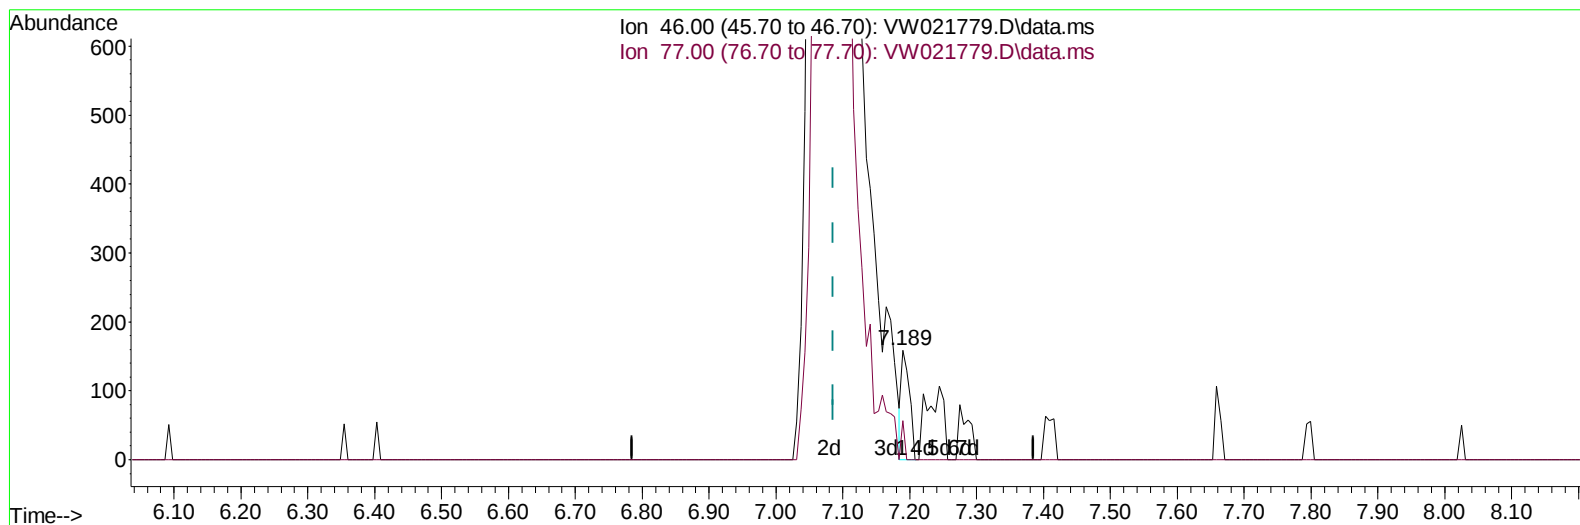

TIC: VW021779.D\data.ms

(21) 2-Butanone-d5 (S)

7.189min (+ 0.104) 0.23 ug/L

response 135

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	15.56
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
Data File : VW021779.D
Acq On : 07 Jan 2022 16:42
Operator : SY/VA
Sample : N1053-21
Misc : 6.75g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLJ8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/10/2022
Supervised By :Mahesh Dadoda 01/10/2022

Quant Time: Jan 07 22:02:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 07 21:59:54 2022
Response via : Initial Calibration

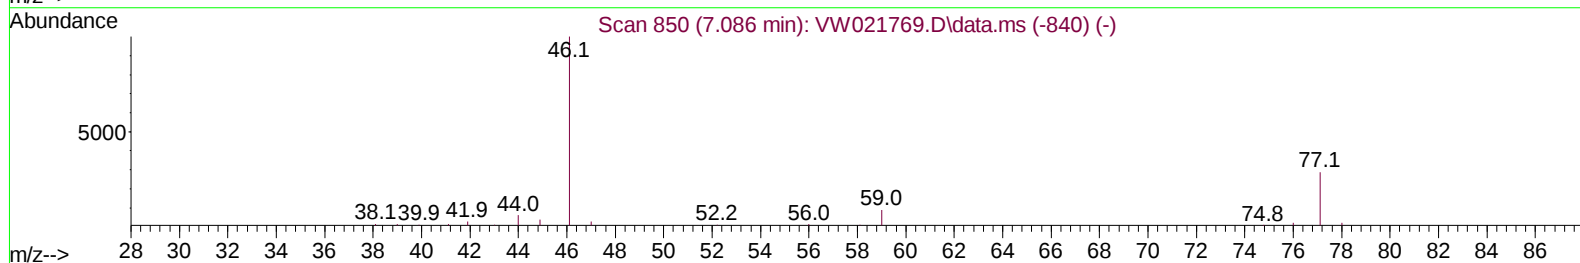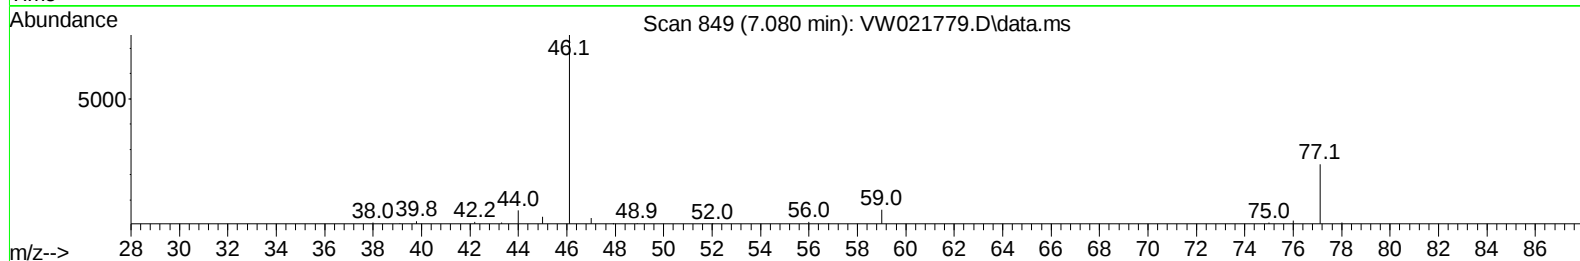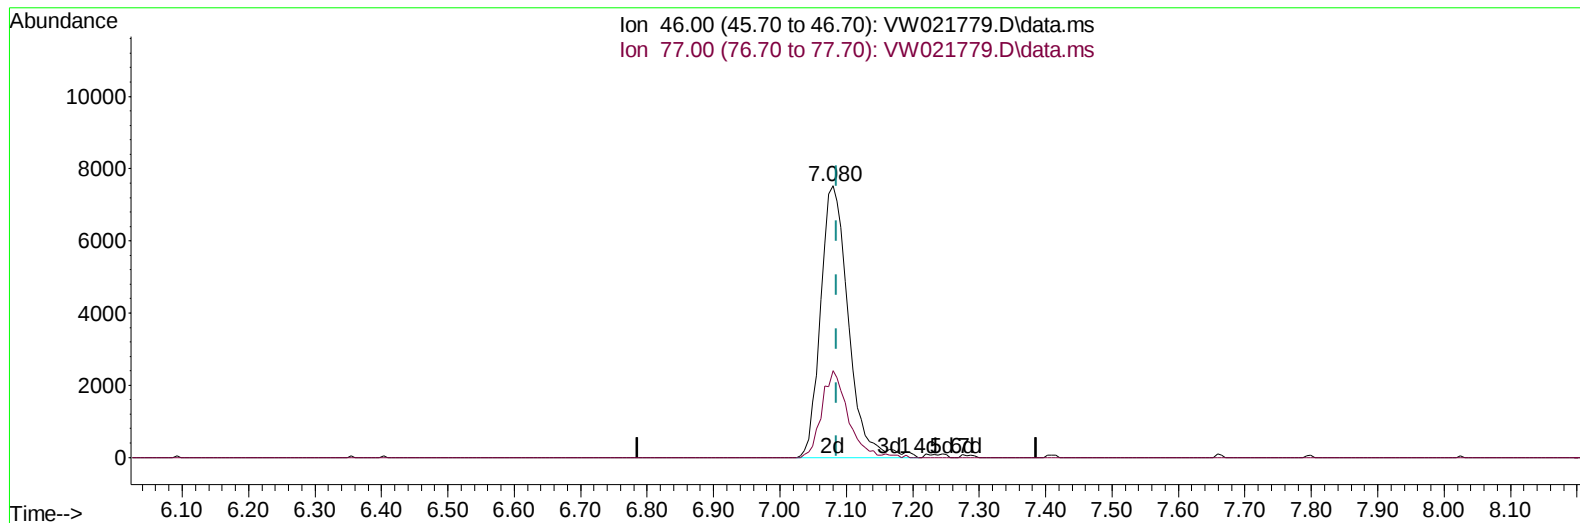

TIC: VW021779.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (-0.006) 37.85 ug/L m

response 21825

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	0.10#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
 Data File : VW021779.D
 Acq On : 07 Jan 2022 16:42
 Operator : SY/VA
 Sample : N1053-21
 Misc : 6.75g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLJ8

Manual IntegrationsAPPROVED

Quant Time: Jan 07 22:02:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 21:59:54 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	199905	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	192231	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	109155	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	55471	14.074	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	56.280%	
7) Chloroethane-d5	2.885	69	40168	15.131	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	60.520%	
11) 1,1-Dichloroethene-d2	4.013	63	75014	13.005	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	52.040%	
21) 2-Butanone-d5	7.080	46	21825m	37.848	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	75.700%	
24) Chloroform-d	7.647	84	117256	18.777	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	75.120%	
26) 1,2-Dichloroethane-d4	8.305	65	59678	18.099	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	72.400%	
32) Benzene-d6	8.275	84	237681	20.823	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	83.280%	
36) 1,2-Dichloropropane-d6	9.274	67	63618	20.546	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	82.200%	
41) Toluene-d8	10.323	98	242943	21.362	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	85.440%	
43) trans-1,3-Dichloroprop...	10.579	79	25367	16.836	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	67.360%	
47) 2-Hexanone-d5	10.921	63	19620	41.780	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	83.560%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	49506	19.393	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	77.560%	
66) 1,2-Dichlorobenzene-d4	13.853	152	93112	22.307	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	89.240%	
Target Compounds						
13) Acetone	4.135	43	1490	3.043	ug/L	Qvalue 58

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
Data File : VW021779.D
Acq On : 07 Jan 2022 16:42
Operator : SY/VA
Sample : N1053-21
Misc : 6.75g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLJ8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/10/2022
Supervised By :Mahesh Dadoda 01/10/2022

Quant Time: Jan 07 22:02:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 07 21:59:54 2022
Response via : Initial Calibration

