




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
 Data File : VW021787.D
 Acq On : 07 Jan 2022 20:42
 Operator : SY/VA
 Sample : VW0107SBL02
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK438

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

Quant Time: Jan 07 22:46:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 22:46:04 2022
 Response via : Initial Calibration

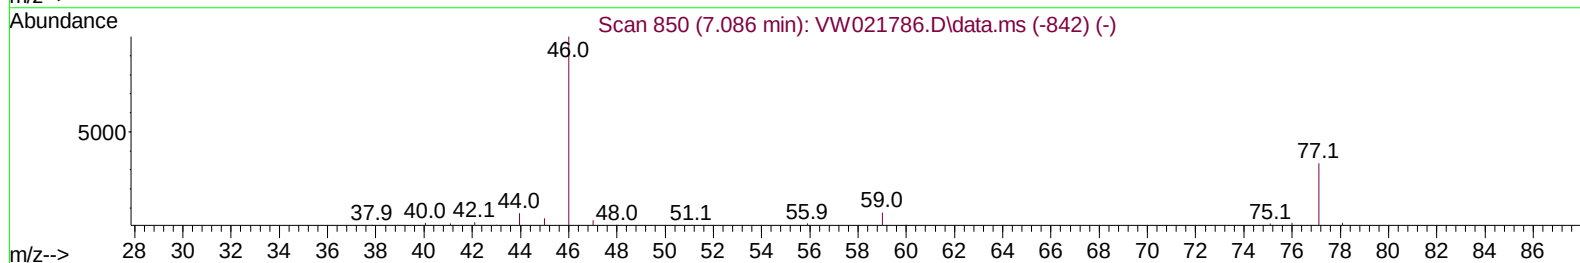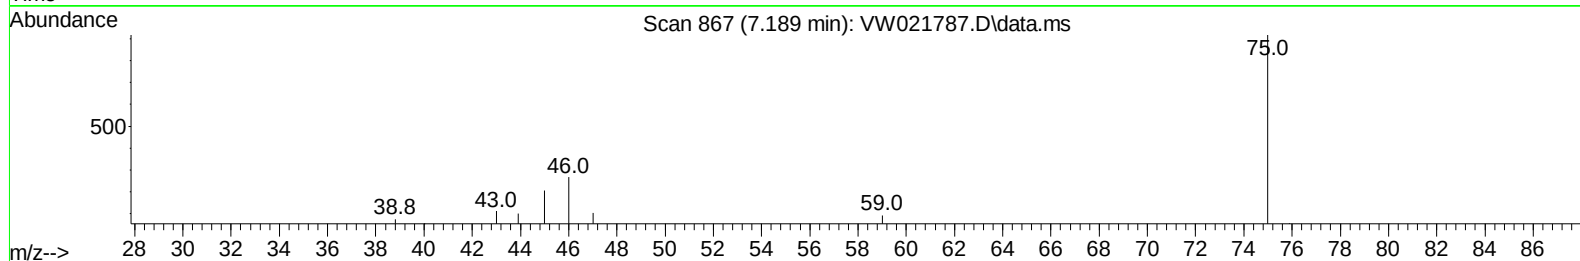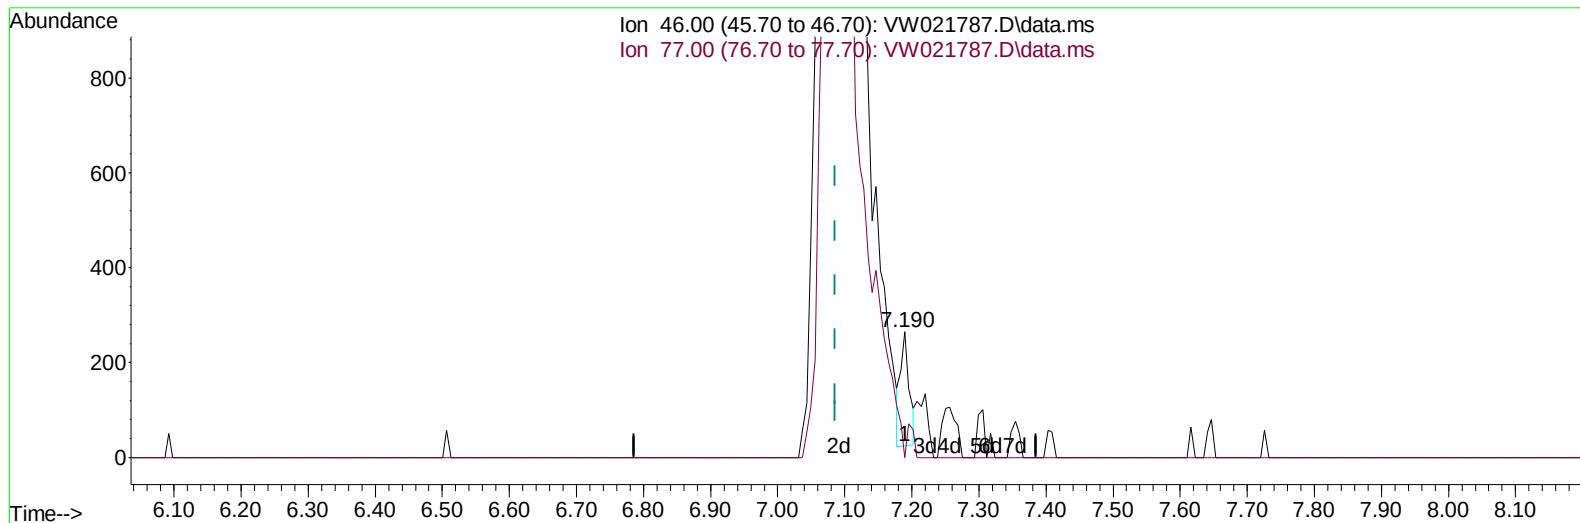

TIC: VW021787.D\data.ms

(21) 2-Butanone-d5 (S)

7.189min (+ 0.104) 0.54 ug/L

response 220

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	21.82
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
 Data File : VW021787.D
 Acq On : 07 Jan 2022 20:42
 Operator : SY/VA
 Sample : VW0107SBL02
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK438

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

Quant Time: Jan 07 22:46:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 22:46:04 2022
 Response via : Initial Calibration

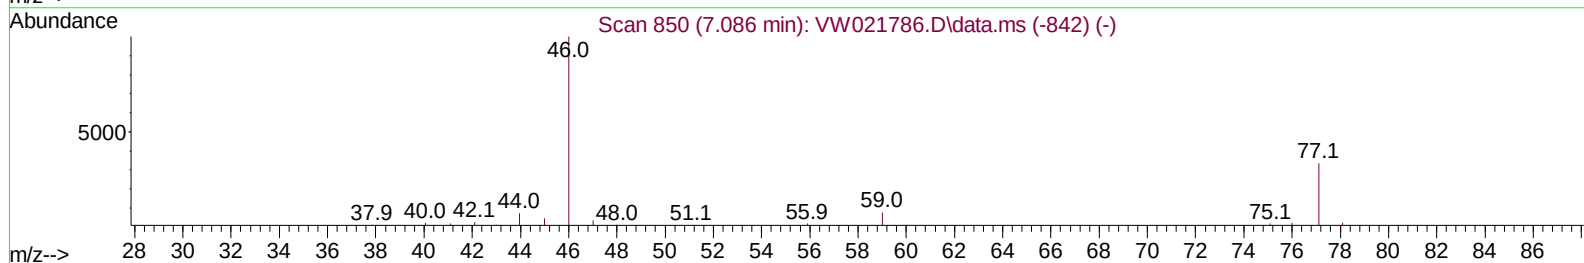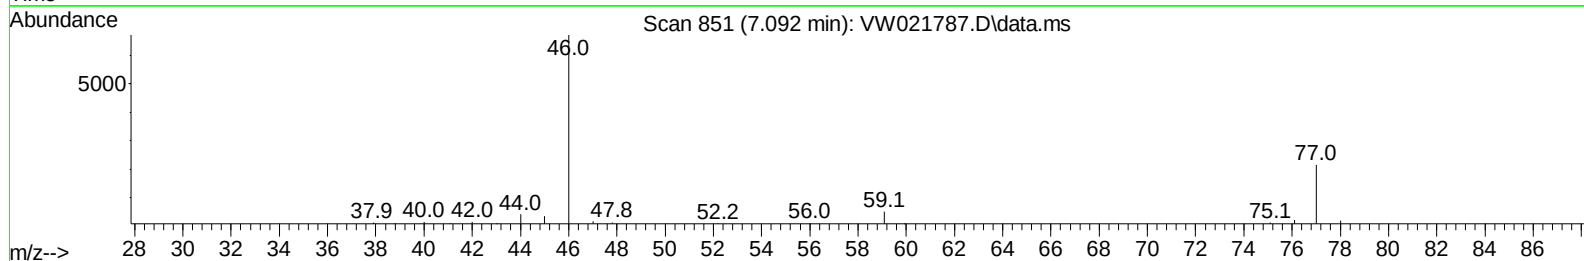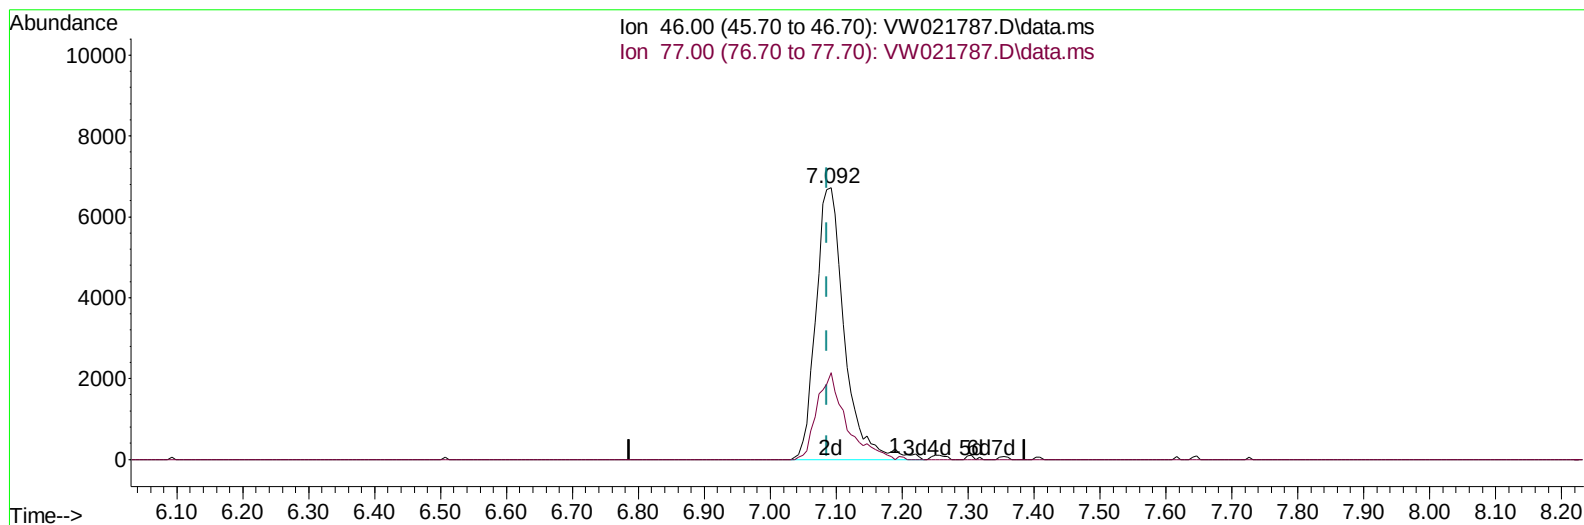

TIC: VW021787.D\data.ms

(21) 2-Butanone-d5 (S)

7.092min (+ 0.006) 49.40 ug/L m

response 20153

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	0.24#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
 Data File : VW021787.D
 Acq On : 07 Jan 2022 20:42
 Operator : SY/VA
 Sample : VW0107SBL02
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK438

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

Quant Time: Jan 07 22:46:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 22:46:04 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		141436	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117		138891	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		80960	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		53884	19.323	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.280%	
7) Chloroethane-d5	2.885	69		40221	21.414	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.640%	
11) 1,1-Dichloroethene-d2	4.019	63		69184	16.953	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.800%	
21) 2-Butanone-d5	7.092	46		20153m	49.396	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.800%	
24) Chloroform-d	7.653	84		107104	24.242	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.960%	
26) 1,2-Dichloroethane-d4	8.305	65		53261	22.830	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.320%	
32) Benzene-d6	8.275	84		213827	25.928	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.720%	
36) 1,2-Dichloropropane-d6	9.274	67		56692	25.340	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.360%	
41) Toluene-d8	10.323	98		206576	25.140	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.560%	
43) trans-1,3-Dichloroprop...	10.579	79		22641	20.798	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.200%	
47) 2-Hexanone-d5	10.927	63		16656	49.090	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.180%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84		46015	24.948	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.800%	
66) 1,2-Dichlorobenzene-d4	13.853	152		81608	26.359	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.440%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
Data File : VW021787.D
Acq On : 07 Jan 2022 20:42
Operator : SY/VA
Sample : VW0107SBL02
Misc : 5.00g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK438

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/10/2022
Supervised By :Mahesh Dadoda 01/10/2022

Quant Time: Jan 07 22:46:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 07 22:46:04 2022
Response via : Initial Calibration

