




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
Data File : VW021800.D
Acq On : 08 Jan 2022 01:53
Operator : SY/VA
Sample : N1053-18
Misc : 6.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLJ5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/10/2022
Supervised By :Mahesh Dadoda 01/10/2022

Quant Time: Jan 08 02:48:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 07 22:46:04 2022
Response via : Initial Calibration

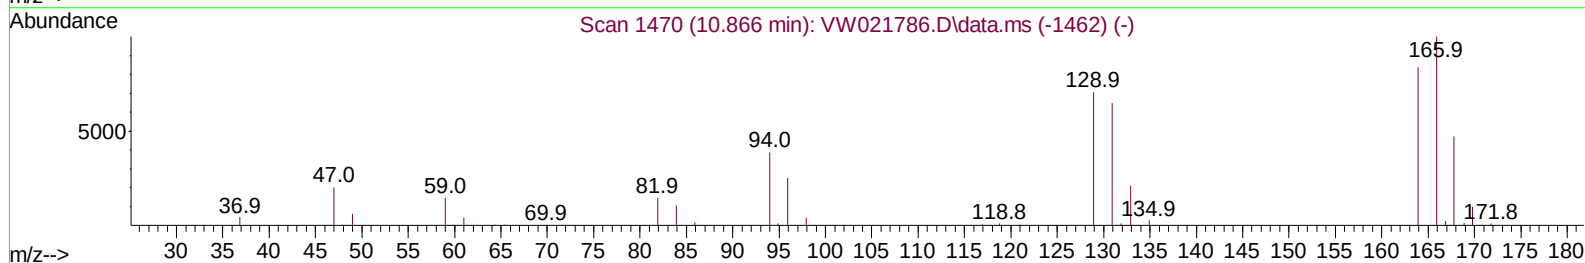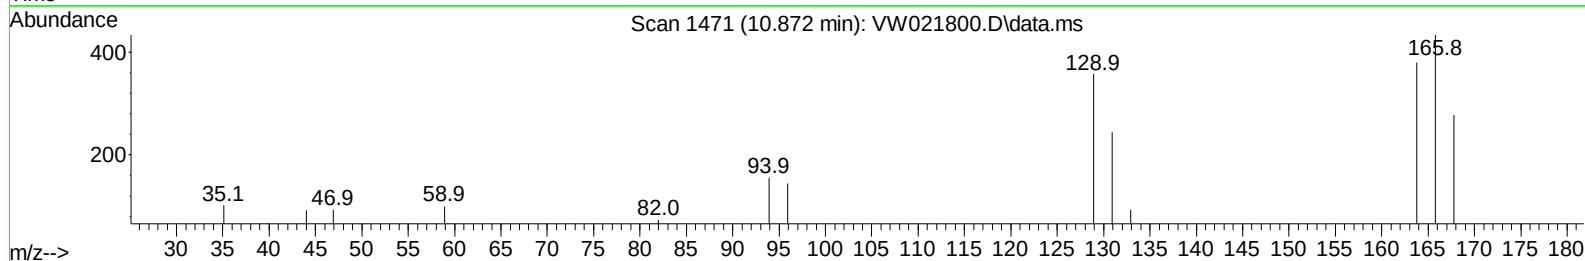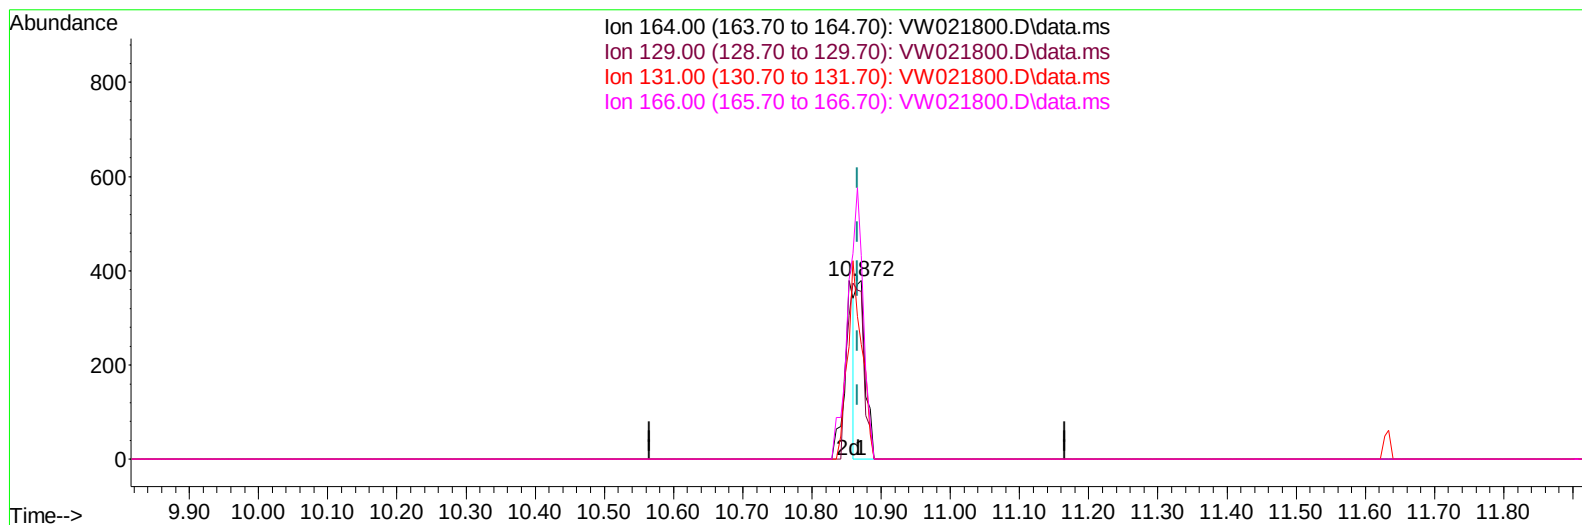

TIC: VW021800.D\data.ms

(46) Tetrachloroethene (T)

10.872min (+ 0.006) 0.37 ug/L

response 362

Ion	Exp%	Act%
164.00	100.00	100.00
129.00	93.60	94.20
131.00	85.30	64.38
166.00	126.70	114.25




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
 Data File : VW021800.D
 Acq On : 08 Jan 2022 01:53
 Operator : SY/VA
 Sample : N1053-18
 Misc : 6.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLJ5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

Quant Time: Jan 08 02:48:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 22:46:04 2022
 Response via : Initial Calibration

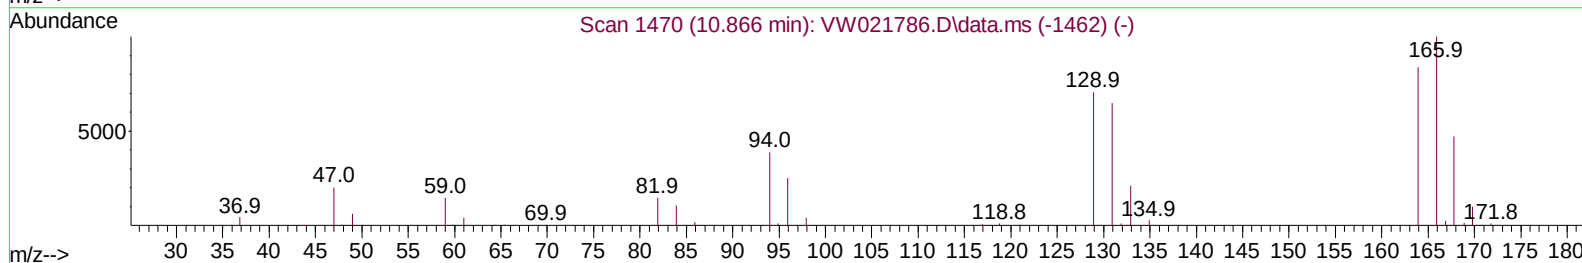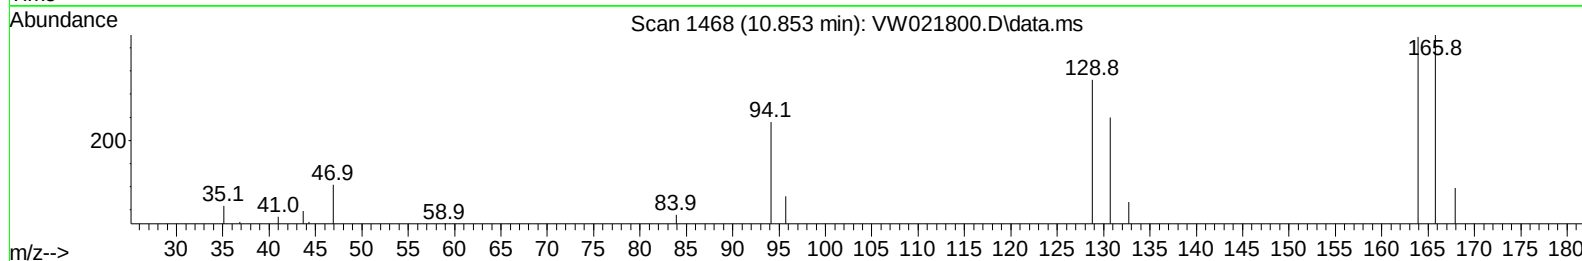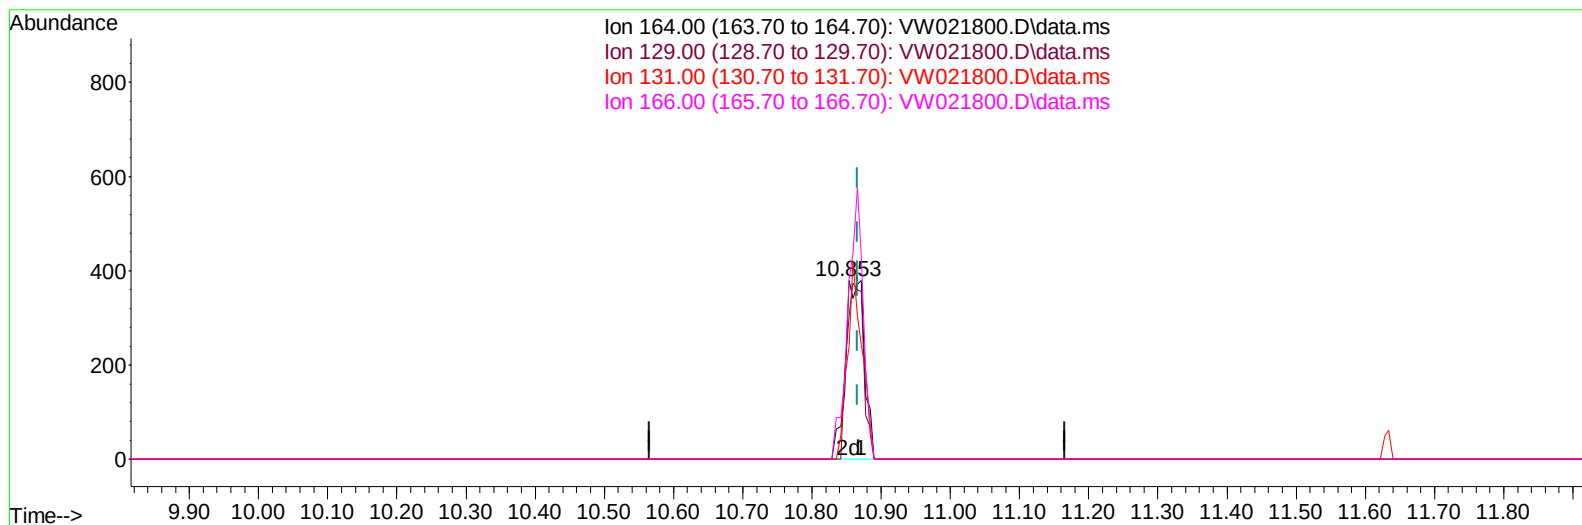

TIC: VW021800.D\data.ms

(46) Tetrachloroethene (T)

10.853min (-0.012) 0.73 ug/L m

response 726

Ion	Exp%	Act%
164.00	100.00	100.00
129.00	93.60	80.47
131.00	85.30	63.06
166.00	126.70	100.79

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
 Data File : VW021800.D
 Acq On : 08 Jan 2022 01:53
 Operator : SY/VA
 Sample : N1053-18
 Misc : 6.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLJ5

Manual IntegrationsAPPROVED

Quant Time: Jan 08 02:48:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 22:46:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/10/2022
 Supervised By :Mahesh Dadoda 01/10/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		80403	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117		61019	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		16061	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		23941	15.102	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	60.400%	
7) Chloroethane-d5	2.885	69		18194	17.040	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	68.160%	
11) 1,1-Dichloroethene-d2	4.019	63		32126	13.848	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	55.400%	
21) 2-Butanone-d5	7.086	46		13862	59.768	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	119.540%	
24) Chloroform-d	7.653	84		54256	21.602	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	86.400%	
26) 1,2-Dichloroethane-d4	8.311	65		29867	22.520	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	90.080%	
32) Benzene-d6	8.275	84		104248	28.773	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	115.080%	
36) 1,2-Dichloropropane-d6	9.274	67		29356	29.867	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	119.480%	
41) Toluene-d8	10.323	98		86766	24.035	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	96.160%	
43) trans-1,3-Dichloroprop...	10.579	79		8709	18.209	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	72.840%	
47) 2-Hexanone-d5	10.927	63		9540	64.000	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	128.000%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84		20581	25.399	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	101.600%	
66) 1,2-Dichlorobenzene-d4	13.853	152		14007	22.806	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	91.240%	
Target Compounds							
13) Acetone	4.141	43		1779	9.034	ug/L	Qvalue 75
46) Tetrachloroethene	10.853	164		726m	0.734	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010722\
Data File : VW021800.D
Acq On : 08 Jan 2022 01:53
Operator : SY/VA
Sample : N1053-18
Misc : 6.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLJ5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/10/2022
Supervised By :Mahesh Dadoda 01/10/2022

Quant Time: Jan 08 02:48:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 07 22:46:04 2022
Response via : Initial Calibration

