




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
Data File : VW027828.D  
Acq On : 08 Jan 2024 13:28  
Operator : SY/MD  
Sample : VSTD2.504  
Misc : 5.00g/10mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
VSTD2.5404

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/09/2024  
Supervised By :Mahesh Dadoda 01/09/2024

Quant Time: Jan 09 03:51:06 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
Quant Title : SFAM01.0  
QLast Update : Tue Jan 09 03:50:03 2024  
Response via : Initial Calibration

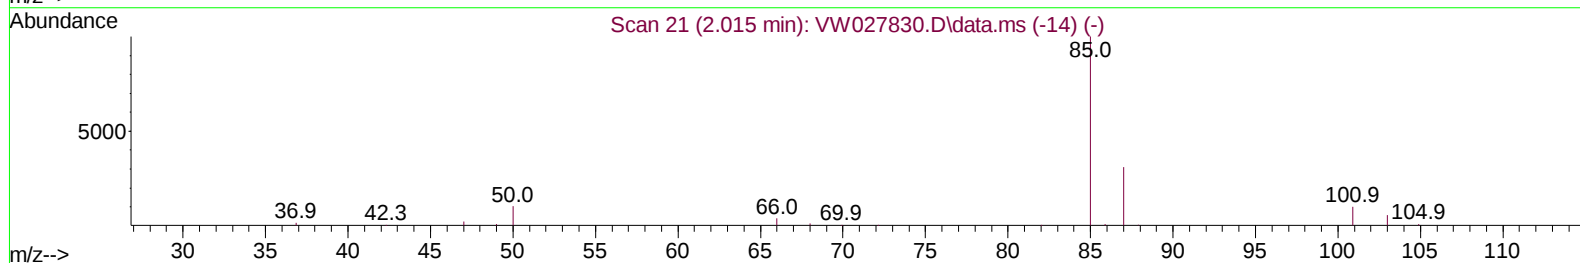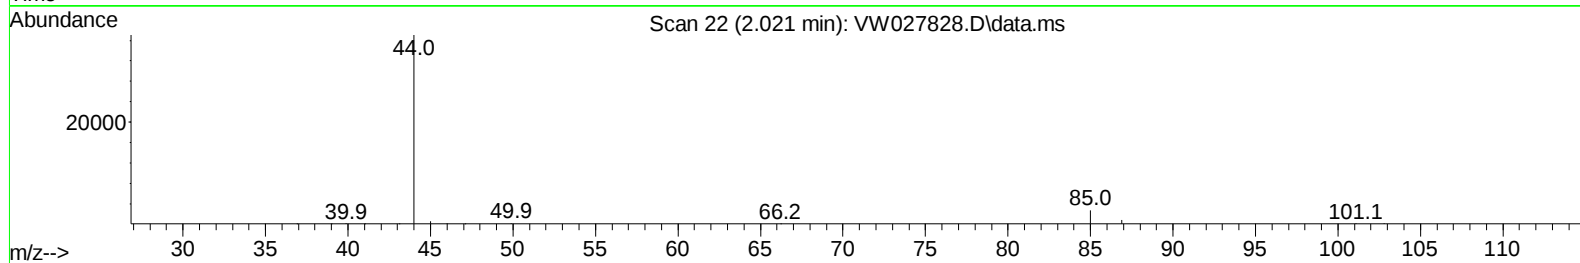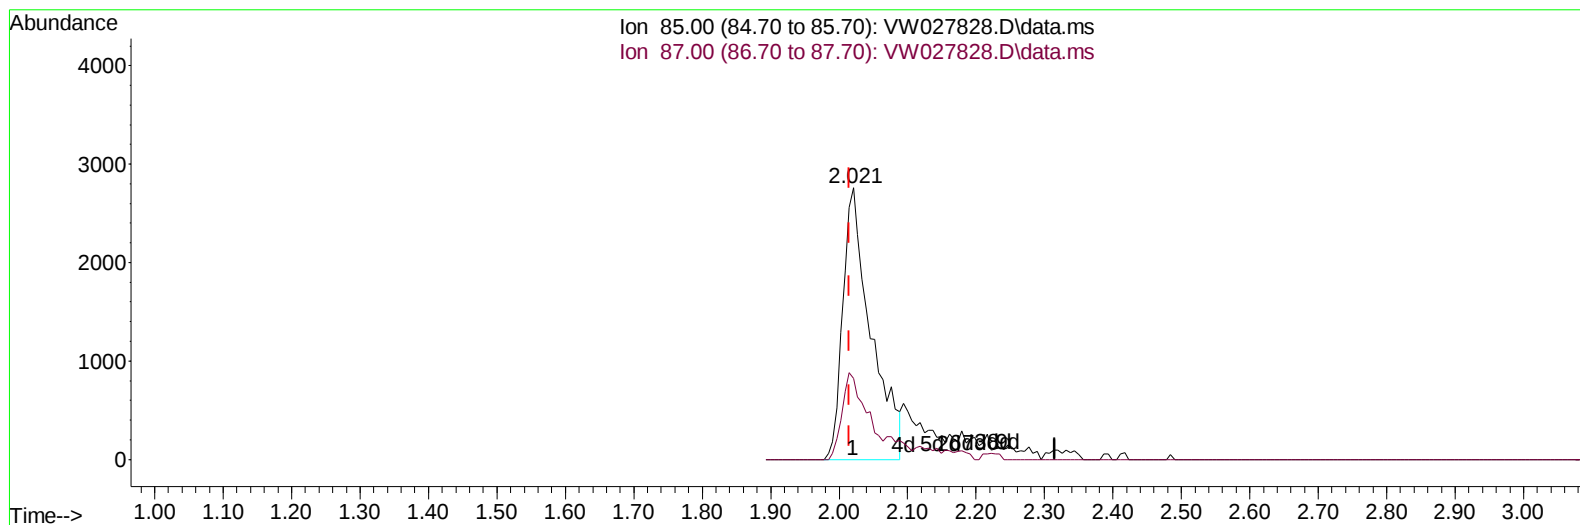

TIC: VW027828.D\data.ms

## (2) Dichlorodifluoromethane (T)

2.021min (+ 0.006) 2.31 ug/L

response 7820

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 85.00 | 100.00 | 100.00 |
| 87.00 | 31.20  | 27.74  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
Data File : VW027828.D  
Acq On : 08 Jan 2024 13:28  
Operator : SY/MD  
Sample : VSTD2.504  
Misc : 5.00g/10mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
VSTD2.5404

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/09/2024  
Supervised By :Mahesh Dadoda 01/09/2024

Quant Time: Jan 09 03:51:06 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
Quant Title : SFAM01.0  
QLast Update : Tue Jan 09 03:50:03 2024  
Response via : Initial Calibration

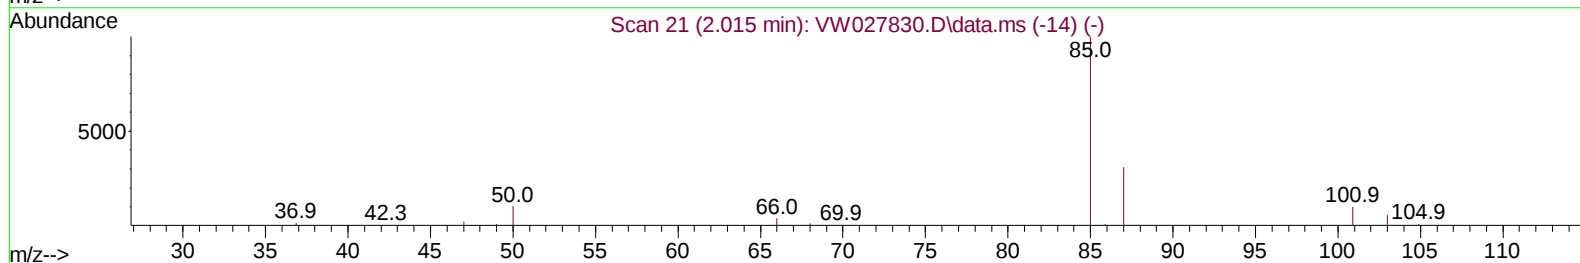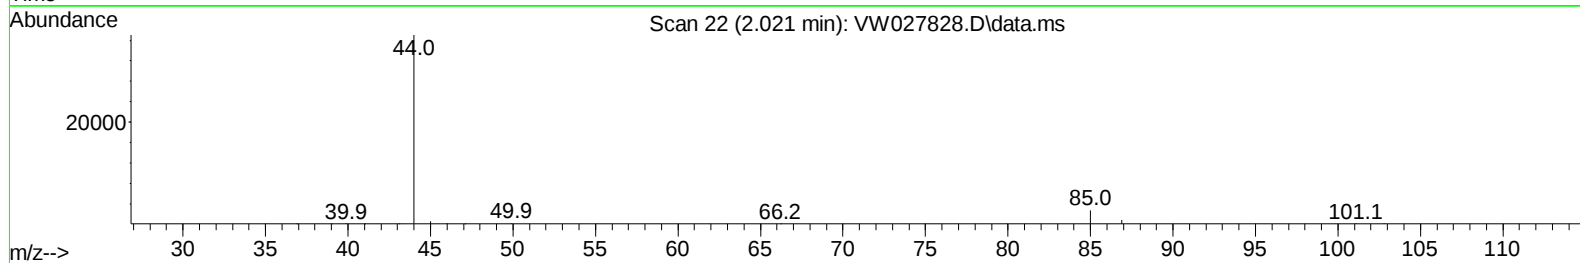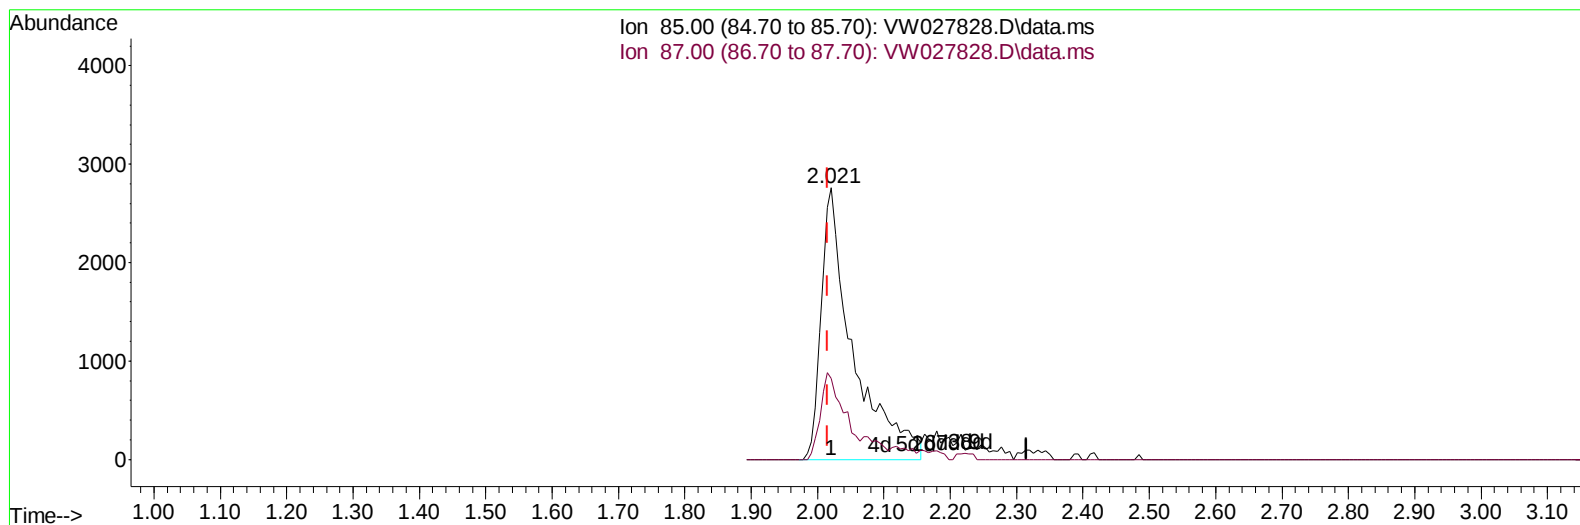

TIC: VW027828.D\data.ms

## (2) Dichlorodifluoromethane (T)

2.021min (+ 0.006) 2.70 ug/L m

response 9159

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 85.00 | 100.00 | 100.00 |
| 87.00 | 31.20  | 23.68# |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
Data File : VW027828.D  
Acq On : 08 Jan 2024 13:28  
Operator : SY/MD  
Sample : VSTD2.504  
Misc : 5.00g/10mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
VSTD2.5404

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/09/2024  
Supervised By :Mahesh Dadoda 01/09/2024

Quant Time: Jan 09 03:51:06 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
Quant Title : SFAM01.0  
QLast Update : Tue Jan 09 03:50:03 2024  
Response via : Initial Calibration

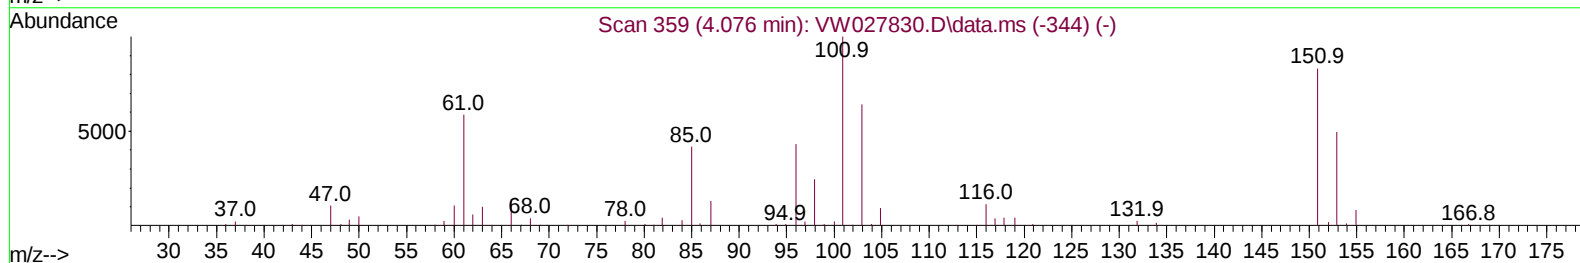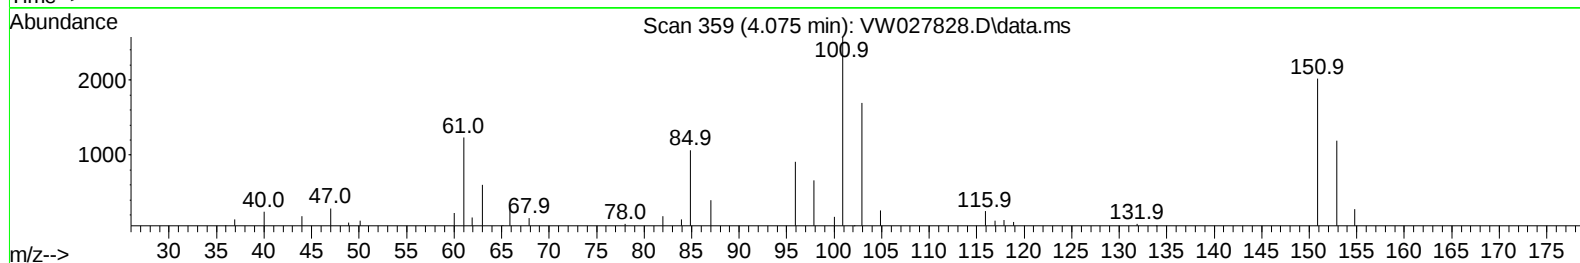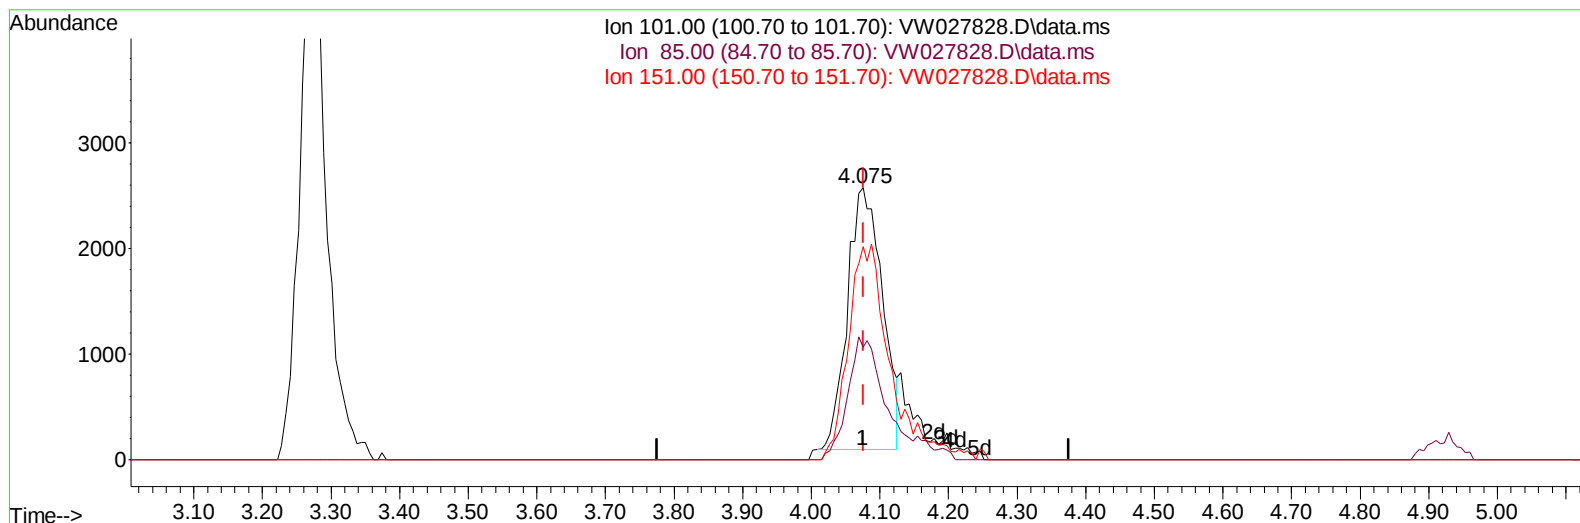

TIC: VW027828.D\data.ms

## (10) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

4.075min (-0.000) 2.05 ug/L

response 8767

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 101.00 | 100.00 | 100.00 |
| 85.00  | 40.70  | 22.31# |
| 151.00 | 75.80  | 47.01# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
Data File : VW027828.D  
Acq On : 08 Jan 2024 13:28  
Operator : SY/MD  
Sample : VSTD2.504  
Misc : 5.00g/10mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
VSTD2.5404

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/09/2024  
Supervised By :Mahesh Dadoda 01/09/2024

Quant Time: Jan 09 03:51:06 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
Quant Title : SFAM01.0  
QLast Update : Tue Jan 09 03:50:03 2024  
Response via : Initial Calibration

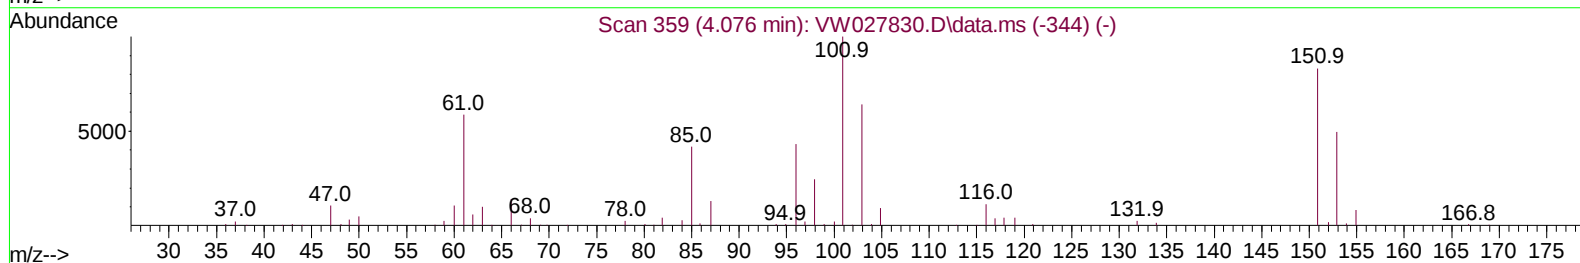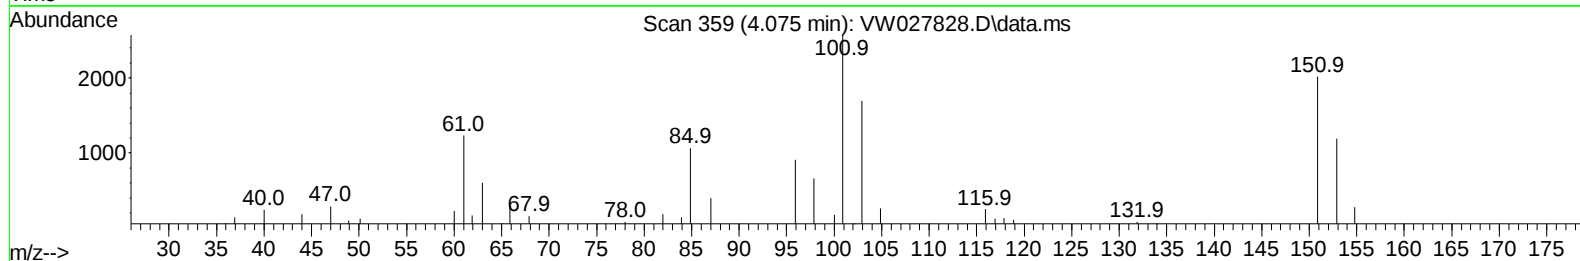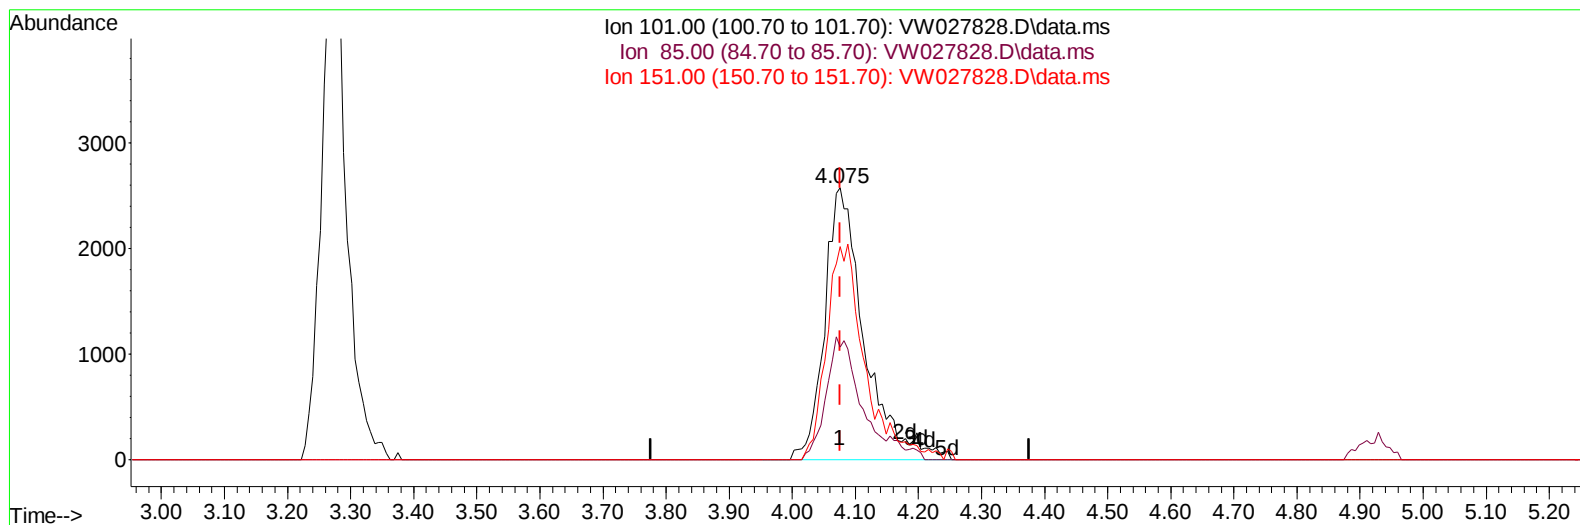

TIC: VW027828.D\data.ms

## (10) 1,1,2-Trichloro-1,2,2-trifluoroethane (T)

4.075min (-0.000) 2.64 ug/L m

response 11260

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 101.00 | 100.00 | 100.00 |
| 85.00  | 40.70  | 17.37# |
| 151.00 | 75.80  | 36.60# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
 Data File : VW027828.D  
 Acq On : 08 Jan 2024 13:28  
 Operator : SY/MD  
 Sample : VSTD2.504  
 Misc : 5.00g/10mL/MSVOA\_W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 VSTD2.5404

Manual IntegrationsAPPROVED

Quant Time: Jan 09 03:51:06 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
 Quant Title : SFAM01.0  
 QLast Update : Tue Jan 09 03:50:03 2024  
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/09/2024  
 Supervised By :Mahesh Dadoda 01/09/2024

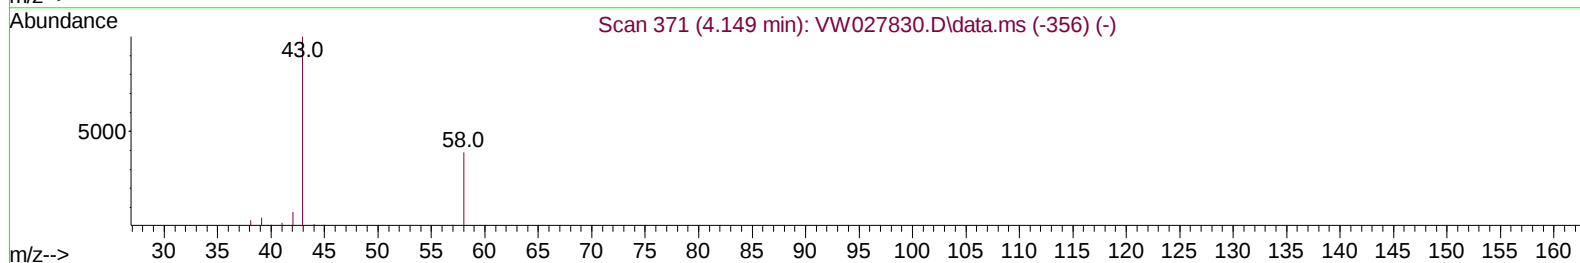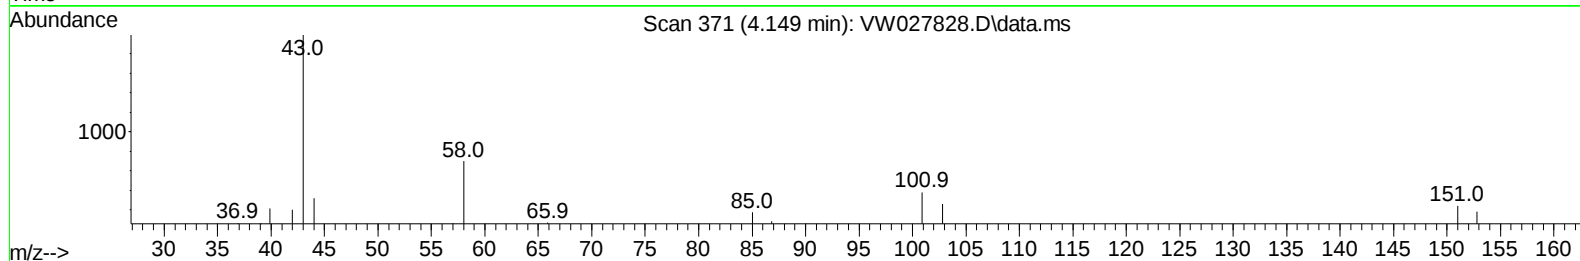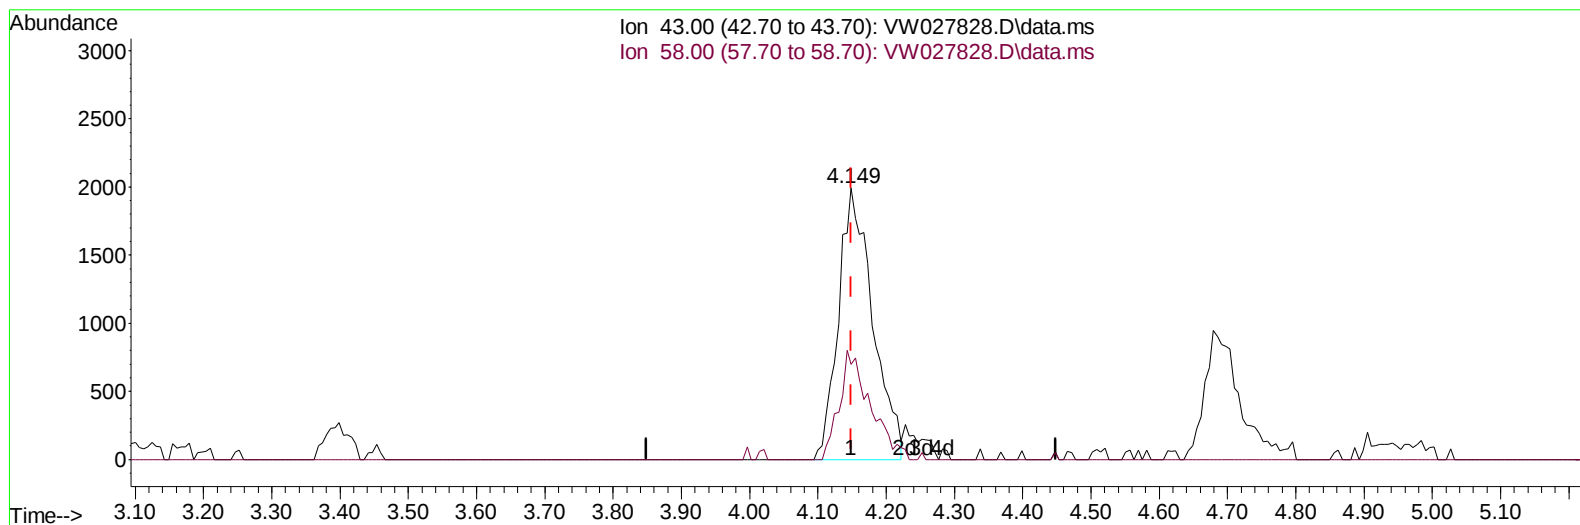

TIC: VW027828.D\data.ms

(13) Acetone (T)

4.149min (-0.000) 8.00 ug/L

response 6926

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.00 | 100.00 | 100.00 |
| 58.00 | 35.10  | 34.90  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
 Data File : VW027828.D  
 Acq On : 08 Jan 2024 13:28  
 Operator : SY/MD  
 Sample : VSTD2.504  
 Misc : 5.00g/10mL/MSVOA\_W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 VSTD2.5404

Manual IntegrationsAPPROVED

Quant Time: Jan 09 03:51:06 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
 Quant Title : SFAM01.0  
 QLast Update : Tue Jan 09 03:50:03 2024  
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/09/2024  
 Supervised By :Mahesh Dadoda 01/09/2024

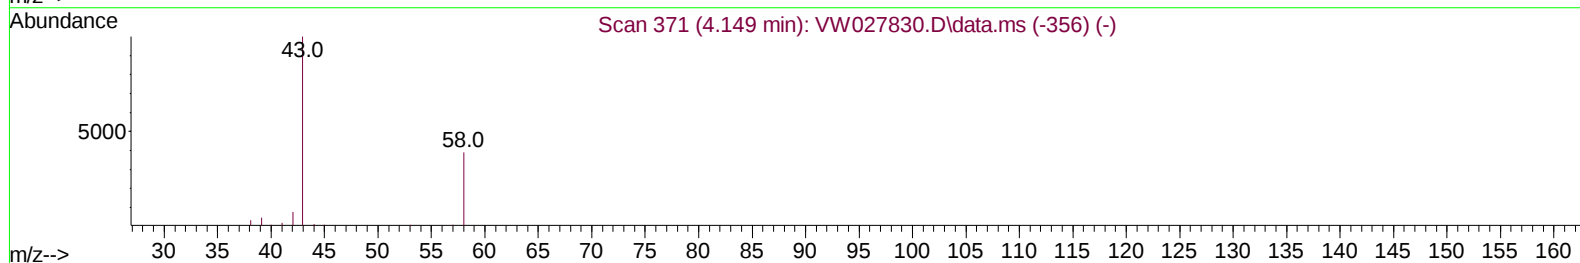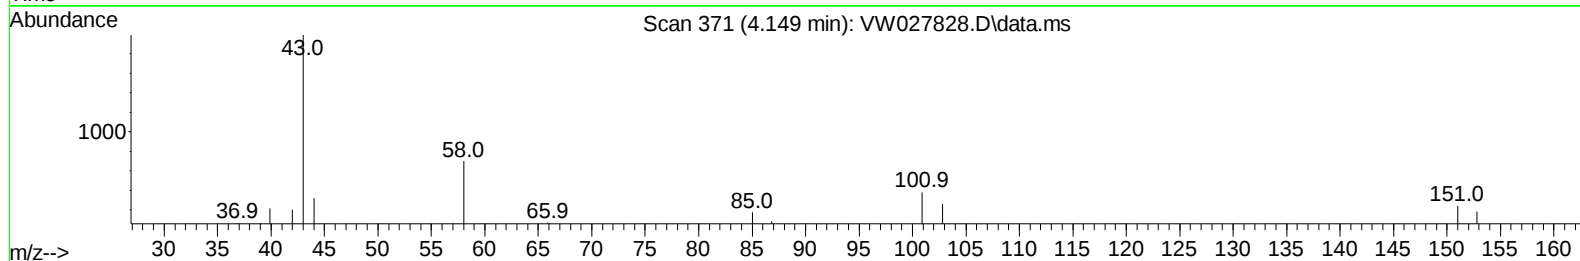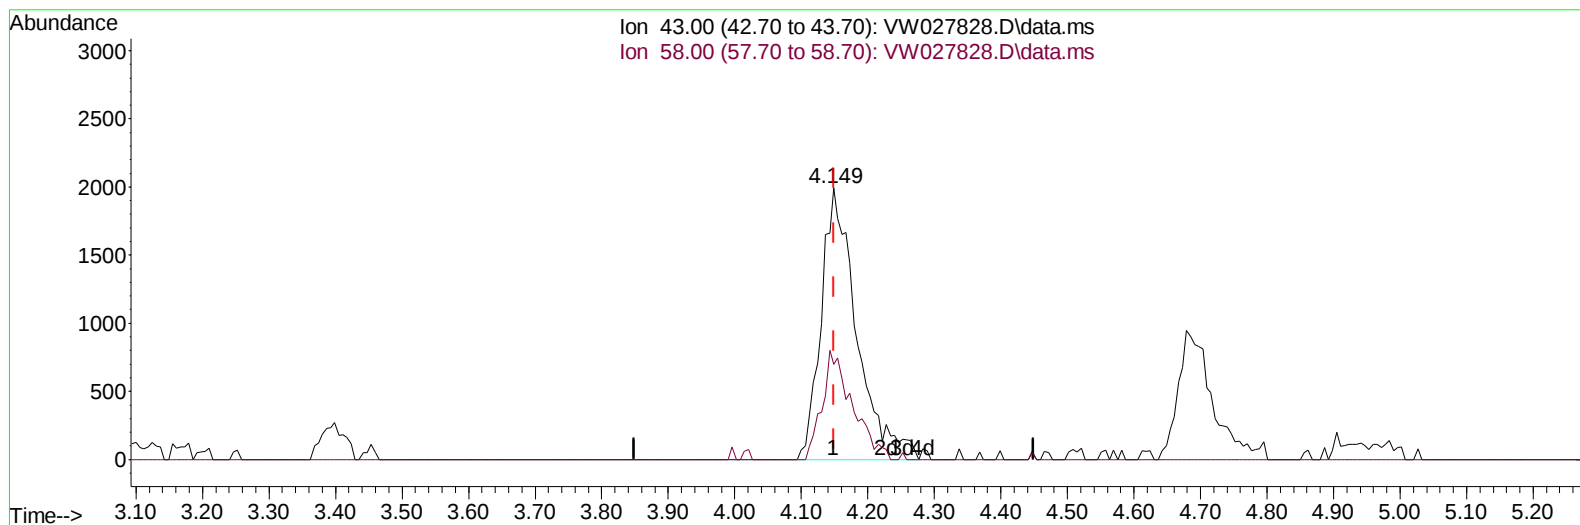

TIC: VW027828.D\data.ms

(13) Acetone (T)

4.149min (-0.000) 8.52 ug/L m

response 7371

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.00 | 100.00 | 100.00 |
| 58.00 | 35.10  | 32.79  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
Data File : VW027828.D  
Acq On : 08 Jan 2024 13:28  
Operator : SY/MD  
Sample : VSTD2.504  
Misc : 5.00g/10mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
VSTD2.5404

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/09/2024  
Supervised By :Mahesh Dadoda 01/09/2024

Quant Time: Jan 09 03:51:06 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
Quant Title : SFAM01.0  
QLast Update : Tue Jan 09 03:50:03 2024  
Response via : Initial Calibration

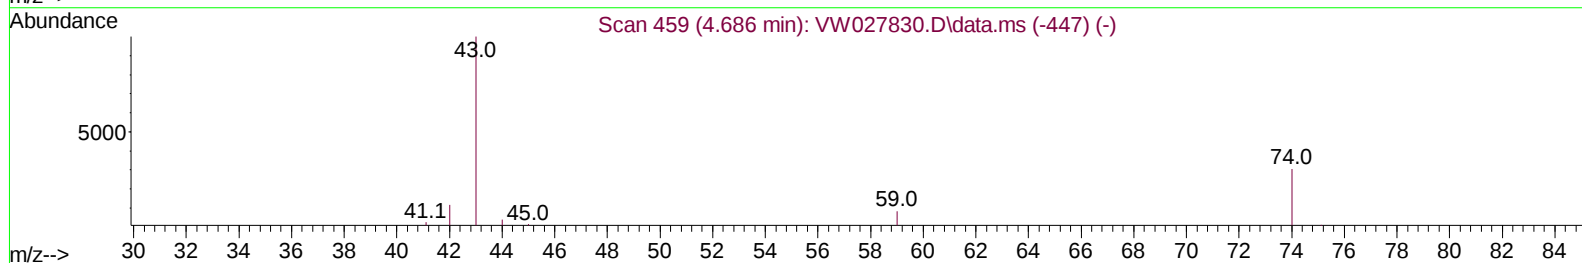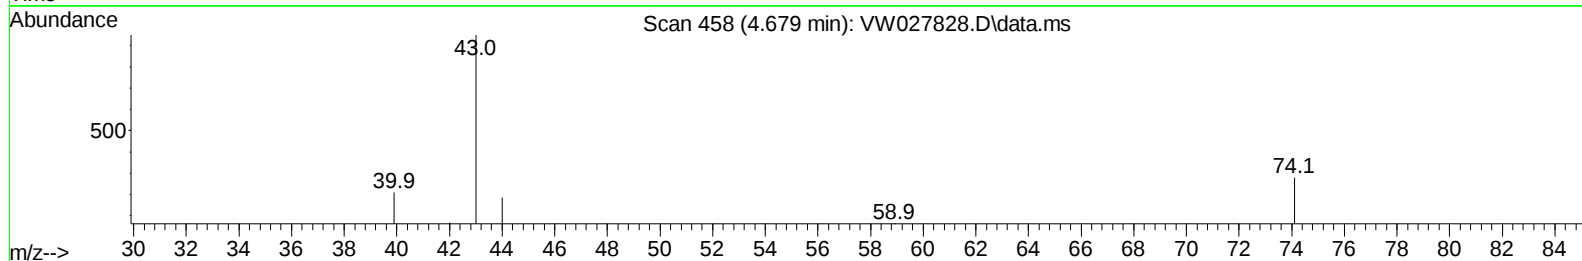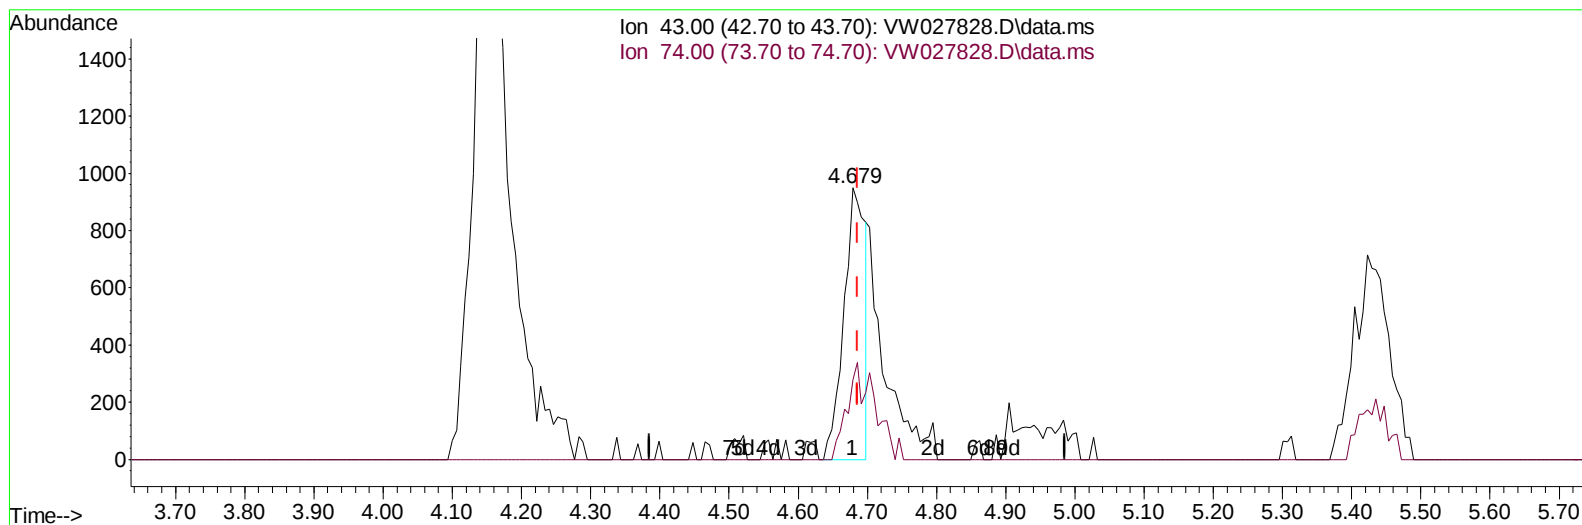

TIC: VW027828.D\data.ms

## (15) Methyl Acetate (T)

4.679min (-0.007) 1.67 ug/L

response 2003

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.00 | 100.00 | 100.00 |
| 74.00 | 27.40  | 23.91  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
 Data File : VW027828.D  
 Acq On : 08 Jan 2024 13:28  
 Operator : SY/MD  
 Sample : VSTD2.504  
 Misc : 5.00g/10mL/MSVOA\_W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 VSTD2.5404

Manual IntegrationsAPPROVED

Quant Time: Jan 09 03:51:06 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
 Quant Title : SFAM01.0  
 QLast Update : Tue Jan 09 03:50:03 2024  
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/09/2024  
 Supervised By :Mahesh Dadoda 01/09/2024

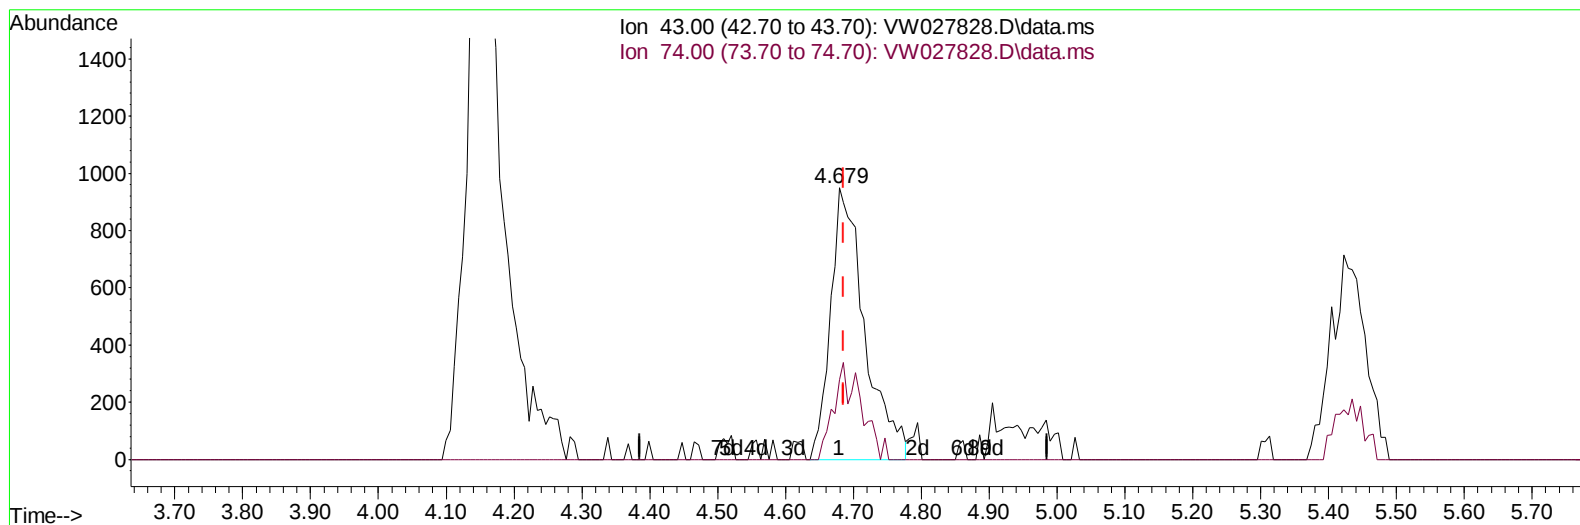




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
Data File : VW027828.D  
Acq On : 08 Jan 2024 13:28  
Operator : SY/MD  
Sample : VSTD2.504  
Misc : 5.00g/10mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
VSTD2.5404

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/09/2024  
Supervised By :Mahesh Dadoda 01/09/2024

Quant Time: Jan 09 03:51:06 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
Quant Title : SFAM01.0  
QLast Update : Tue Jan 09 03:50:03 2024  
Response via : Initial Calibration

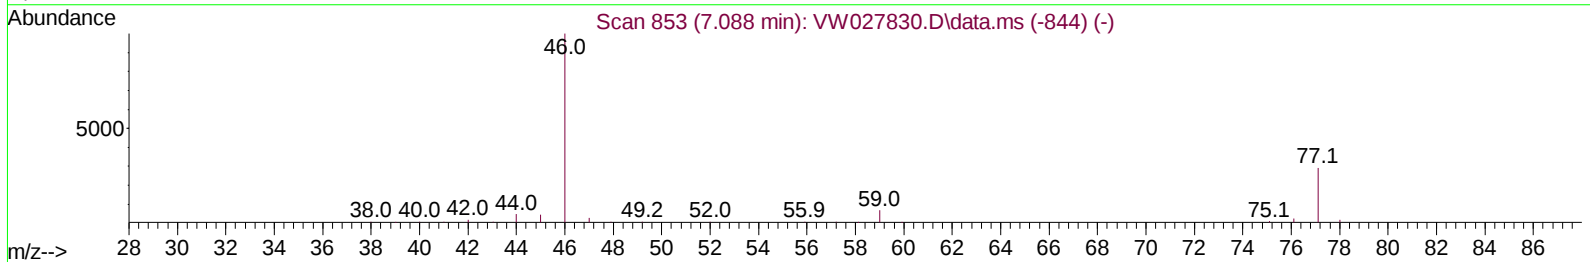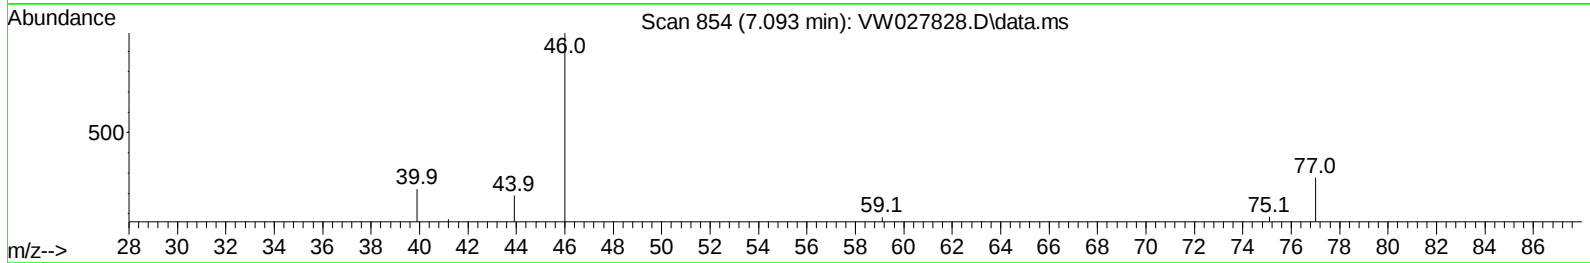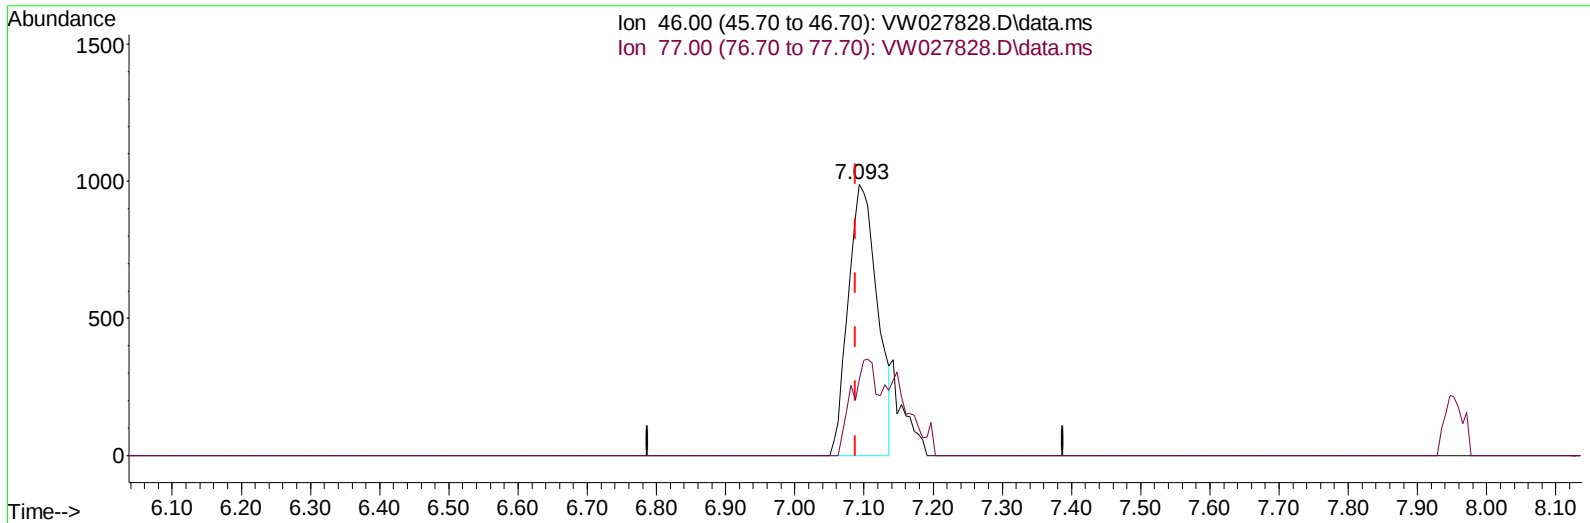

TIC: VW027828.D\data.ms

## (21) 2-Butanone-d5 (S)

7.093min (+ 0.006) 4.06 ug/L

response 2907

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 46.00 | 100.00 | 100.00 |
| 77.00 | 31.60  | 8.88#  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
Data File : VW027828.D  
Acq On : 08 Jan 2024 13:28  
Operator : SY/MD  
Sample : VSTD2.504  
Misc : 5.00g/10mL/MSVOA\_W/SoIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
VSTD2.5404

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/09/2024  
Supervised By :Mahesh Dadoda 01/09/2024

Quant Time: Jan 09 03:51:06 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
Quant Title : SFAM01.0  
QLast Update : Tue Jan 09 03:50:03 2024  
Response via : Initial Calibration

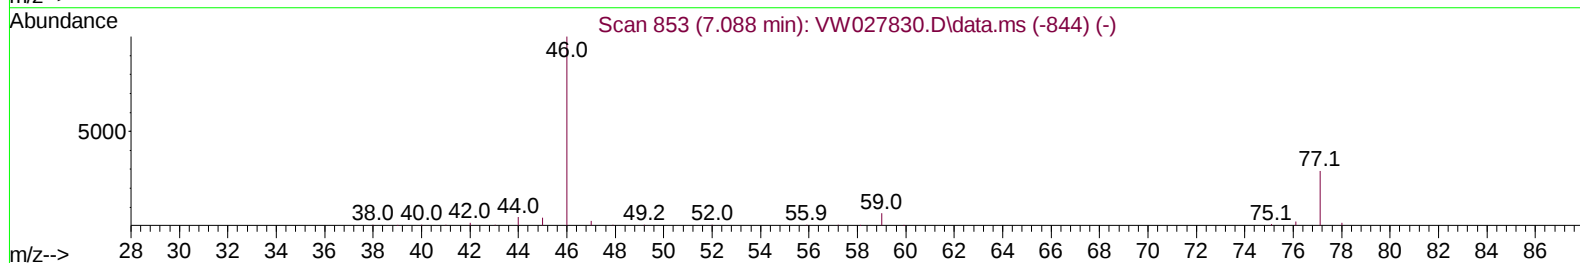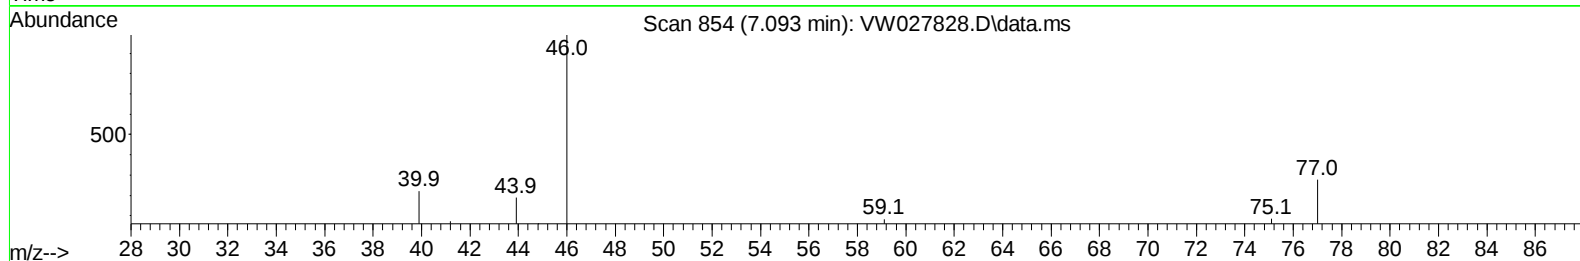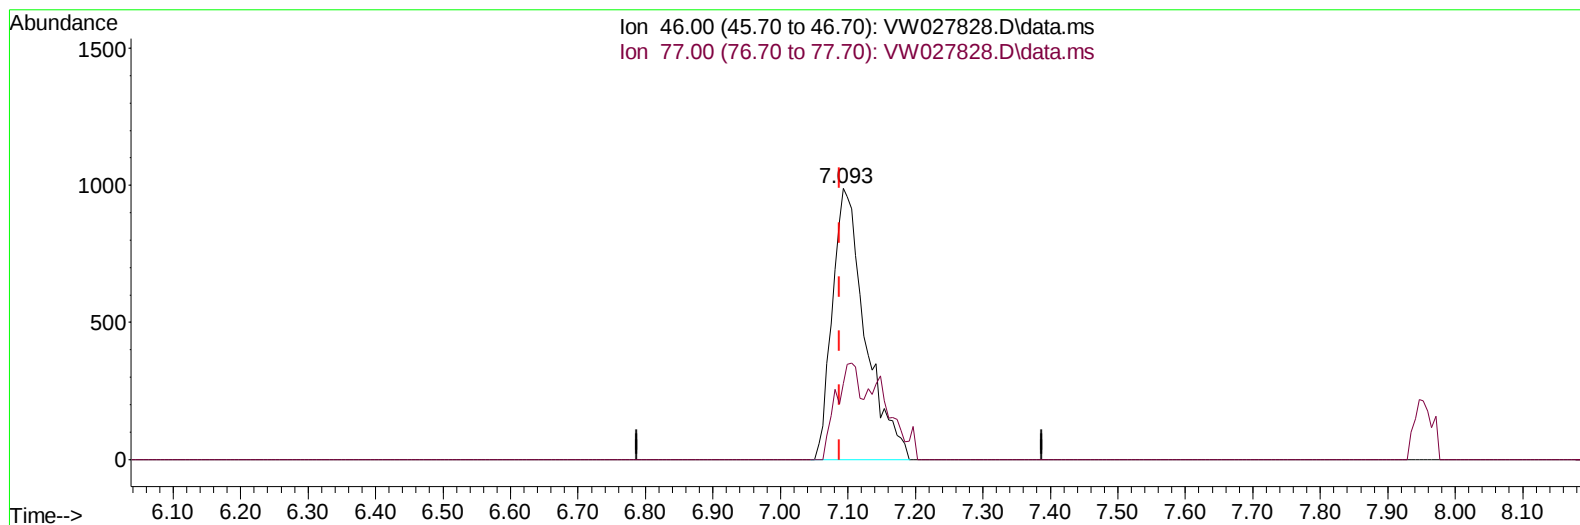

TIC: VW027828.D\data.ms

## (21) 2-Butanone-d5 (S)

7.093min (+ 0.006) 4.68 ug/L m

response 3345

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 46.00 | 100.00 | 100.00 |
| 77.00 | 31.60  | 7.71#  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
 Data File : VW027828.D  
 Acq On : 08 Jan 2024 13:28  
 Operator : SY/MD  
 Sample : VSTD2.504  
 Misc : 5.00g/10mL/MSVOA\_W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 VSTD2.5404

Manual IntegrationsAPPROVED

Quant Time: Jan 09 03:51:06 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
 Quant Title : SFAM01.0  
 QLast Update : Tue Jan 09 03:50:03 2024  
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/09/2024  
 Supervised By :Mahesh Dadoda 01/09/2024

| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| -----                         |        |      |          |        |        |          |
| Internal Standards            |        |      |          |        |        |          |
| 1) 1,4-Difluorobenzene        | 8.843  | 114  | 352426   | 25.000 | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 11.629 | 117  | 316886   | 25.000 | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 13.555 | 152  | 152893   | 25.000 | ug/L   | 0.00     |
| System Monitoring Compounds   |        |      |          |        |        |          |
| 4) Vinyl Chloride-d3          | 2.368  | 65   | 10481    | 2.434  | ug/L   | 0.00     |
| 7) Chloroethane-d5            | 2.905  | 69   | 10487    | 2.781  | ug/L   | 0.00     |
| 11) 1,1-Dichloroethene-d2     | 4.021  | 65   | 5340     | 2.759  | ug/L   | 0.00     |
| 21) 2-Butanone-d5             | 7.093  | 46   | 3345m    | 4.675  | ug/L   | 0.00     |
| 24) Chloroform-d              | 7.648  | 84   | 21999    | 2.583  | ug/L   | 0.00     |
| 26) 1,2-Dichloroethane-d4     | 8.306  | 65   | 10063    | 2.604  | ug/L   | 0.00     |
| 32) Benzene-d6                | 8.276  | 84   | 47022    | 2.640  | ug/L   | 0.00     |
| 36) 1,2-Dichloropropane-d6    | 9.276  | 67   | 12695    | 2.548  | ug/L   | 0.00     |
| 41) Toluene-d8                | 10.324 | 98   | 42048    | 2.515  | ug/L   | 0.00     |
| 43) trans-1,3-Dichloroprop... | 10.574 | 79   | 4774     | 2.515  | ug/L   | 0.00     |
| 47) 2-Hexanone-d5             | 10.922 | 63   | 2991     | 4.599  | ug/L   | 0.00     |
| 56) 1,1,2,2-Tetrachloroeth... | 12.690 | 84   | 9034     | 2.570  | ug/L   | 0.00     |
| 66) 1,2-Dichlorobenzene-d4    | 13.848 | 152  | 13584    | 2.508  | ug/L   | 0.00     |
| Target Compounds              |        |      |          |        |        |          |
|                               |        |      |          |        | Qvalue |          |
| 2) Dichlorodifluoromethane    | 2.021  | 85   | 9159m    | 2.700  | ug/L   |          |
| 3) Chloromethane              | 2.222  | 50   | 11502    | 2.522  | ug/L   | 98       |
| 5) Vinyl chloride             | 2.375  | 62   | 9574     | 2.088  | ug/L   | 93       |
| 6) Bromomethane               | 2.789  | 94   | 9289     | 2.588  | ug/L   | 99       |
| 8) Chloroethane               | 2.929  | 64   | 7122     | 2.298  | ug/L   | 91       |
| 9) Trichlorofluoromethane     | 3.271  | 101  | 13465    | 2.565  | ug/L   | 98       |
| 10) 1,1,2-Trichloro-1,2,2-... | 4.075  | 101  | 11260m   | 2.637  | ug/L   |          |
| 12) 1,1-Dichloroethene        | 4.045  | 96   | 10555    | 2.508  | ug/L   | 99       |
| 13) Acetone                   | 4.149  | 43   | 7371m    | 8.515  | ug/L   |          |
| 14) Carbon disulfide          | 4.386  | 76   | 32192    | 2.501  | ug/L   | 97       |
| 15) Methyl Acetate            | 4.679  | 43   | 3319m    | 2.763  | ug/L   |          |
| 16) Methylene chloride        | 4.917  | 84   | 18148    | 3.509  | ug/L   | 97       |
| 17) trans-1,2-Dichloroethene  | 5.429  | 96   | 11266    | 2.512  | ug/L   | 96       |
| 18) Methyl tert-butyl Ether   | 5.429  | 73   | 13435    | 2.439  | ug/L   | 94       |
| 19) 1,1-Dichloroethane        | 6.221  | 63   | 19174    | 2.519  | ug/L   | 95       |
| 20) cis-1,2-Dichloroethene    | 7.166  | 96   | 12291    | 2.543  | ug/L   | 83       |
| 22) 2-Butanone                | 7.191  | 43   | 4811     | 5.447  | ug/L   | 89       |
| 23) Bromochloromethane        | 7.520  | 128  | 5302     | 2.500  | ug/L # | 90       |
| 25) Chloroform                | 7.678  | 83   | 20023    | 2.536  | ug/L   | 96       |
| 27) 1,2-Dichloroethane        | 8.398  | 62   | 11523    | 2.592  | ug/L   | 97       |
| 29) Cyclohexane               | 7.959  | 56   | 15324    | 2.377  | ug/L   | 100      |
| 30) 1,1,1-Trichloroethane     | 7.867  | 97   | 16104    | 2.537  | ug/L   | 100      |
| 31) Carbon tetrachloride      | 8.069  | 117  | 13551    | 2.451  | ug/L   | 98       |
| 33) Benzene                   | 8.325  | 78   | 44742    | 2.564  | ug/L   | 100      |
| 34) Trichloroethene           | 9.093  | 95   | 12125    | 2.536  | ug/L   | 95       |
| 35) Methylcyclohexane         | 9.337  | 83   | 19886    | 2.474  | ug/L   | 99       |
| 37) 1,2-Dichloropropane       | 9.367  | 63   | 10899    | 2.598  | ug/L   | 100      |
| 38) Bromodichloromethane      | 9.648  | 83   | 13514    | 2.571  | ug/L   | 95       |
| 39) cis-1,3-Dichloropropene   | 10.074 | 75   | 15272    | 2.347  | ug/L   | 95       |
| 40) 4-Methyl-2-pentanone      | 10.209 | 43   | 7948     | 4.829  | ug/L   | 99       |
| 42) Toluene                   | 10.385 | 91   | 46641    | 2.441  | ug/L   | 89       |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
 Data File : VW027828.D  
 Acq On : 08 Jan 2024 13:28  
 Operator : SY/MD  
 Sample : VSTD2.504  
 Misc : 5.00g/10mL/MSVOA\_W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 VSTD2.5404

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/09/2024  
 Supervised By :Mahesh Dadoda 01/09/2024

Quant Time: Jan 09 03:51:06 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
 Quant Title : SFAM01.0  
 QLast Update : Tue Jan 09 03:50:03 2024  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc  | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|-------|--------|----------|
| 44) trans-1,3-Dichloropropene | 10.605 | 75   | 11485    | 2.291 | ug/L   | 95       |
| 45) 1,1,2-Trichloroethane     | 10.788 | 97   | 8117     | 2.582 | ug/L   | 95       |
| 46) Tetrachloroethene         | 10.861 | 164  | 10562    | 2.744 | ug/L   | 94       |
| 48) 2-Hexanone                | 10.971 | 43   | 5671     | 4.709 | ug/L   | 98       |
| 49) Dibromochloromethane      | 11.129 | 129  | 8807     | 2.577 | ug/L   | 98       |
| 50) 1,2-Dibromoethane         | 11.233 | 107  | 7390     | 2.566 | ug/L   | 81       |
| 51) Chlorobenzene             | 11.653 | 112  | 32621    | 2.598 | ug/L   | 98       |
| 52) Ethylbenzene              | 11.727 | 91   | 52279    | 2.430 | ug/L   | 95       |
| 53) m,p-Xylene                | 11.836 | 106  | 20554    | 2.468 | ug/L   | 97       |
| 54) o-Xylene                  | 12.165 | 106  | 18934    | 2.423 | ug/L   | 98       |
| 55) Styrene                   | 12.178 | 104  | 30533    | 2.304 | ug/L   | 100      |
| 57) 1,1,2,2-Tetrachloroethane | 12.708 | 83   | 8412     | 2.462 | ug/L # | 95       |
| 59) Bromoform                 | 12.348 | 173  | 4639     | 2.462 | ug/L # | 98       |
| 60) Isopropylbenzene          | 12.458 | 105  | 49138    | 2.334 | ug/L   | 98       |
| 61) 1,2,3-Trichloropropane    | 12.763 | 75   | 6027     | 2.575 | ug/L   | 97       |
| 62) 1,3,5-Trimethylbenzene    | 12.940 | 105  | 39895    | 2.387 | ug/L   | 98       |
| 63) 1,2,4-Trimethylbenzene    | 13.245 | 105  | 38719    | 2.322 | ug/L   | 96       |
| 64) 1,3-Dichlorobenzene       | 13.495 | 146  | 24062    | 2.521 | ug/L   | 100      |
| 65) 1,4-Dichlorobenzene       | 13.574 | 146  | 23965    | 2.549 | ug/L   | 93       |
| 67) 1,2-Dichlorobenzene       | 13.866 | 146  | 20405    | 2.453 | ug/L   | 97       |
| 68) 1,2-Dibromo-3-chloropr... | 14.476 | 75   | 1218     | 2.708 | ug/L   | 98       |
| 69) 1,3,5-Trichlorobenzene    | 14.616 | 180  | 16550    | 2.483 | ug/L   | 95       |
| 70) 1,2,4-trichlorobenzene    | 15.122 | 180  | 13198    | 2.444 | ug/L   | 92       |
| 71) Naphthalene               | 15.360 | 128  | 20428    | 2.272 | ug/L   | 98       |
| 72) 1,2,3-Trichlorobenzene    | 15.543 | 180  | 11580    | 2.537 | ug/L   | 98       |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_W\Data\VW010824\  
Data File : VW027828.D  
Acq On : 08 Jan 2024 13:28  
Operator : SY/MD  
Sample : VSTD2.504  
Misc : 5.00g/10mL/MSVOA\_W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
VSTD2.5404

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/09/2024  
Supervised By :Mahesh Dadoda 01/09/2024

Quant Time: Jan 09 03:51:06 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_W\Method\SFAMWLM010824SMA.M  
Quant Title : SFAM01.0  
QLast Update : Tue Jan 09 03:50:03 2024  
Response via : Initial Calibration

