
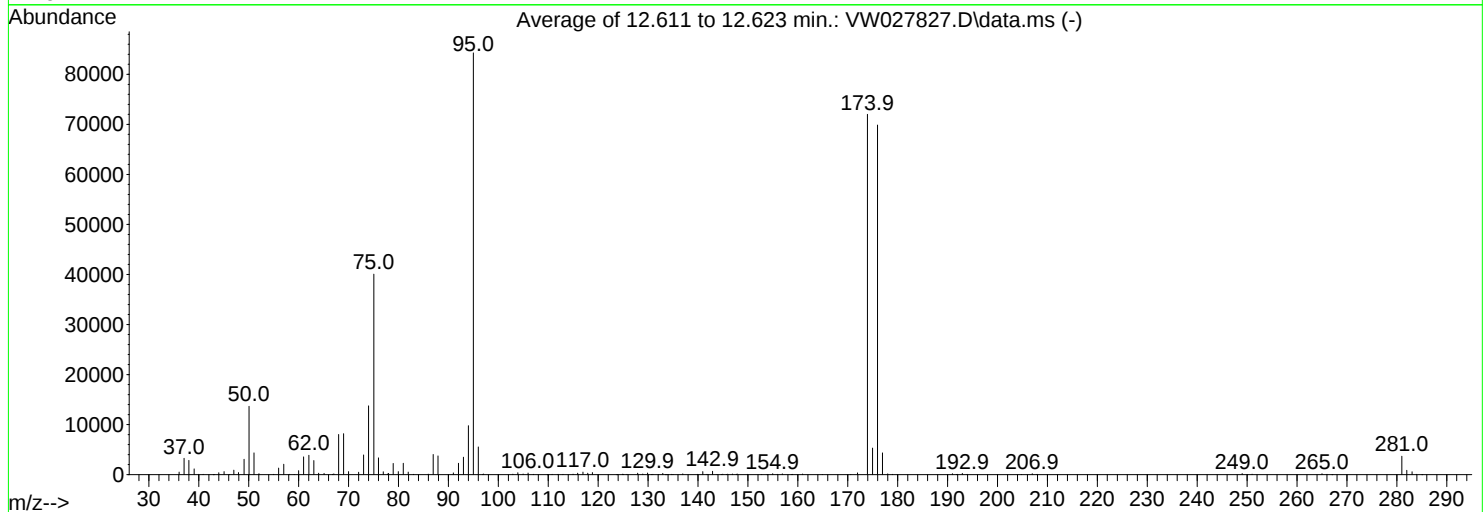


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010824\
Data File : VW027827.D
Acq On : 08 Jan 2024 12:52
Operator : SY/MD
Sample : BFB424
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB424

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Title : SFAM01.0
Last Update : Tue Jan 09 04:13:17 2024

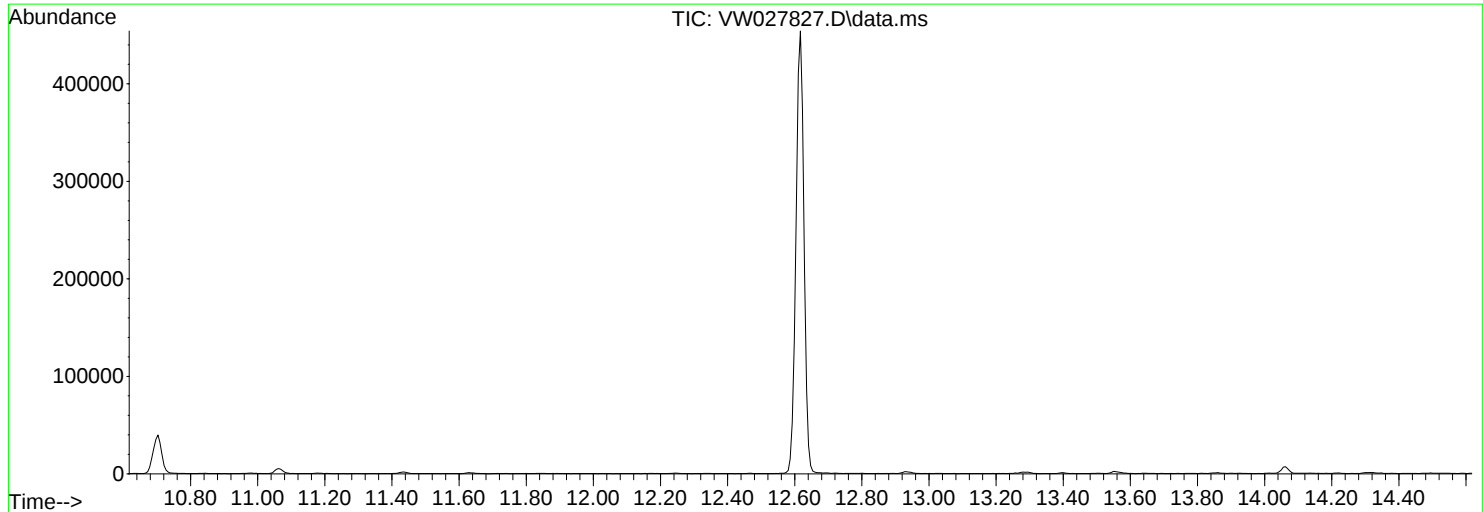

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	13658	PASS
75	95	30	80	47.5	40080	PASS
95	95	100	100	100.0	84291	PASS
96	95	5	9	6.6	5544	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.4	71992	PASS
175	174	5	9	7.4	5302	PASS
176	174	95	101	97.1	69883	PASS
177	176	5	9	6.2	4357	PASS

m/z	Abundance
40.00	147.0
41.10	56.0
42.00	111.0
42.90	63.0
44.10	171.0
55.00	155.0

Instrument :
MSVOA_W
ClientSampleId :
BFB424

m/z	Abundance
36.00	576.0
37.10	3381.0
38.00	3290.0
39.10	1214.0
40.00	255.0
43.00	97.0
44.00	654.0
45.10	640.0
46.10	78.0
47.00	1002.0
47.90	410.0
49.10	3253.0
50.00	14557.0
51.00	4662.0
52.00	221.0
55.00	288.0
56.00	1355.0
57.00	2235.0
58.20	69.0
59.10	58.0
60.00	827.0
61.00	3638.0
62.10	3988.0
63.00	2980.0
64.00	417.0
65.10	325.0
67.10	297.0
68.00	8054.0
69.00	8858.0
70.00	687.0
72.00	459.0
73.00	4172.0
74.00	13766.0
75.00	41656.0
76.00	3513.0
77.00	532.0
77.80	382.0
79.00	2371.0
79.90	561.0
80.90	2394.0
82.00	604.0
83.00	115.0
86.10	92.0
87.00	4647.0
87.90	3887.0
91.00	321.0
92.00	2352.0
93.00	3401.0
94.00	9884.0
95.00	84072.0
96.00	5683.0
96.90	220.0
102.90	166.0
103.90	407.0
105.00	144.0
105.90	336.0
107.00	69.0
109.80	56.0
110.80	96.0
112.00	53.0
113.00	65.0
115.00	71.0
115.90	260.0
116.90	510.0
117.90	291.0
118.80	449.0
124.80	143.0
125.80	107.0
127.90	264.0
128.90	154.0
129.90	280.0
130.70	139.0
132.10	63.0
132.90	527.0
133.90	149.0
134.70	147.0
137.00	97.0
139.90	58.0
141.00	566.0
141.80	116.0
142.90	628.0
144.90	110.0
145.70	101.0
146.80	145.0
147.70	228.0
149.90	84.0
152.70	61.0
153.80	56.0
154.90	185.0
156.90	205.0
158.90	88.0
161.00	180.0

Instrument :
MSVOA_W
ClientSampleId :
BFB424

164.90	86.0
171.90	396.0
174.00	66752.0
174.90	5368.0
176.00	61608.0
177.00	4023.0
178.00	180.0
179.00	104.0
190.90	294.0
191.80	84.0
192.00	86.0
193.00	487.0
193.90	108.0
204.80	78.0
207.00	298.0
207.90	105.0
249.00	382.0
250.10	74.0
251.10	129.0
265.00	272.0
266.00	115.0
267.00	54.0
281.00	5340.0
282.10	1357.0
283.00	1033.0
283.90	188.0
285.00	56.0

Instrument :
MSVOA_W
ClientSampleId :
BFB424

m/z	Abundance
36.10	521.0
37.00	3618.0
38.00	3165.0
39.00	1218.0
39.90	186.0
40.90	85.0
42.90	72.0
44.00	599.0
45.00	658.0
47.00	953.0
48.00	554.0
49.00	3694.0
50.00	14718.0
51.10	4759.0
52.10	208.0
55.10	212.0
56.00	1428.0
57.00	2327.0
58.00	99.0
59.10	52.0
60.00	809.0
61.00	4098.0
62.00	4678.0
63.10	3076.0
64.00	275.0
65.10	202.0
66.80	228.0
68.00	9123.0
69.00	8882.0
70.00	574.0
72.00	505.0
73.00	4296.0
74.00	15507.0
75.10	44952.0
76.00	3690.0
76.90	626.0
78.00	529.0
78.90	2453.0
80.00	711.0
81.00	2476.0
82.00	507.0
83.00	84.0
85.90	138.0
87.00	4235.0
87.90	4264.0
91.00	397.0
92.00	2456.0
93.00	3727.0
94.00	10745.0
95.00	92264.0
96.00	5920.0
97.10	189.0
102.90	92.0
103.90	449.0
104.90	169.0
106.00	350.0
107.00	104.0
110.10	69.0
111.90	53.0
112.90	82.0
114.90	165.0
116.00	401.0
116.90	606.0
117.90	417.0
118.90	364.0
123.70	52.0
125.10	199.0
125.70	53.0
127.90	401.0
129.00	133.0
129.90	416.0
130.90	125.0
133.00	293.0
134.10	62.0
135.00	120.0
136.90	206.0
139.90	70.0
140.90	721.0
142.00	136.0
142.90	742.0
145.00	182.0
145.90	157.0
146.90	133.0
147.90	277.0
149.90	116.0
152.80	60.0
154.90	176.0
155.90	74.0
156.90	170.0
159.00	92.0
160.90	103.0
170.60	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB424

172.00	384.0
174.00	75336.0
174.90	5414.0
175.90	80336.0
176.90	4878.0
178.00	182.0
178.90	67.0
191.00	224.0
192.00	70.0
192.80	201.0
193.90	62.0
206.90	202.0
207.90	88.0
249.00	227.0
251.00	113.0
264.90	199.0
266.00	101.0
281.00	4281.0
281.90	882.0
283.10	540.0

Instrument :
MSVOA_W
ClientSampleId :
BFB424

m/z	Abundance
36.00	419.0
37.00	2771.0
38.00	2122.0
39.00	991.0
40.00	164.0
40.80	79.0
42.90	55.0
44.00	399.0
45.00	492.0
47.00	703.0
47.90	342.0
49.10	2269.0
50.10	11698.0
51.10	3593.0
52.10	123.0
55.10	196.0
56.00	1123.0
57.00	1721.0
60.00	737.0
61.00	2894.0
62.10	2934.0
63.00	2432.0
64.10	202.0
65.10	244.0
67.00	227.0
68.00	6922.0
69.00	6788.0
70.00	533.0
72.00	500.0
73.00	3302.0
74.00	11965.0
75.00	33632.0
76.00	2831.0
77.00	583.0
78.00	250.0
79.00	1915.0
80.00	590.0
80.90	1936.0
81.90	464.0
85.80	78.0
86.90	3216.0
87.90	3098.0
91.00	330.0
92.00	1959.0
93.00	3306.0
94.00	8703.0
95.00	76536.0
96.00	5029.0
97.00	173.0
103.90	322.0
104.90	90.0
105.90	284.0
107.00	66.0
110.70	77.0
111.90	86.0
112.90	52.0
114.90	70.0
115.80	168.0
117.00	449.0
117.90	207.0
118.90	439.0
124.90	114.0
127.90	247.0
128.90	100.0
129.90	239.0
131.00	92.0
133.50	51.0
134.80	102.0
136.90	165.0
139.90	55.0
140.90	561.0
141.80	77.0
142.90	665.0
143.80	73.0
144.70	62.0
146.00	127.0
147.00	83.0
147.80	165.0
155.00	179.0
155.90	93.0
156.90	138.0
158.70	99.0
160.90	98.0
172.00	250.0
173.90	73888.0
175.00	5124.0
175.90	67704.0
177.00	4170.0
177.90	117.0
190.90	111.0
191.90	76.0
193.00	70.0

Instrument :
MSVOA_W
ClientSampleId :
BFB424

206.90	114.0
249.00	102.0
250.90	76.0
265.10	106.0
281.00	1381.0
282.10	366.0
283.00	180.0

Instrument :
MSVOA_W
ClientSampleId :
BFB424