

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010924\
 Data File : VW027843.D
 Acq On : 09 Jan 2024 13:16
 Operator : SY/MD
 Sample : P1017-06
 Misc : 4.16g/10mL/MSVOA_W/SOIL/Vial B
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCMH7

Quant Time: Jan 10 00:43:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 10 00:40:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	528856	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	494123	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	239440	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	108308	16.780	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.120%
7) Chloroethane-d5	2.899	69	94013	16.613	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.440%
11) 1,1-Dichloroethene-d2	4.021	65	47719	16.434	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.720%
21) 2-Butanone-d5	7.088	46	47397	44.406	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.820%
24) Chloroform-d	7.648	84	229041	17.910	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	71.640%
26) 1,2-Dichloroethane-d4	8.307	65	114544	19.770	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.080%
32) Benzene-d6	8.270	84	499423	17.808	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	71.240%
36) 1,2-Dichloropropane-d6	9.270	67	141692	18.262	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	73.040%
41) Toluene-d8	10.319	98	467852	17.845	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	71.360%
43) trans-1,3-Dichloroprop...	10.575	79	56744	18.815	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.280%
47) 2-Hexanone-d5	10.922	63	45892	45.062	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.120%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	112618	20.375	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.520%
66) 1,2-Dichlorobenzene-d4	13.849	152	169383	20.124	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.480%
Target Compounds					Qvalue	
13) Acetone	4.155	43	15864	11.629	ug/L	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010924\
Data File : VW027843.D
Acq On : 09 Jan 2024 13:16
Operator : SY/MD
Sample : P1017-06
Misc : 4.16g/10mL/MSVOA_W/SOIL/Vial B
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DCMH7

Quant Time: Jan 10 00:43:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 10 00:40:17 2024
Response via : Initial Calibration

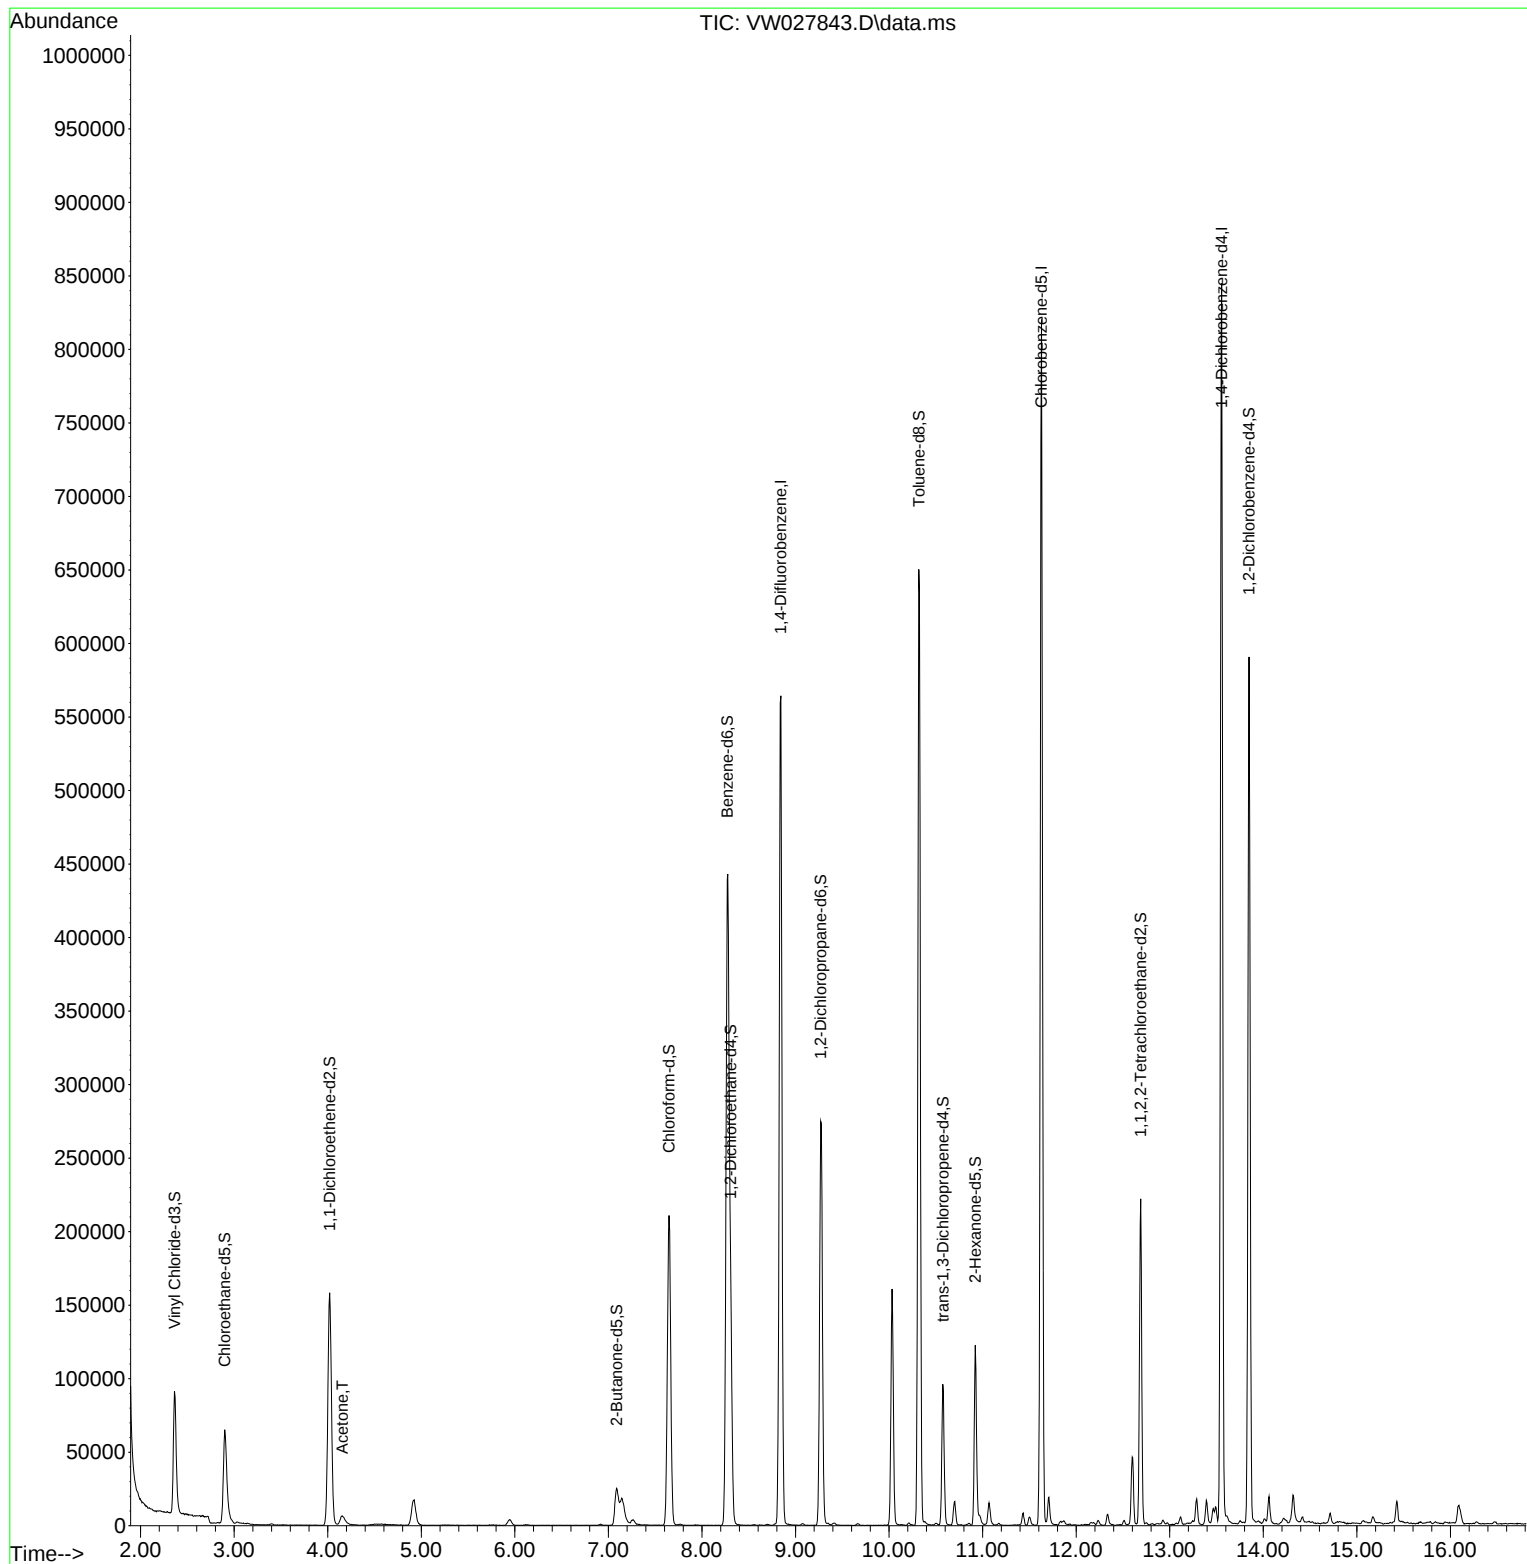

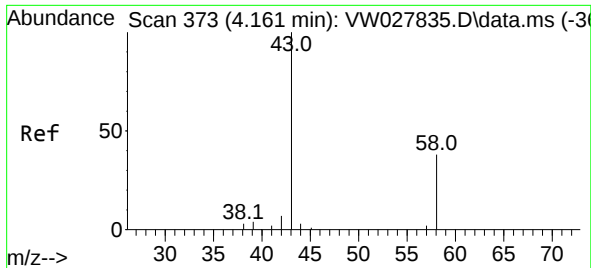

#13
 Acetone
 Concen: 11.629 ug/L
 RT: 4.155 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VW027843.D
 Acq: 09 Jan 2024 13:16

Instrument :
 MSVOA_W
 ClientSampleId :
 DCMH7

Tgt Ion: 43 Resp: 15864

Ion	Ratio	Lower	Upper
43	100		
58	11.8	0.0	70.2

