

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011022\
 Data File : VW0217804.D
 Acq On : 10 Jan 2022 09:14
 Operator : SY/VA
 Sample : VW0110SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jan 10 12:18:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 22:46:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	123309	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	122950	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	68545	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	49822	20.492	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.960%
7) Chloroethane-d5	2.885	69	35465	21.658	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.640%
11) 1,1-Dichloroethene-d2	4.019	63	64624	18.164	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.640%
21) 2-Butanone-d5	7.080	46	19646	55.233	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.460%
24) Chloroform-d	7.653	84	95153	24.703	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.800%
26) 1,2-Dichloroethane-d4	8.311	65	50082	24.623	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.480%
32) Benzene-d6	8.275	84	191906	26.287	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.160%
36) 1,2-Dichloropropane-d6	9.275	67	51141	25.823	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.280%
41) Toluene-d8	10.323	98	187042	25.714	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	102.840%
43) trans-1,3-Dichloroprop...	10.579	79	20867	21.653	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.600%
47) 2-Hexanone-d5	10.927	63	16478	54.862	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.720%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	44276	27.118	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.480%
66) 1,2-Dichlorobenzene-d4	13.853	152	72644	27.714	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.840%
Target Compounds						
					Qvalue	
34) Trichloroethene	8.842	95	3418	1.605	ug/L #	5
37) 1,2-Dichloropropane	9.275	63	6234	3.750	ug/L #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011022\
Data File : VW0217804.D
Acq On : 10 Jan 2022 09:14
Operator : SY/VA
Sample : VW0110SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jan 10 12:18:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 07 22:46:04 2022
Response via : Initial Calibration

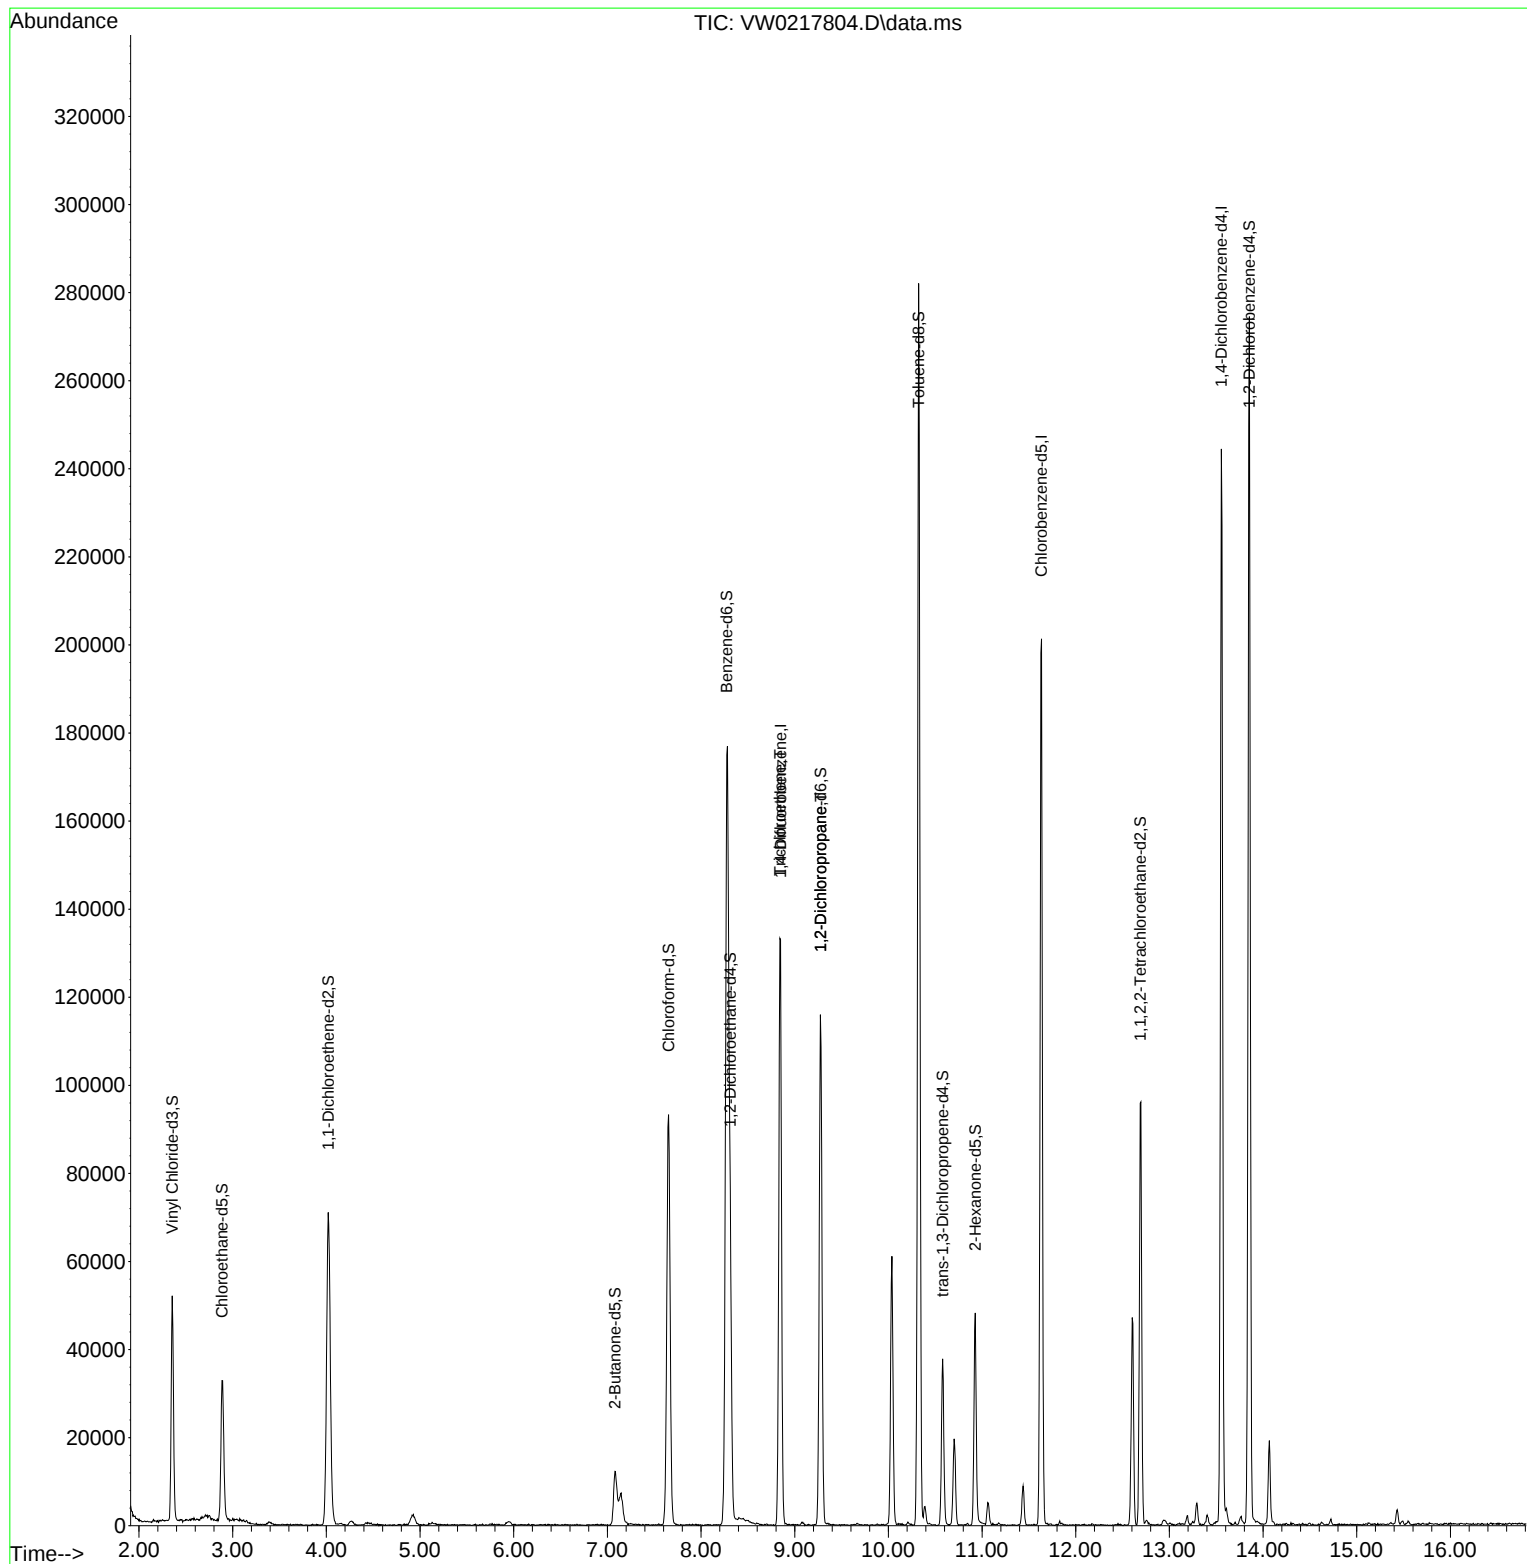



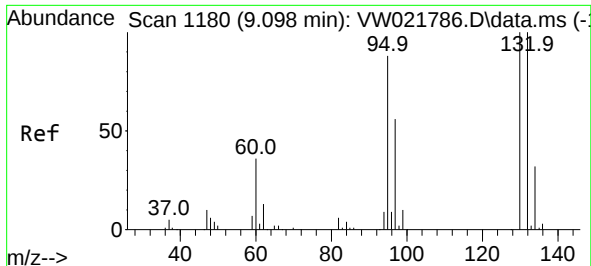


#34
 Trichloroethene
 Concen: 1.605 ug/L
 RT: 8.842 min Scan# 1180
 Delta R.T. -0.256 min
 Lab File: VW0217804.D
 Acq: 10 Jan 2022 09:14

Instrument :
 MSVOA_W
 ClientSampleId :

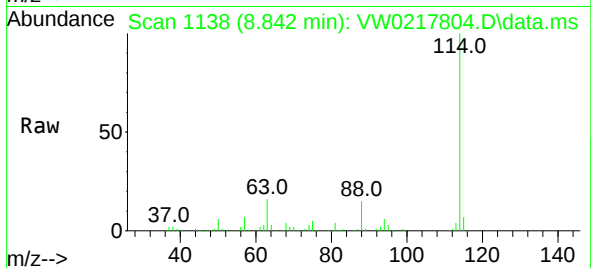

Tgt Ion: 95 Resp: 3418
 Ion Ratio Lower Upper
 95 100
 97 0.0 47.0 87.2#
 132 0.0 65.5 121.6#
 130 0.0 69.4 128.8#

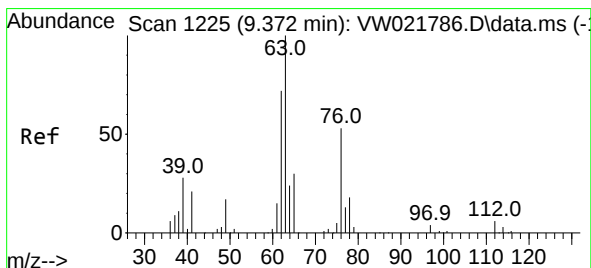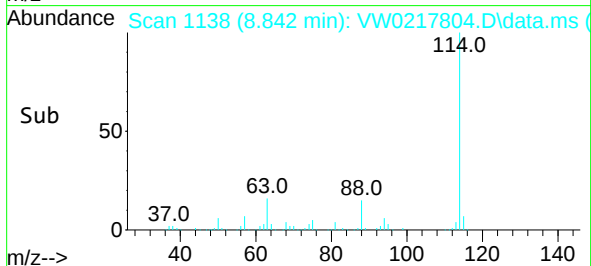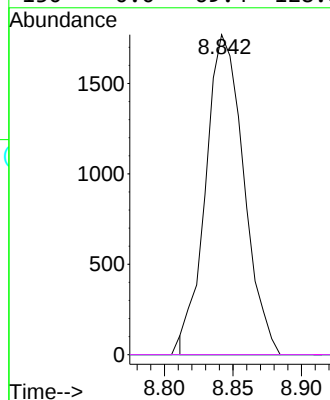

#37
 1,2-Dichloropropane
 Concen: 3.750 ug/L
 RT: 9.275 min Scan# 1209
 Delta R.T. -0.098 min
 Lab File: VW0217804.D
 Acq: 10 Jan 2022 09:14

Tgt Ion: 63 Resp: 6234
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.2 4.8#

