

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011022\
 Data File : VW021809.D
 Acq On : 10 Jan 2022 11:13
 Operator : SY/VA
 Sample : N1074-17
 Misc : 7.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLM0

Manual IntegrationsAPPROVED

Quant Time: Jan 10 12:48:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 22:46:04 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/11/2022
 Supervised By :Mahesh Dadoda 01/12/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	169698	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	166905	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	91618	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	46871	14.009	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.040%
7) Chloroethane-d5	2.885	69	35421	15.718	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.880%
11) 1,1-Dichloroethene-d2	4.019	63	64583	13.190	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.760%
21) 2-Butanone-d5	7.080	46	19904m	40.661	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.320%
24) Chloroform-d	7.653	84	102225	19.284	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.120%
26) 1,2-Dichloroethane-d4	8.305	65	53177	18.998	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	76.000%
32) Benzene-d6	8.275	84	206507	20.837	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.360%
36) 1,2-Dichloropropane-d6	9.274	67	55562	20.667	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.680%
41) Toluene-d8	10.323	98	203712	20.631	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.520%
43) trans-1,3-Dichloroprop...	10.579	79	23377	17.870	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.480%
47) 2-Hexanone-d5	10.927	63	17383	42.634	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.260%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	46456	20.960	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.840%
66) 1,2-Dichlorobenzene-d4	13.853	152	81731	23.328	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.320%

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011022\
Data File : VW0217809.D
Acq On : 10 Jan 2022 11:13
Operator : SY/VA
Sample : N1074-17
Misc : 7.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLM0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/11/2022
Supervised By :Mahesh Dadoda 01/12/2022

Quant Time: Jan 10 12:48:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 07 22:46:04 2022
Response via : Initial Calibration

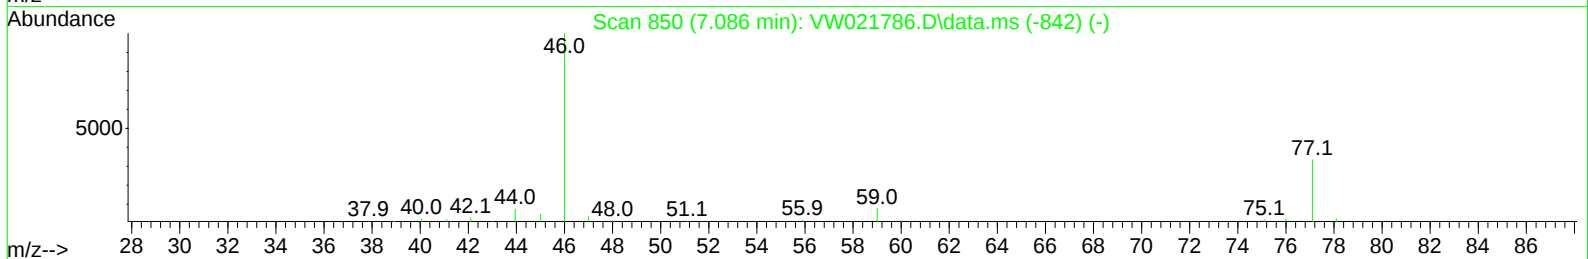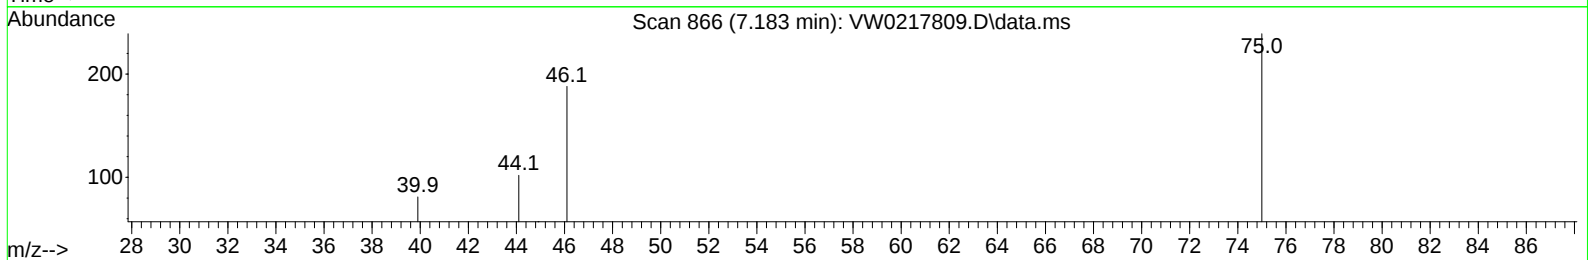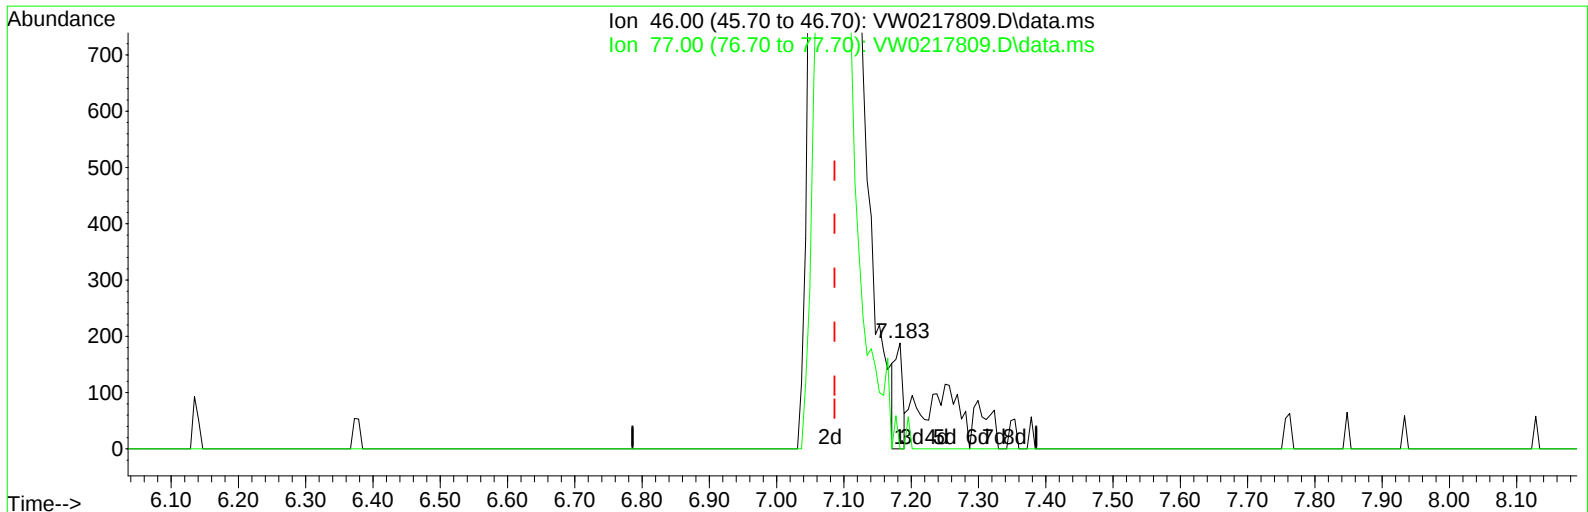

TIC: VW0217809.D\data.ms

(21) 2-Butanone-d5 (S)

7.183min (+ 0.097) 0.31 ug/L

response 150

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	14.67
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011022\
 Data File : VW0217809.D
 Acq On : 10 Jan 2022 11:13
 Operator : SY/VA
 Sample : N1074-17
 Misc : 7.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLM0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/11/2022
 Supervised By :Mahesh Dadoda 01/12/2022

Quant Time: Jan 10 12:48:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 22:46:04 2022
 Response via : Initial Calibration

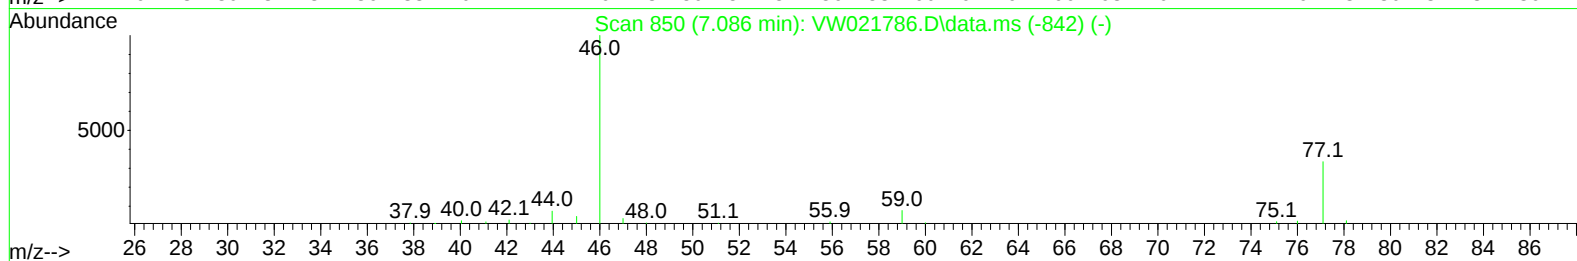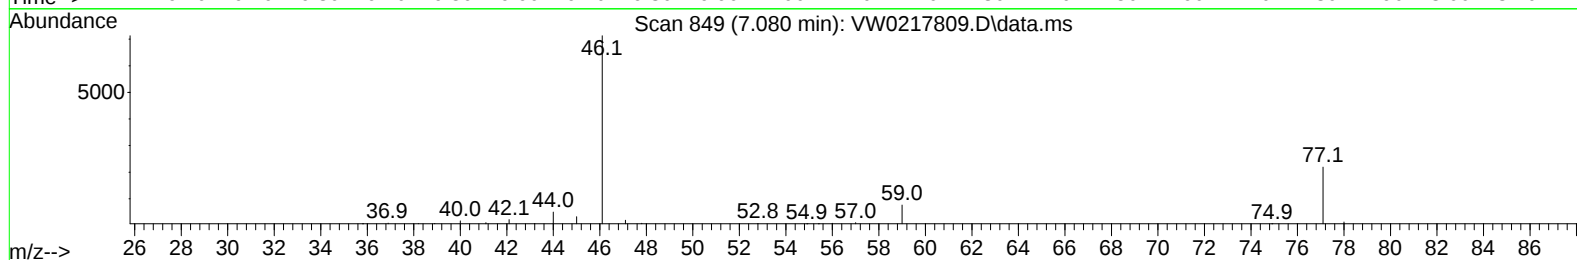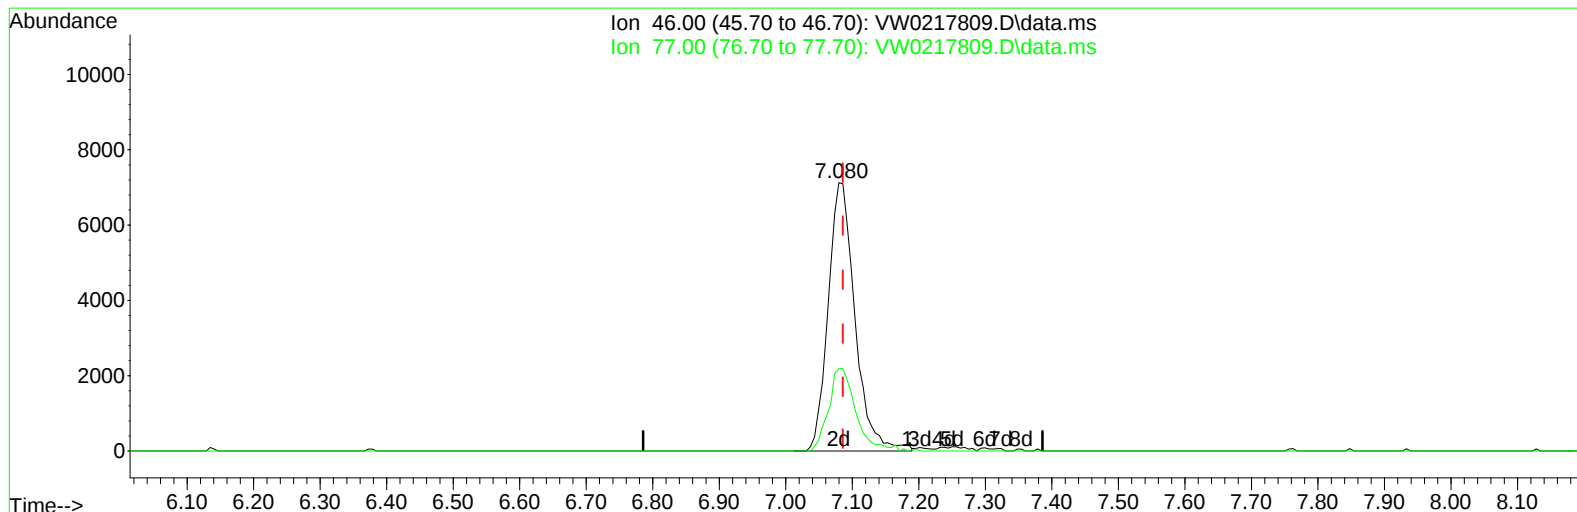

TIC: VW0217809.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (-0.006) 40.66 ug/L m

response 19904

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	0.11#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011022\
Data File : VW021809.D
Acq On : 10 Jan 2022 11:13
Operator : SY/VA
Sample : N1074-17
Misc : 7.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLM0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/11/2022
Supervised By :Mahesh Dadoda 01/12/2022

Quant Time: Jan 10 12:48:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 07 22:46:04 2022
Response via : Initial Calibration

