

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011022\
 Data File : VW021816.D
 Acq On : 10 Jan 2022 14:01
 Operator : SY/VA
 Sample : N1053-22
 Misc : 7.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLJ9

Quant Time: Jan 11 00:19:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 22:46:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	186606	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	185076	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	103517	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	48039	13.057	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.240%
7) Chloroethane-d5	2.885	69	36199	14.608	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.440%
11) 1,1-Dichloroethene-d2	4.019	63	65729	12.208	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	48.840%
21) 2-Butanone-d5	7.080	46	21317	39.602	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.200%
24) Chloroform-d	7.653	84	108623	18.635	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.520%
26) 1,2-Dichloroethane-d4	8.305	65	55457	18.017	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	72.080%
32) Benzene-d6	8.275	84	215746	19.632	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	78.520%
36) 1,2-Dichloropropane-d6	9.274	67	58689	19.687	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	78.760%
41) Toluene-d8	10.323	98	217507	19.865	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.440%
43) trans-1,3-Dichloroprop...	10.579	79	24069	16.592	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.360%
47) 2-Hexanone-d5	10.927	63	19302	42.692	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.380%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	48694	19.812	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	83093	20.991	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.960%
Target Compounds						
13) Acetone	4.135	43	1378	3.015	ug/L	Qvalue 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011022\
Data File : VW021816.D
Acq On : 10 Jan 2022 14:01
Operator : SY/VA
Sample : N1053-22
Misc : 7.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLJ9


Quant Time: Jan 11 00:19:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 07 22:46:04 2022
Response via : Initial Calibration

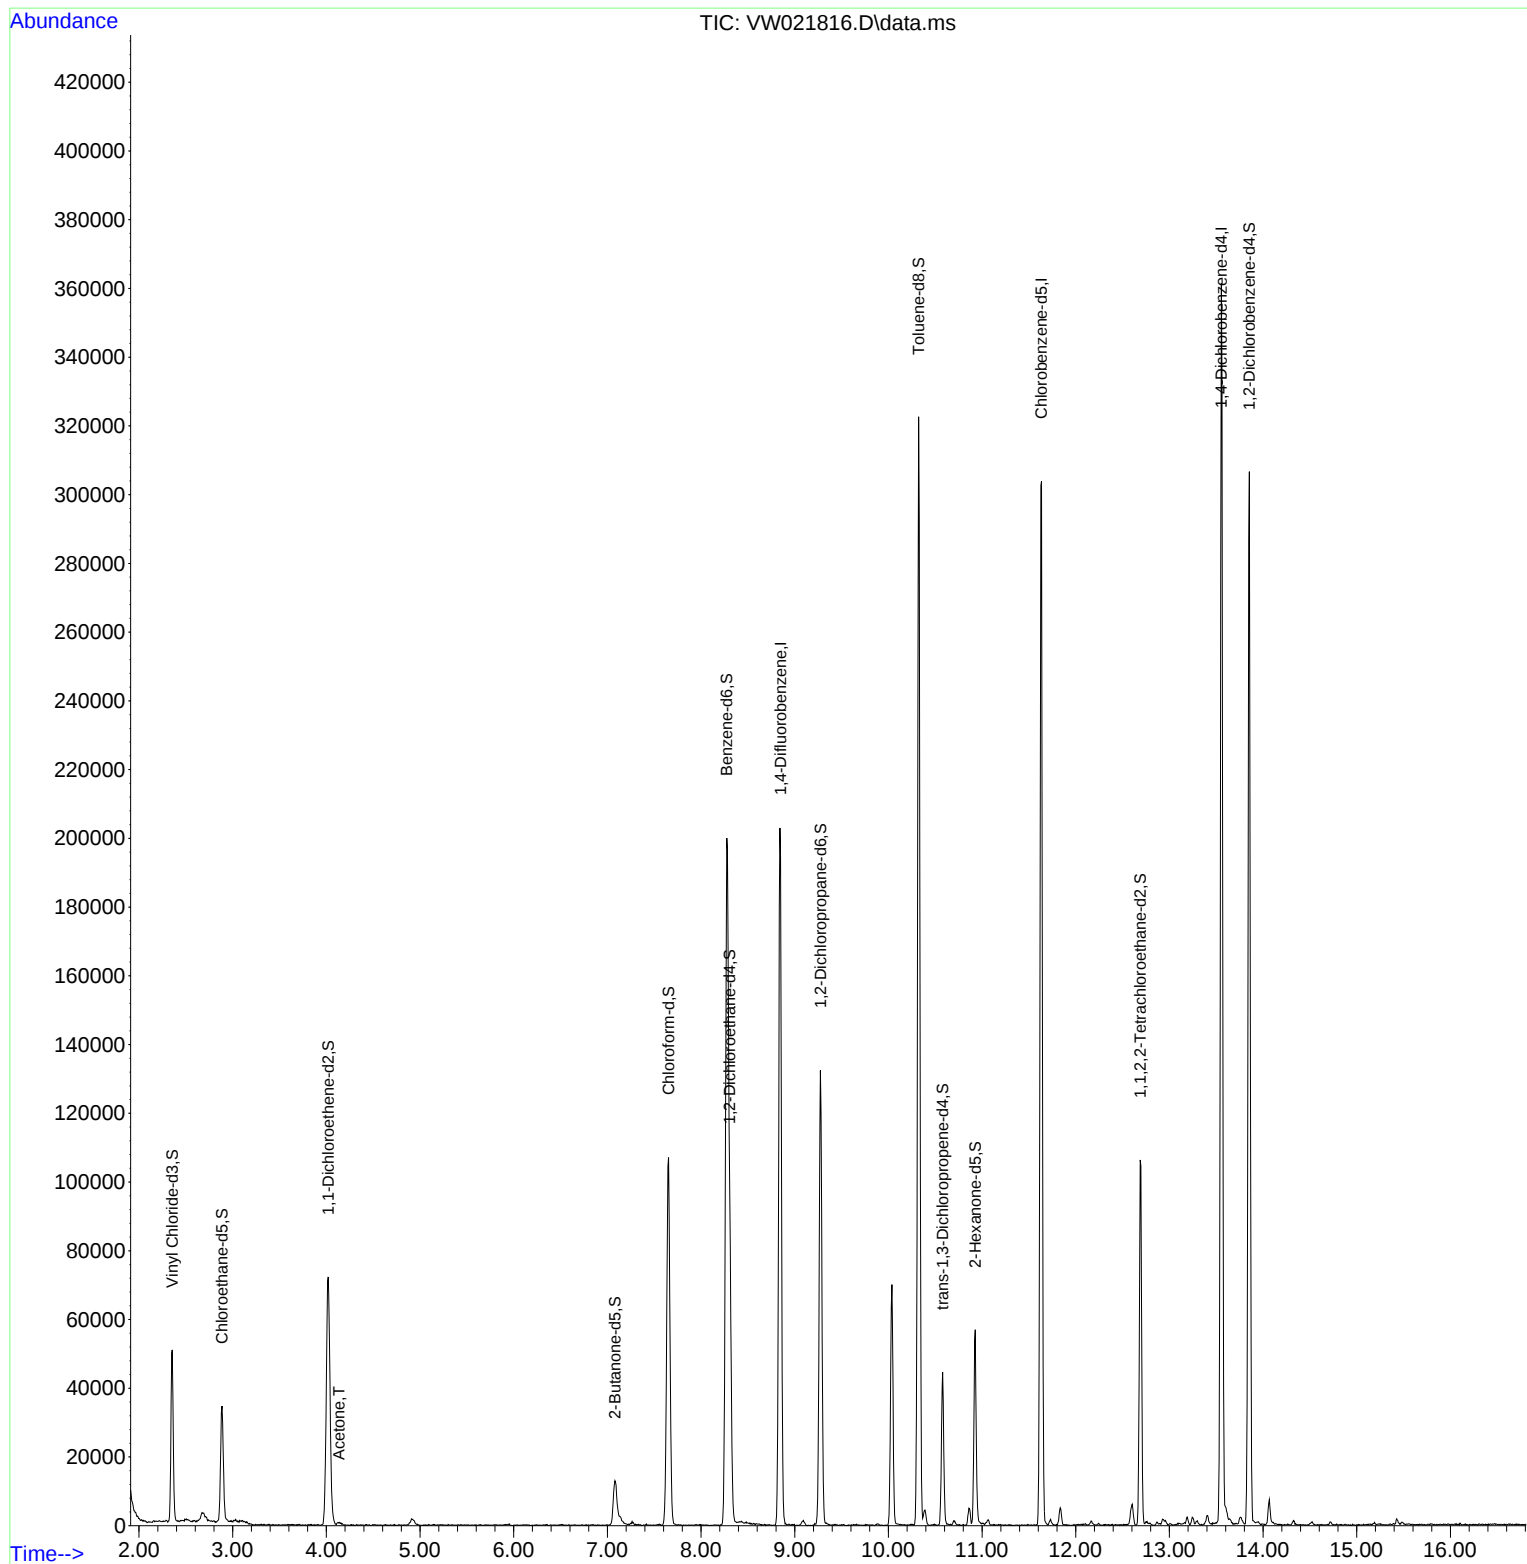

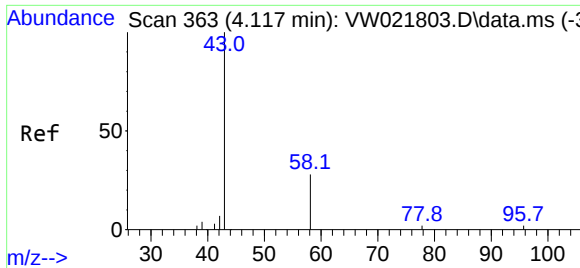

#13
 Acetone
 Concen: 3.015 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. -0.012 min
 Lab File: VW021816.D
 Acq: 10 Jan 2022 14:01

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLJ9

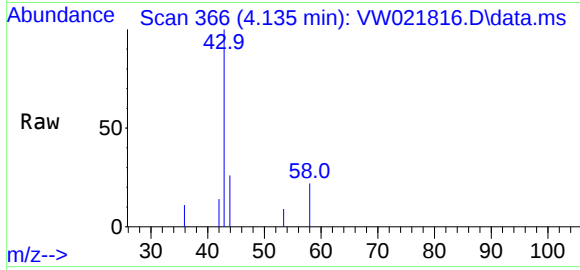

Tgt Ion: 43 Resp: 1378
 Ion Ratio Lower Upper
 43 100
 58 11.5 0.0 52.8

