

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011022\
 Data File : VW021819.D
 Acq On : 10 Jan 2022 15:13
 Operator : SY/VA
 Sample : N1053-18RE
 Misc : 6.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLJ5RE

Quant Time: Jan 11 00:20:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 07 22:46:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	97633	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	76694	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	21958	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	34150	17.740	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.960%
7) Chloroethane-d5	2.885	69	26758	20.638	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.560%
11) 1,1-Dichloroethene-d2	4.013	63	42335	15.028	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.120%
21) 2-Butanone-d5	7.080	46	23241	82.523	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	165.040%#
24) Chloroform-d	7.653	84	70766	23.203	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.800%
26) 1,2-Dichloroethane-d4	8.311	65	40455	25.121	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.480%
32) Benzene-d6	8.275	84	134921	29.627	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	118.520%
36) 1,2-Dichloropropane-d6	9.274	67	38327	31.025	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	124.080%#
41) Toluene-d8	10.323	98	114233	25.177	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.720%
43) trans-1,3-Dichloroprop...	10.579	79	12944	21.533	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.120%
47) 2-Hexanone-d5	10.920	63	17462	93.203	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	186.400%#
56) 1,1,2,2-Tetrachloroeth...	12.695	84	33095	32.495	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	129.960%#
66) 1,2-Dichlorobenzene-d4	13.853	152	20537	24.458	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.840%
Target Compounds						
13) Acetone	4.135	43	4174	17.455	ug/L	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011022\
Data File : VW021819.D
Acq On : 10 Jan 2022 15:13
Operator : SY/VA
Sample : N1053-18RE
Misc : 6.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLJ5RE


Quant Time: Jan 11 00:20:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 07 22:46:04 2022
Response via : Initial Calibration

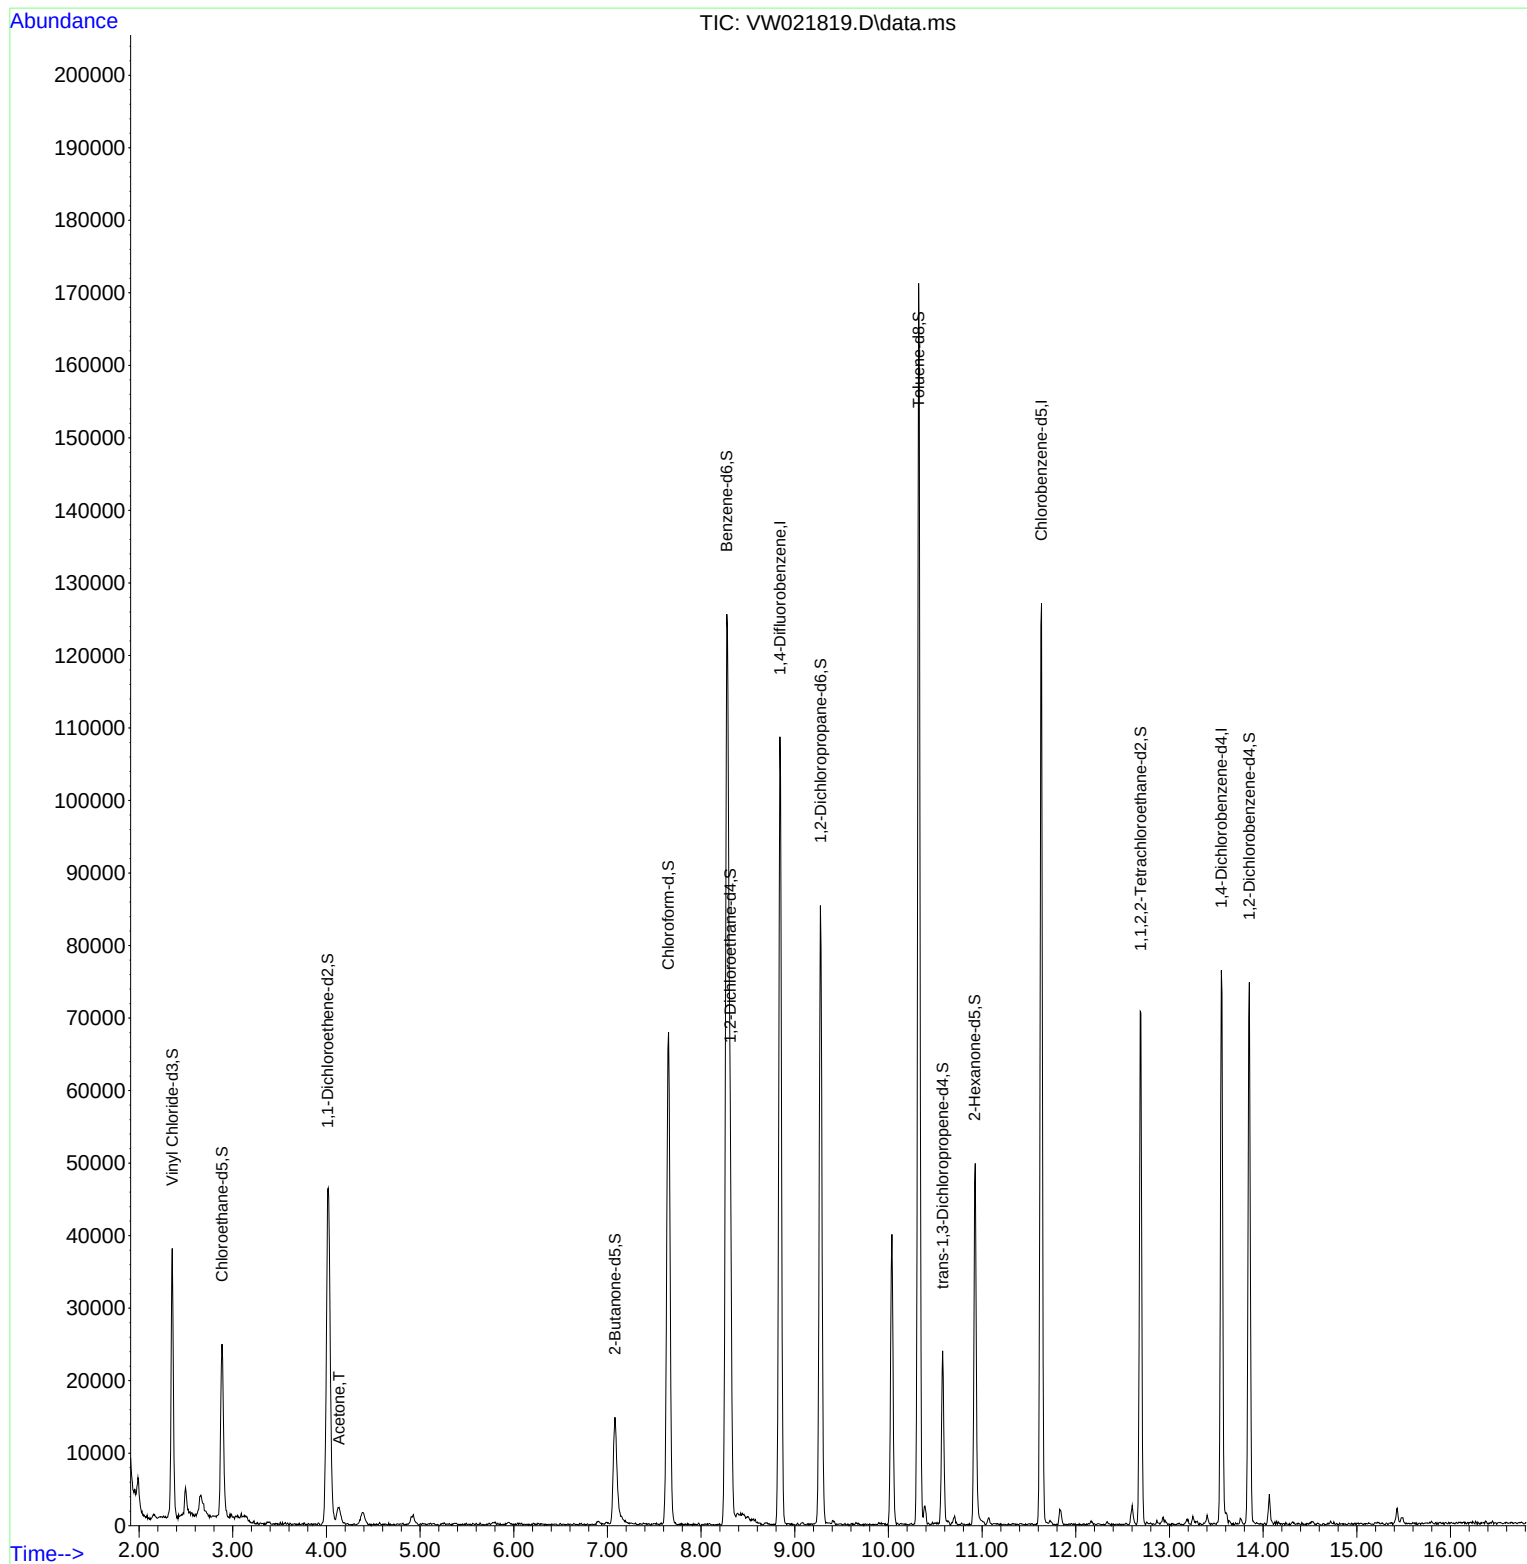

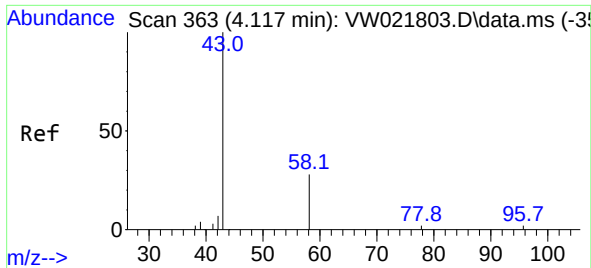

#13
 Acetone
 Concen: 17.455 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. -0.012 min
 Lab File: VW021819.D
 Acq: 10 Jan 2022 15:13

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLJ5RE

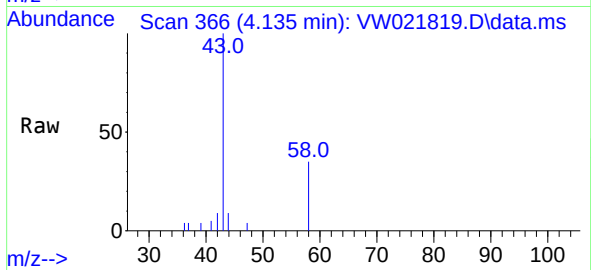

Tgt Ion: 43 Resp: 4174
 Ion Ratio Lower Upper
 43 100
 58 34.5 0.0 52.8

