


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011022\
 Data File : VW021802.D
 Acq On : 10 Jan 2022 07:53
 Operator : SY/VA
 Sample : BFB496
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB496

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Title : SFAM01.0
 Last Update : Fri Jan 07 22:46:04 2022

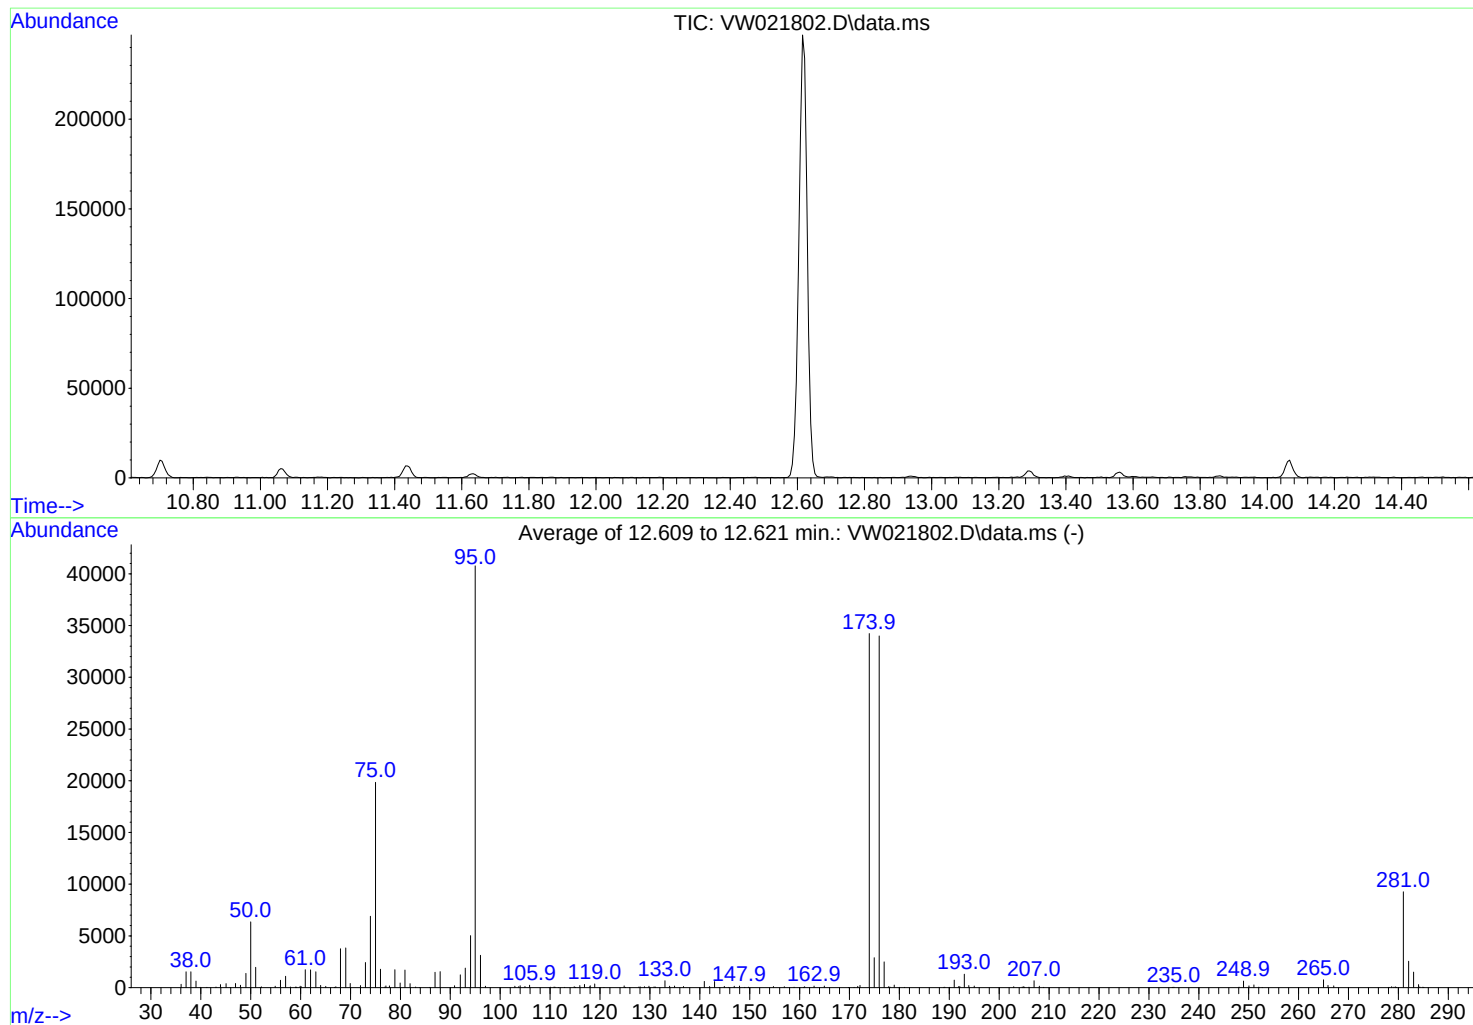

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	6350	PASS
75	95	30	80	48.7	19845	PASS
95	95	100	100	100.0	40773	PASS
96	95	5	9	7.6	3118	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.9	34224	PASS
175	174	5	9	8.4	2890	PASS
176	174	95	105	99.3	33992	PASS
177	176	5	10	7.3	2487	PASS

m/z	Abundance
36.00	339.0
37.10	1582.0
38.00	1488.0
39.00	750.0
39.80	94.0
43.10	93.0
43.90	285.0
45.10	361.0
45.90	56.0
47.00	365.0
47.80	220.0
49.10	1332.0
50.00	6325.0
51.00	1926.0
52.20	127.0
55.00	212.0
56.00	688.0
57.00	1118.0
57.90	123.0
60.10	330.0
61.00	1680.0
62.00	2023.0
63.00	1649.0
64.10	251.0
65.00	108.0
67.10	135.0
68.00	3748.0
69.00	4104.0
70.00	391.0
72.10	163.0
73.00	2483.0
74.00	7046.0
75.00	20896.0
76.00	1721.0
77.10	273.0
77.90	165.0
78.90	1795.0
80.00	506.0
80.90	1839.0
81.90	470.0
82.90	59.0
86.90	1709.0
87.90	1671.0
90.90	208.0
92.00	1300.0
93.00	1965.0
94.00	5372.0
95.00	44424.0
96.00	3339.0
97.10	151.0
103.00	66.0
104.00	268.0
105.00	136.0
105.90	248.0
111.00	122.0
112.90	61.0
114.90	117.0
115.90	214.0
117.00	324.0
118.00	279.0
118.90	328.0
125.10	101.0
127.70	103.0
128.00	105.0
128.80	145.0
129.90	152.0
130.90	137.0
133.10	446.0
133.90	50.0
135.00	146.0
136.70	124.0
140.90	704.0
141.90	125.0
142.90	703.0
143.90	61.0
144.90	115.0
145.80	102.0
146.80	104.0
148.00	173.0
149.00	80.0
149.80	69.0
154.80	139.0
156.90	79.0
158.90	79.0
161.00	109.0
163.00	106.0
170.90	103.0
172.00	312.0
173.90	39056.0
174.90	3221.0
175.90	40512.0
176.90	2684.0

Instrument :
MSVOA_W
ClientSampleId :
BFB496

177.90	116.0
178.90	133.0
191.00	362.0
192.10	143.0
192.90	618.0
194.00	127.0
194.90	94.0
202.90	66.0
205.10	132.0
207.00	354.0
208.00	126.0
235.00	53.0
248.80	348.0
250.20	79.0
250.90	206.0
264.90	428.0
266.00	124.0
267.00	105.0
279.60	98.0
281.00	5803.0
282.00	1450.0
283.00	982.0
284.30	170.0

Instrument :
MSVOA_W
ClientSampleId :
BFB496

m/z	Abundance
36.10	362.0
37.00	1698.0
38.00	1711.0
39.10	723.0
39.90	110.0
41.20	71.0
43.00	80.0
44.00	284.0
45.00	377.0
47.00	451.0
48.00	191.0
49.10	1452.0
50.00	6984.0
51.00	2289.0
52.10	107.0
54.80	114.0
56.00	831.0
57.00	1258.0
58.00	74.0
59.20	145.0
59.90	251.0
61.00	2194.0
62.00	1842.0
63.00	1674.0
63.90	250.0
65.00	145.0
67.00	165.0
68.00	4248.0
69.10	4107.0
70.00	423.0
72.00	305.0
73.00	2565.0
74.00	7533.0
75.00	22112.0
76.00	2167.0
77.10	247.0
77.80	250.0
78.90	1968.0
79.90	416.0
80.90	1916.0
81.90	405.0
83.10	57.0
85.90	77.0
87.00	1633.0
88.00	1856.0
90.90	200.0
92.00	1429.0
93.00	2015.0
94.10	5668.0
95.00	45328.0
96.00	3279.0
97.10	178.0
102.80	110.0
104.00	282.0
104.80	106.0
105.90	263.0
110.00	72.0
110.80	116.0
115.10	101.0
116.00	157.0
116.80	296.0
118.10	265.0
118.90	399.0
120.80	50.0
124.80	186.0
125.90	63.0
128.10	137.0
129.00	78.0
129.80	132.0
130.80	82.0
131.10	87.0
132.90	546.0
133.80	132.0
134.90	135.0
136.70	119.0
140.90	718.0
141.90	97.0
143.00	576.0
144.90	174.0
146.90	152.0
148.00	137.0
149.70	65.0
154.70	107.0
156.90	115.0
158.90	72.0
161.00	148.0
162.80	137.0
164.80	169.0
169.80	58.0
171.60	188.0
172.20	335.0
174.00	39184.0

Instrument :
MSVOA_W
ClientSampleId :
BFB496

175.00	3476.0
175.90	37160.0
177.00	2725.0
177.80	141.0
179.00	306.0
189.10	124.0
191.00	809.0
192.10	166.0
193.00	1246.0
193.90	163.0
195.10	126.0
202.90	105.0
204.60	178.0
206.00	53.0
207.00	667.0
208.10	120.0
235.00	104.0
248.10	73.0
249.00	776.0
250.10	210.0
251.10	311.0
252.00	72.0
265.00	830.0
265.80	145.0
267.10	181.0
278.70	141.0
279.10	141.0
281.10	9540.0
282.10	2711.0
283.00	1198.0
284.10	264.0
285.10	108.0

Instrument :
MSVOA_W
ClientSampleId :
BFB496

m/z	Abundance
36.10	266.0
37.00	1294.0
38.00	1386.0
39.10	443.0
40.00	50.0
43.90	314.0
45.00	408.0
46.90	376.0
48.00	278.0
49.00	1330.0
50.00	5740.0
51.00	1702.0
51.90	110.0
54.90	100.0
55.90	616.0
57.00	922.0
59.00	176.0
59.90	186.0
60.90	1303.0
62.00	1294.0
63.10	1274.0
64.00	142.0
65.10	114.0
66.80	79.0
68.00	3285.0
69.00	3308.0
69.90	393.0
71.90	156.0
73.00	2550.0
74.00	6107.0
75.00	16528.0
76.00	1428.0
76.90	213.0
77.70	99.0
78.90	1456.0
79.90	409.0
80.90	1373.0
82.00	285.0
83.10	56.0
83.90	54.0
86.90	1131.0
87.90	1139.0
90.80	137.0
92.00	985.0
93.00	1661.0
94.00	4054.0
95.00	32568.0
96.10	2735.0
97.00	73.0
103.00	254.0
103.70	263.0
105.00	110.0
105.90	168.0
109.80	64.0
110.10	71.0
110.80	86.0
111.70	56.0
112.90	53.0
114.80	185.0
115.90	232.0
116.90	297.0
117.90	239.0
119.00	350.0
120.00	53.0
124.90	348.0
127.90	98.0
128.90	76.0
129.70	116.0
131.10	84.0
133.00	1005.0
134.00	240.0
135.00	206.0
136.80	80.0
140.90	374.0
142.00	95.0
143.00	474.0
144.90	84.0
147.00	156.0
147.90	164.0
154.80	82.0
157.00	66.0
160.80	103.0
162.90	226.0
165.00	291.0
171.70	205.0
173.90	24432.0
174.90	1974.0
176.00	24304.0
176.90	2051.0
178.10	202.0
178.90	290.0
180.00	108.0

Instrument :
MSVOA_W
ClientSampleId :
BFB496

181.00	81.0
188.90	106.0
190.10	95.0
191.00	988.0
191.90	335.0
193.00	2016.0
193.90	327.0
195.00	238.0
202.90	122.0
204.90	282.0
205.90	98.0
207.00	972.0
208.10	170.0
208.90	82.0
234.70	109.0
248.00	80.0
249.00	784.0
250.00	228.0
251.10	256.0
252.10	55.0
252.70	55.0
265.00	1012.0
265.90	381.0
267.00	232.0
278.10	104.0
278.60	147.0
279.40	247.0
281.00	12730.0
282.00	3520.0
283.10	2346.0
284.00	606.0
284.90	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB496

m/z	Abundance
40.00	61.0
44.20	95.0
73.00	103.0
280.90	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB496