

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011123\
 Data File : VW025222.D
 Acq On : 11 Jan 2023 13:00
 Operator : SY/MD
 Sample : VW0111SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK453

Quant Time: Jan 12 04:20:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 04 00:45:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	486758	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	422928	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	203906	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	125312	22.175	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.680%		
7) Chloroethane-d5	2.885	69	82773	23.247	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	93.000%		
11) 1,1-Dichloroethene-d2	4.013	63	221708	17.913	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	71.640%		
21) 2-Butanone-d5	7.080	46	66720	46.585	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.180%		
24) Chloroform-d	7.647	84	291420	23.887	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	95.560%		
26) 1,2-Dichloroethane-d4	8.305	65	152728	24.303	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	97.200%		
32) Benzene-d6	8.274	84	622131	24.497	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	98.000%		
36) 1,2-Dichloropropane-d6	9.274	67	181645	24.451	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	97.800%		
41) Toluene-d8	10.323	98	564799	24.436	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	97.760%		
43) trans-1,3-Dichloroprop...	10.579	79	76312	23.989	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	95.960%		
47) 2-Hexanone-d5	10.920	63	54389	46.462	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	92.920%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	113665	21.878	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	87.520%		
66) 1,2-Dichlorobenzene-d4	13.853	152	175487	24.222	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	96.880%		
Target Compounds					Qvalue	
34) Trichloroethene	8.841	95	15597	2.339	ug/L	# 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011123\
Data File : VW025222.D
Acq On : 11 Jan 2023 13:00
Operator : SY/MD
Sample : VW0111SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK453

Quant Time: Jan 12 04:20:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 04 00:45:59 2023
Response via : Initial Calibration

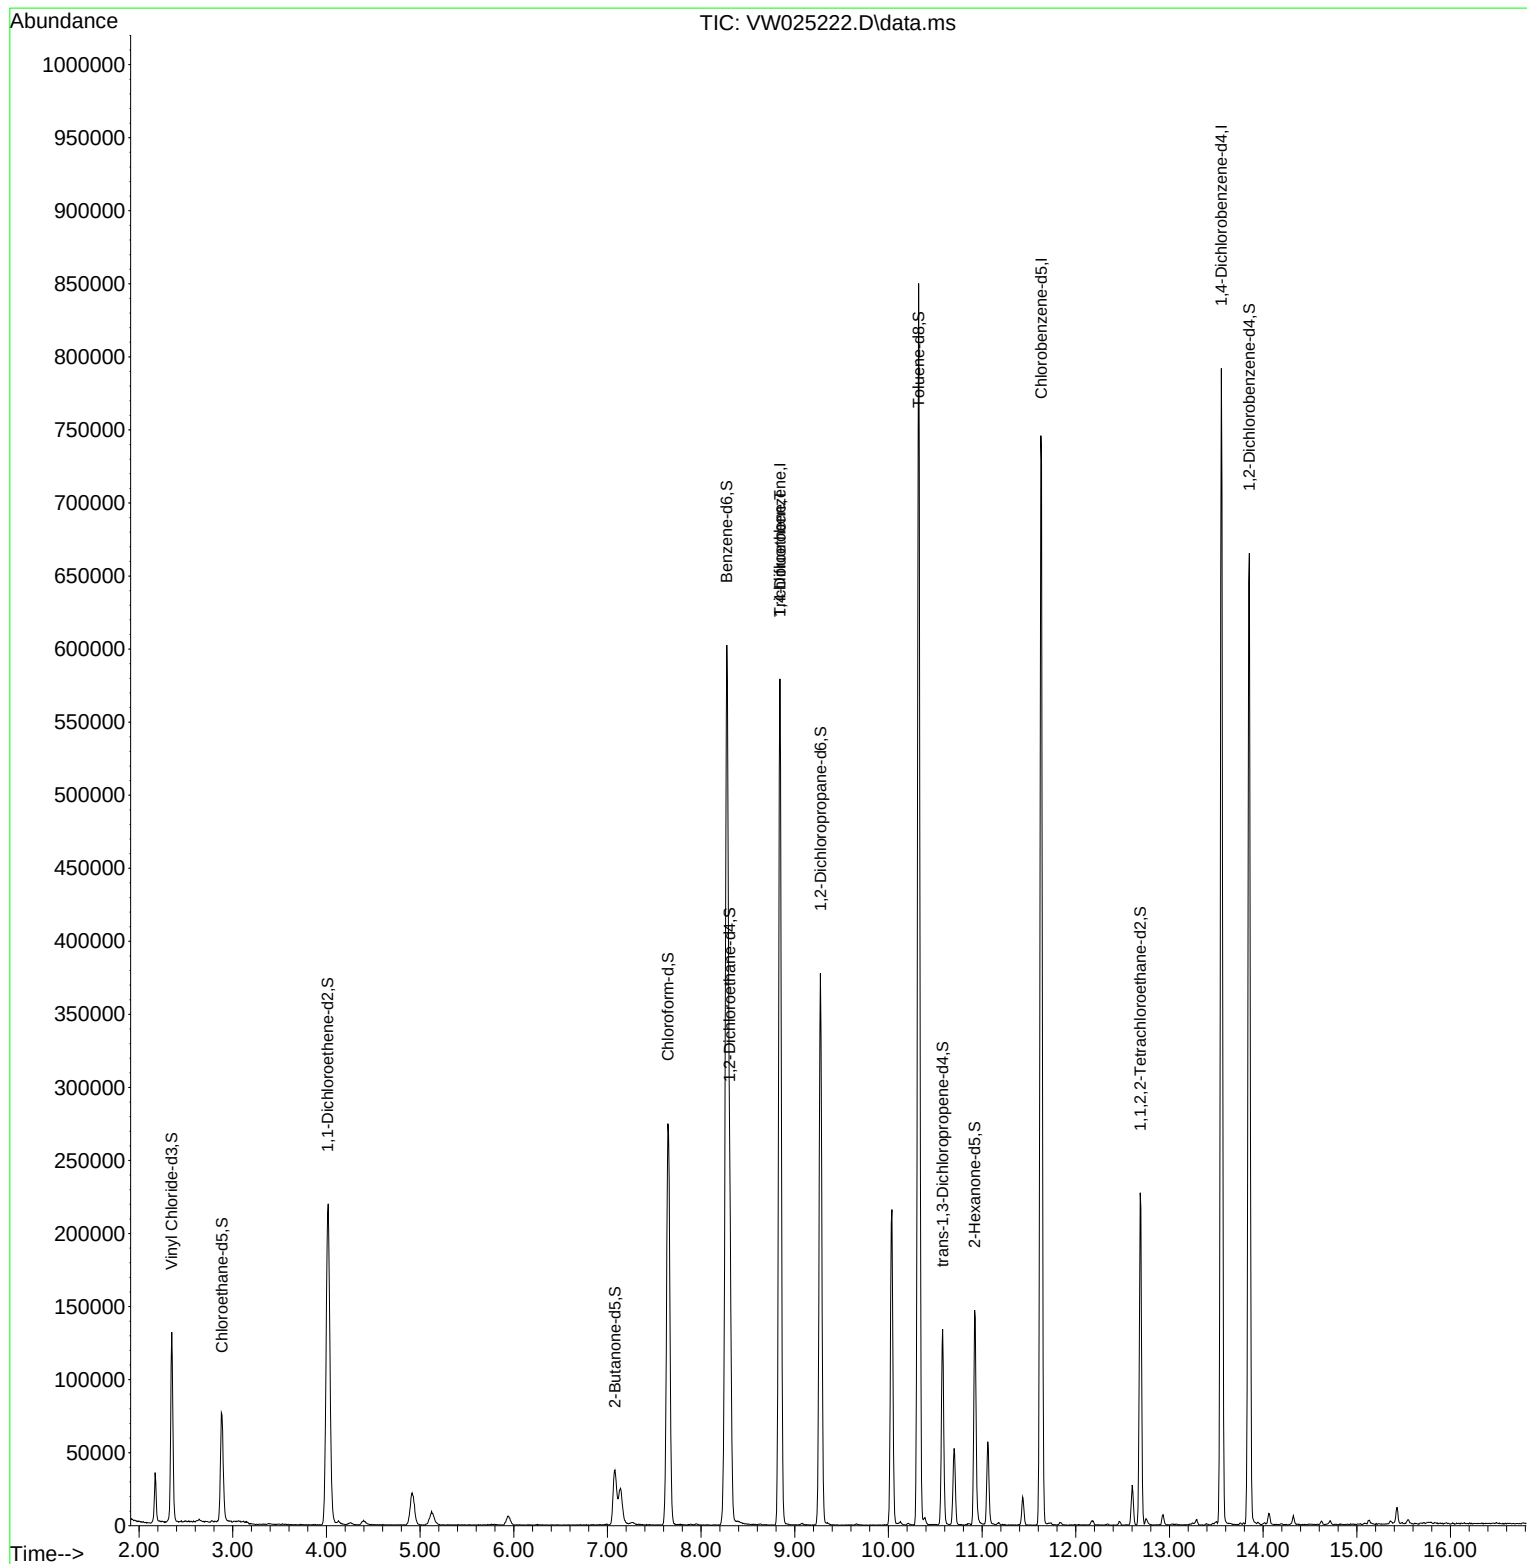

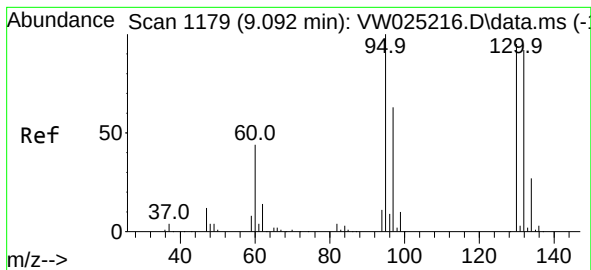

#34

Trichloroethene

Concen: 2.339 ug/L

RT: 8.841 min Scan# 11

Delta R.T. -0.250 min

Lab File: VW025222.D


Acq: 11 Jan 2023 13:00

Instrument :

MSVOA_W

ClientSampleId :

VBLK453

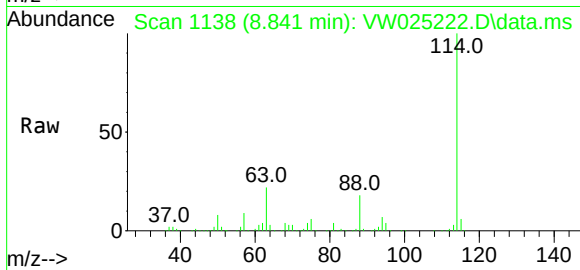

Tgt Ion: 95 Resp: 15597

Ion Ratio Lower Upper

95 100

97 0.0 44.4 82.4#

132 0.0 64.5 119.7#

130 0.0 66.8 124.0#

