

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011123\
Data File : VW025223.D
Acq On : 11 Jan 2023 13:35
Operator : SY/MD
Sample : 01120-01
Misc : 5.24g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C1141


Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/12/2023
Supervised By :Mahesh Dadoda 01/12/2023

Quant Time: Jan 12 04:20:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 04 00:45:59 2023
Response via : Initial Calibration

01/12/2023
Supervised By :Mahesh
Dadoda

01/12/2023

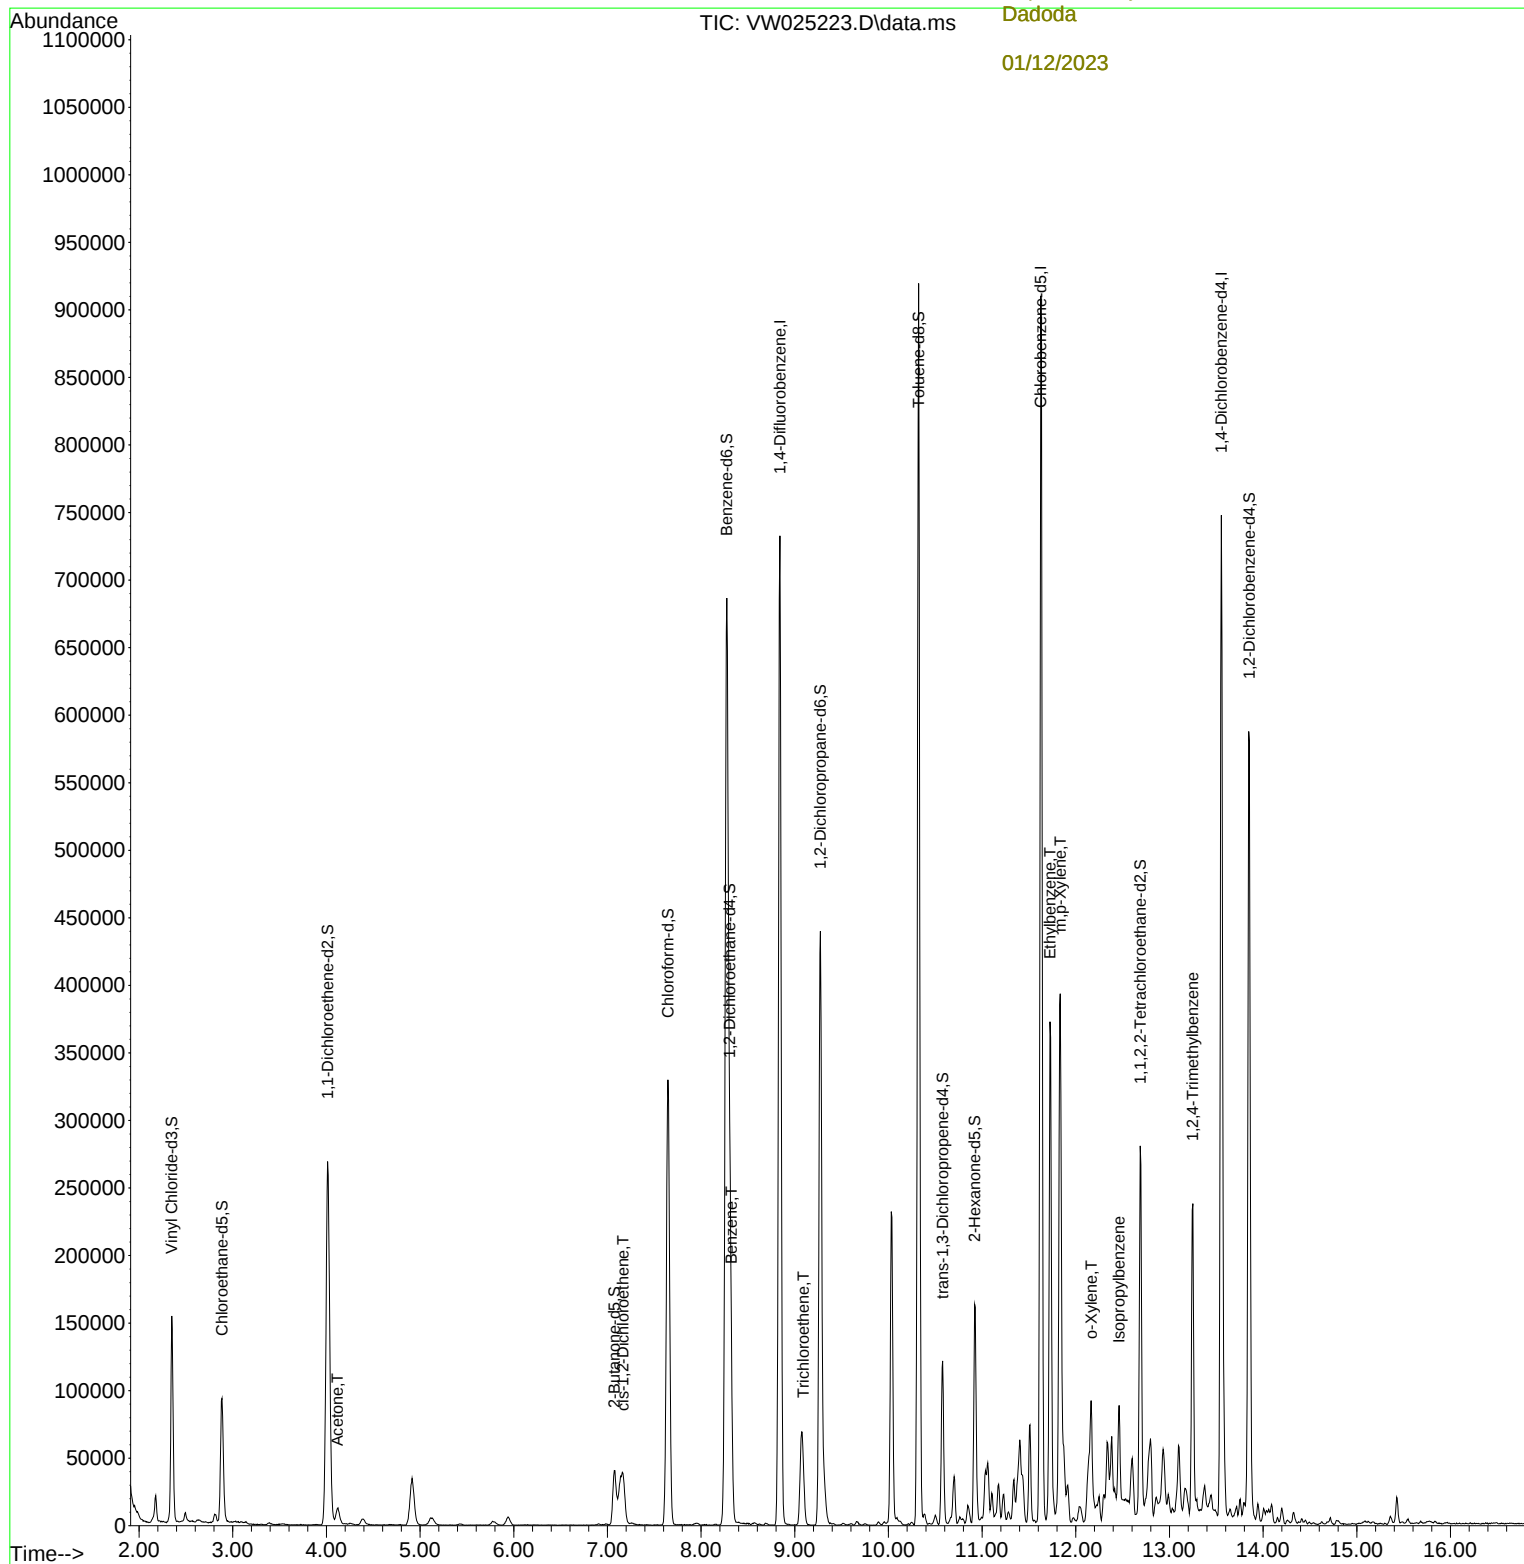




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011123\
 Data File : VW025223.D
 Acq On : 11 Jan 2023 13:35
 Operator : SY/MD
 Sample : 01120-01
 Misc : 5.24g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1141

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/12/2023
 Supervised By :Mahesh Dadoda 01/12/2023

01/12/2023
 Supervised By :Mahesh

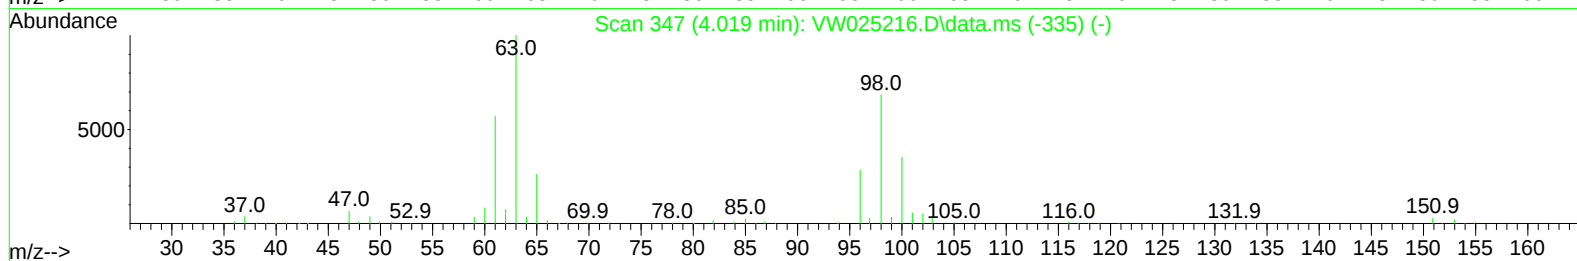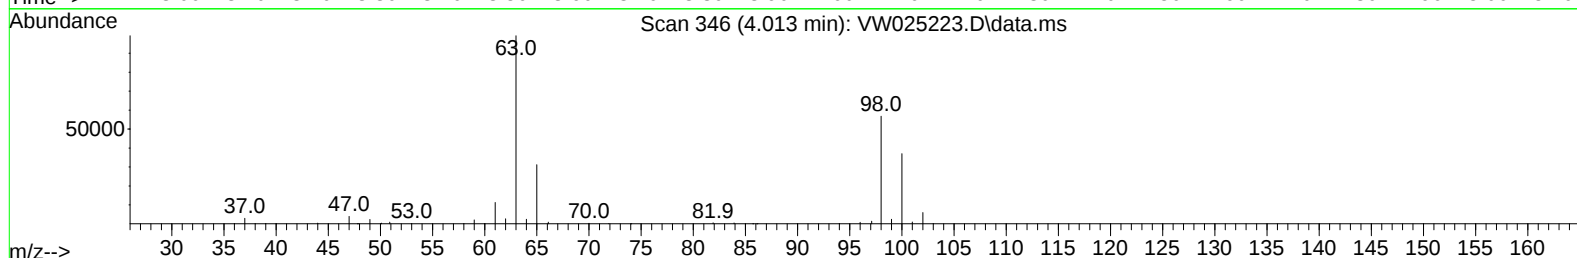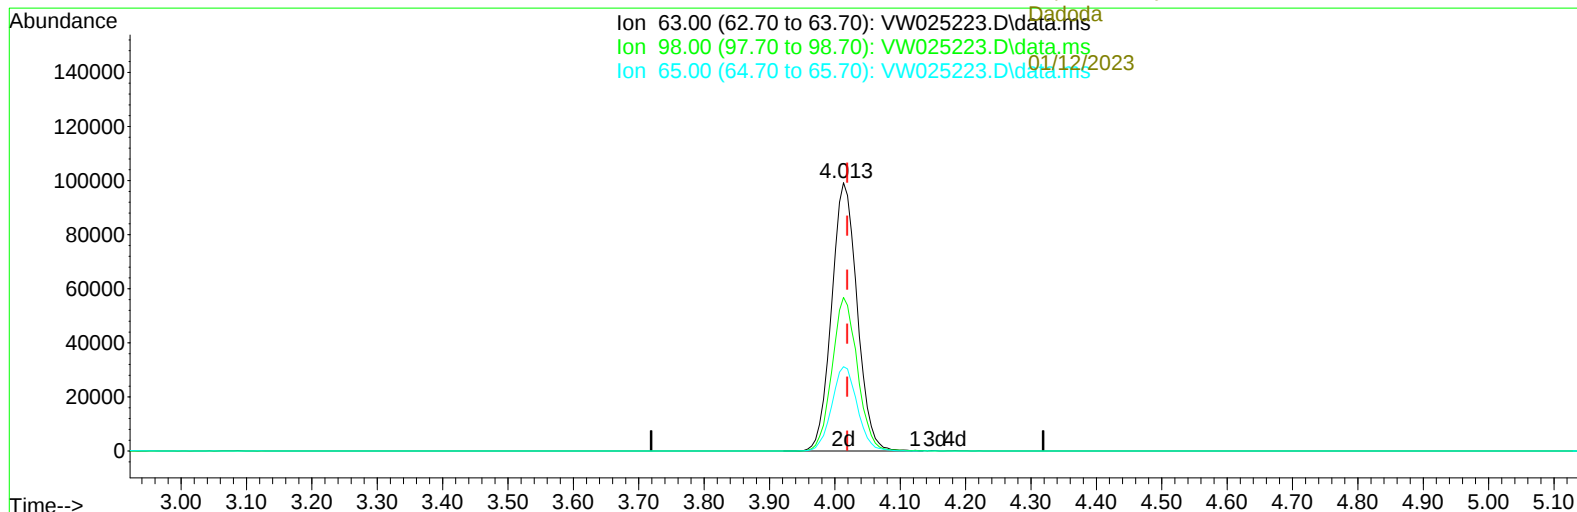

TIC: VW025223.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 17.40 ug/L m

response 268911

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	73.00	0.04#
65.00	23.40	0.02#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011123\
 Data File : VW025223.D
 Acq On : 11 Jan 2023 13:35
 Operator : SY/MD
 Sample : 01120-01
 Misc : 5.24g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1141

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/12/2023
 Supervised By :Mahesh Dadoda 01/12/2023

01/12/2023
 Supervised By :Mahesh
 Dadoda

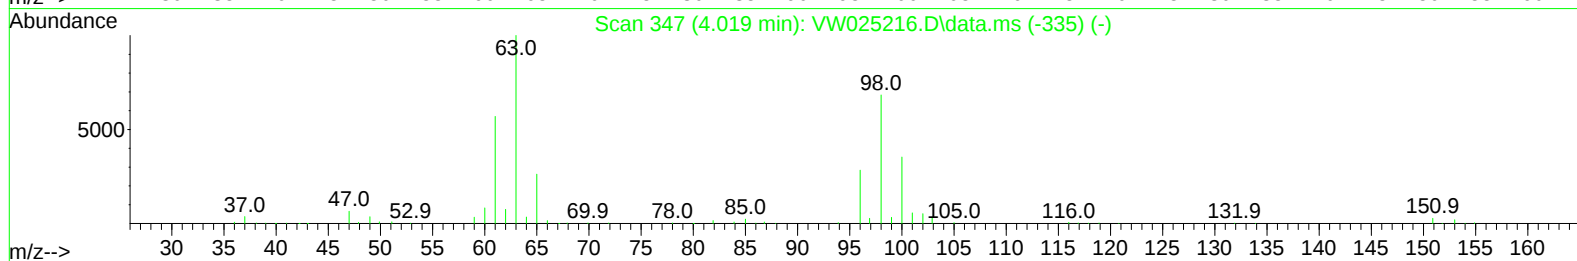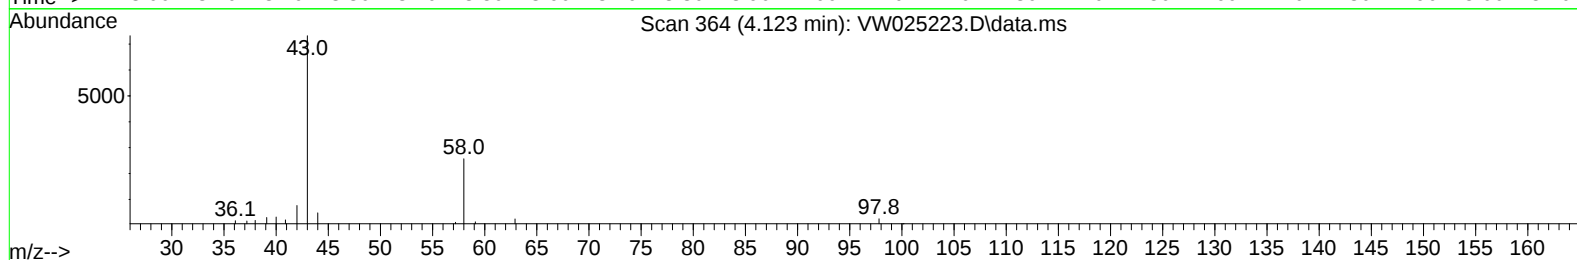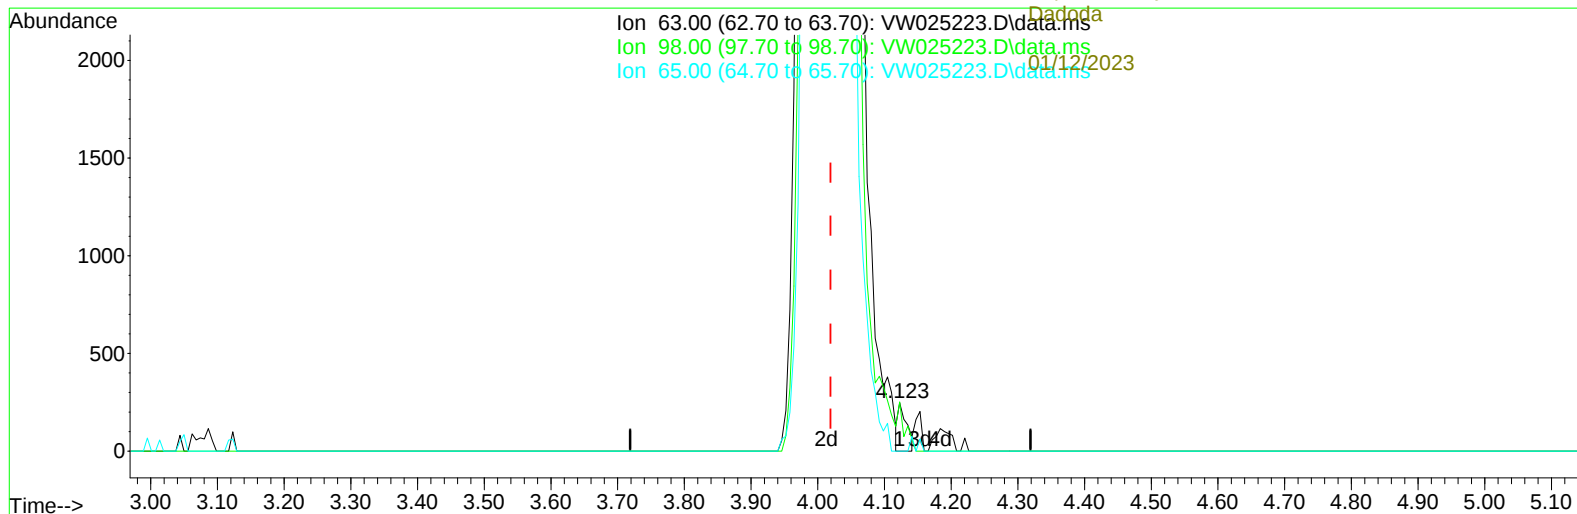

TIC: VW025223.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.123min (+ 0.104) 0.01 ug/L

response 226

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	73.00	52.65
65.00	23.40	23.01
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011123\
 Data File : VW025223.D
 Acq On : 11 Jan 2023 13:35
 Operator : SY/MD
 Sample : 01120-01
 Misc : 5.24g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1141

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/12/2023
 Supervised By :Mahesh Dadoda 01/12/2023

Quant Time: Jan 12 04:20:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 04 00:45:59 2023
 Response via : Initial Calibration

01/12/2023
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	607904	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	503802	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	194026	25.000	ug/L	0.00

01/12/2023

System Monitoring Compounds

4) Vinyl Chloride-d3	2.349	65	144578	20.486	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.960%
7) Chloroethane-d5	2.885	69	104460	23.491	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.960%
11) 1,1-Dichloroethene-d2	4.013	63	268911m	17.397	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.600%
21) 2-Butanone-d5	7.074	46	69668	38.950	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.900%
24) Chloroform-d	7.647	84	340926	22.376	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.520%
26) 1,2-Dichloroethane-d4	8.305	65	173063	22.051	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.200%
32) Benzene-d6	8.275	84	739153	24.433	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.720%
36) 1,2-Dichloropropane-d6	9.274	67	213387	24.113	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.440%
41) Toluene-d8	10.323	98	588863	21.387	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.560%
43) trans-1,3-Dichloroprop...	10.579	79	71097	18.762	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.040%
47) 2-Hexanone-d5	10.920	63	54246	38.901	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.800%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	130816	21.138	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	156087	22.642	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.560%

Target Compounds						Qvalue
13) Acetone	4.117	43	21056	10.066	ug/L	99
20) cis-1,2-Dichloroethene	7.165	96	16654	1.985	ug/L	98
33) Benzene	8.323	78	50123	1.646	ug/L	100
34) Trichloroethene	9.091	95	9585	1.207	ug/L #	92
52) Ethylbenzene	11.725	91	247256	6.926	ug/L	97
53) m,p-Xylene	11.835	106	118316	8.576	ug/L	94
54) o-Xylene	12.164	106	19985	1.574	ug/L	94
60) Isopropylbenzene	12.463	105	47887	1.638	ug/L	99
63) 1,2,4-Trimethylbenzene	13.249	105	131487	5.377	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed