


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011123\
Data File : VW025220.D
Acq On : 11 Jan 2023 11:39
Operator : SY/MD
Sample : BFB470
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB470

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
Title : SFAM01.0
Last Update : Wed Jan 04 00:45:59 2023

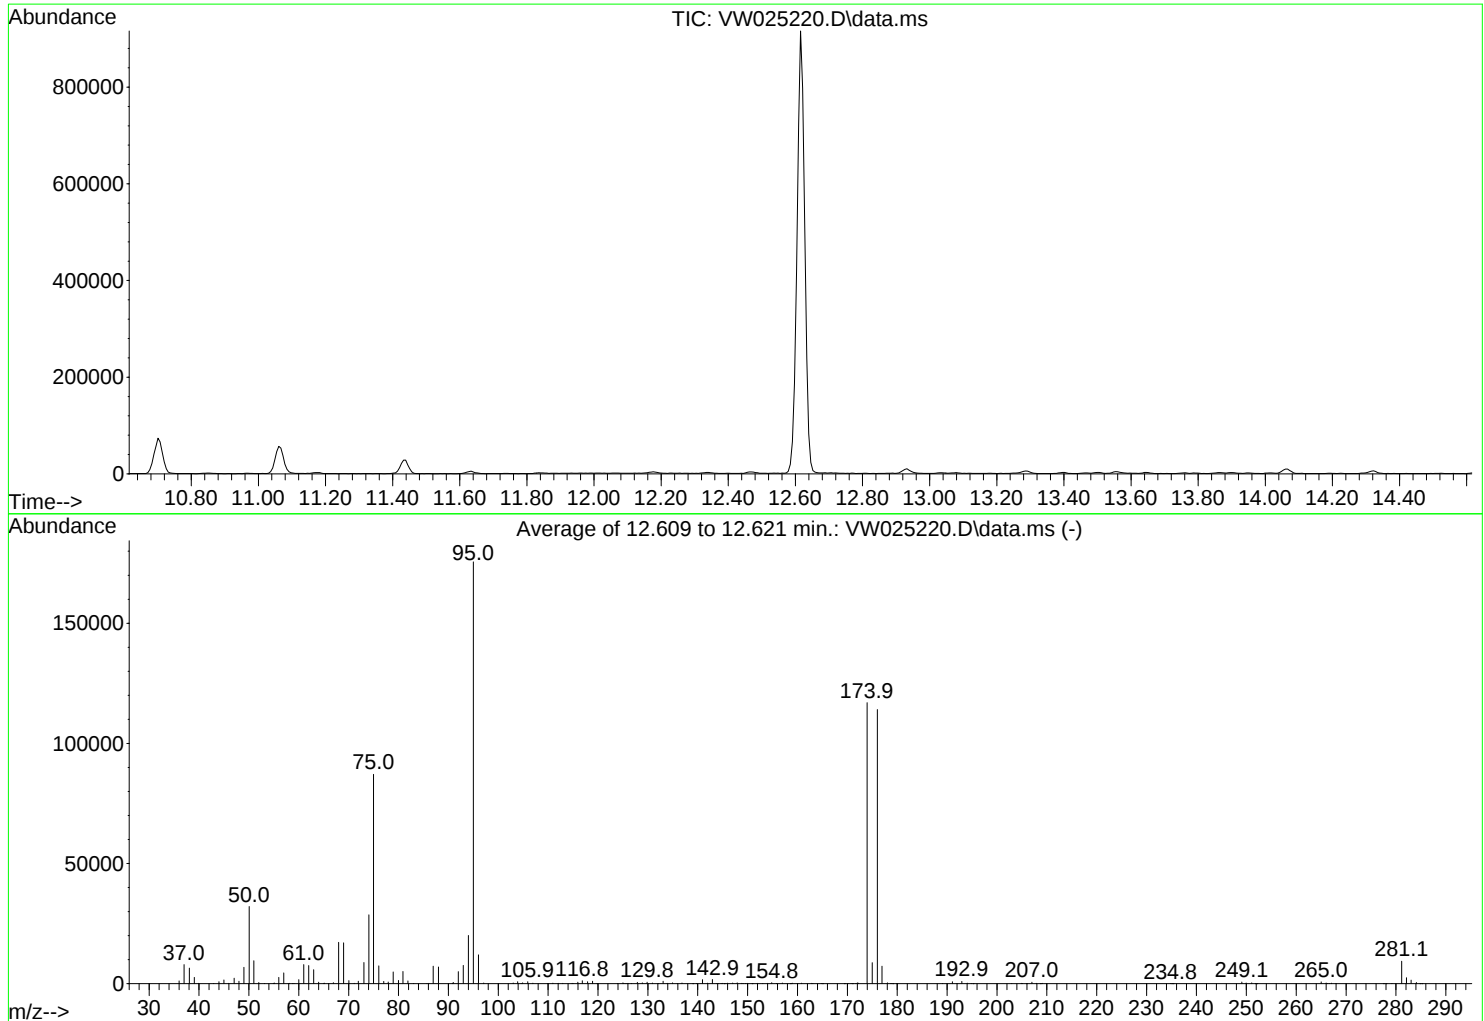

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	32077	PASS
75	95	30	80	49.6	87131	PASS
95	95	100	100	100.0	175573	PASS
96	95	5	9	6.8	11979	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	66.6	116981	PASS
175	174	5	9	7.5	8762	PASS
176	174	95	105	97.6	114120	PASS
177	176	5	10	6.4	7269	PASS

m/z	Abundance
35.10	97.0
36.10	305.0
38.10	161.0
39.10	60.0
39.80	173.0
40.90	80.0
43.00	57.0
44.00	263.0
55.10	73.0
56.90	115.0

Instrument :
MSVOA_W
ClientSampleId :
BFB470

m/z	Abundance
36.00	1472.0
37.00	7125.0
38.10	6765.0
39.10	2558.0
40.00	244.0
41.00	90.0
42.90	158.0
43.90	926.0
45.00	1559.0
47.00	2140.0
48.00	991.0
49.00	6115.0
50.10	30384.0
51.00	8733.0
52.00	546.0
53.20	77.0
54.90	393.0
56.00	2546.0
57.10	4519.0
57.90	232.0
58.80	281.0
60.00	1600.0
61.00	7692.0
62.00	7187.0
63.00	5686.0
64.00	578.0
65.00	439.0
67.00	455.0
68.00	16280.0
69.00	15079.0
70.00	1115.0
71.20	94.0
72.00	1080.0
73.10	8935.0
74.10	27056.0
75.00	82432.0
76.10	6908.0
77.10	1030.0
78.10	615.0
78.90	4463.0
80.00	1051.0
80.90	4626.0
81.90	988.0
83.00	103.0
85.70	256.0
86.90	6637.0
88.00	6555.0
90.80	680.0
92.00	4541.0
93.00	6914.0
94.00	16600.0
95.00	156352.0
96.00	10780.0
97.20	274.0
103.00	452.0
103.90	683.0
104.60	213.0
105.10	256.0
105.90	692.0
107.00	169.0
109.90	161.0
110.90	199.0
112.00	244.0
113.00	100.0
114.80	210.0
116.10	598.0
116.90	983.0
118.00	893.0
118.90	852.0
119.80	91.0
123.90	84.0
125.00	586.0
125.60	172.0
126.10	147.0
128.00	487.0
128.80	252.0
129.80	521.0
131.00	228.0
132.00	91.0
133.10	1548.0
134.90	356.0
136.80	219.0
140.90	1377.0
141.90	179.0
142.90	1551.0
143.80	68.0
144.10	79.0
145.00	225.0
146.00	160.0
146.90	335.0
147.90	316.0
148.90	250.0

Instrument :
MSVOA_W
ClientSampleId :
BFB470

150.10	130.0
150.90	52.0
151.90	131.0
153.20	53.0
153.90	55.0
154.90	301.0
155.80	111.0
156.90	296.0
158.60	73.0
159.00	171.0
160.00	63.0
160.90	169.0
162.80	240.0
163.10	224.0
164.80	157.0
169.40	67.0
170.10	73.0
170.70	77.0
171.70	291.0
172.10	481.0
174.00	86584.0
175.00	7368.0
176.00	89416.0
177.00	6099.0
178.00	466.0
178.70	266.0
179.90	81.0
189.10	109.0
191.10	1160.0
193.00	1536.0
194.00	299.0
194.90	211.0
203.00	88.0
204.90	432.0
205.90	54.0
207.00	1018.0
207.90	236.0
209.10	266.0
234.80	150.0
235.30	98.0
249.10	1028.0
250.00	398.0
251.10	552.0
252.10	98.0
265.10	1090.0
266.10	313.0
266.60	209.0
267.10	352.0
268.10	64.0
277.50	90.0
279.30	126.0
281.20	13060.0
282.10	3734.0
283.00	2227.0
284.20	640.0
285.20	107.0

Instrument :
MSVOA_W
ClientSampleId :
BFB470

m/z	Abundance
36.00	1610.0
37.00	9080.0
38.00	7259.0
39.10	3166.0
40.00	325.0
41.00	79.0
43.00	116.0
44.00	1157.0
45.00	1754.0
46.00	193.0
47.00	2734.0
48.00	1026.0
49.00	7426.0
50.00	35768.0
51.00	11038.0
52.00	523.0
53.20	79.0
55.10	491.0
56.00	2767.0
57.00	5113.0
58.10	151.0
59.10	171.0
60.00	1766.0
61.00	8907.0
62.00	8158.0
63.00	6814.0
64.00	593.0
65.20	347.0
66.00	61.0
66.90	382.0
68.00	19192.0
69.00	19040.0
70.00	1524.0
71.00	176.0
71.90	1011.0
73.00	9390.0
74.00	31544.0
75.00	100200.0
76.10	7939.0
76.90	1076.0
77.90	810.0
79.00	5323.0
80.00	1695.0
80.90	5541.0
81.90	1293.0
83.10	128.0
86.90	7862.0
88.00	7449.0
91.00	789.0
92.00	5478.0
93.00	8162.0
94.00	23248.0
95.00	200256.0
96.00	14108.0
97.10	316.0
103.00	322.0
103.90	713.0
104.90	236.0
105.90	915.0
107.00	203.0
110.10	186.0
110.90	173.0
112.10	142.0
112.90	136.0
115.00	309.0
115.90	541.0
116.90	1404.0
117.90	823.0
118.90	1093.0
124.00	79.0
125.00	362.0
125.90	182.0
126.70	87.0
127.90	697.0
128.90	413.0
129.80	707.0
130.80	317.0
132.10	74.0
133.00	887.0
134.00	315.0
135.00	445.0
136.90	326.0
139.80	159.0
140.90	1816.0
141.90	142.0
143.00	1948.0
143.90	177.0
145.00	232.0
146.00	191.0
147.00	228.0
147.90	426.0
148.80	209.0

Instrument :
MSVOA_W
ClientSampleId :
BFB470

149.60	145.0
152.00	105.0
153.00	155.0
154.00	227.0
154.80	411.0
155.80	106.0
156.90	278.0
158.90	282.0
160.10	69.0
160.90	297.0
162.90	208.0
164.80	105.0
170.20	124.0
170.80	113.0
171.90	526.0
173.90	134592.0
175.00	9737.0
176.00	128144.0
176.90	8288.0
178.00	295.0
178.90	156.0
189.10	61.0
191.00	992.0
192.00	154.0
192.90	1025.0
194.10	225.0
194.70	85.0
195.20	91.0
202.90	77.0
205.10	127.0
207.00	533.0
207.90	107.0
208.70	59.0
209.20	60.0
235.00	91.0
249.10	564.0
249.90	270.0
251.10	251.0
264.90	663.0
265.90	258.0
266.30	186.0
267.00	284.0
267.90	57.0
278.00	61.0
279.10	78.0
281.10	10323.0
282.10	2636.0
283.10	1600.0
284.00	418.0
284.80	109.0

Instrument :
MSVOA_W
ClientSampleId :
BFB470

m/z	Abundance
36.00	1280.0
37.00	7567.0
38.00	5932.0
39.00	2336.0
40.00	296.0
40.90	52.0
43.00	149.0
44.10	1067.0
45.00	1228.0
45.90	169.0
47.10	2014.0
48.00	891.0
49.00	6844.0
50.00	30080.0
51.00	8826.0
52.00	345.0
53.10	64.0
55.10	517.0
56.00	2522.0
57.10	4178.0
58.10	229.0
59.00	88.0
60.00	1605.0
61.00	7204.0
62.00	7315.0
63.00	4842.0
64.00	592.0
65.10	225.0
66.00	158.0
67.00	430.0
68.00	16066.0
69.00	16944.0
70.10	1112.0
71.20	71.0
72.00	971.0
73.00	8040.0
74.00	27264.0
75.00	78760.0
76.00	7357.0
77.10	773.0
77.90	670.0
78.90	4826.0
80.00	1234.0
80.90	5143.0
81.90	1101.0
83.00	63.0
86.10	356.0
87.00	7296.0
88.00	6728.0
91.00	556.0
92.00	5071.0
93.00	7729.0
94.00	20224.0
95.00	170112.0
96.10	11048.0
97.00	299.0
103.00	133.0
103.90	923.0
104.80	429.0
105.90	721.0
106.80	195.0
109.70	61.0
110.00	51.0
111.00	167.0
111.90	139.0
112.90	133.0
114.80	207.0
115.90	601.0
116.80	1126.0
117.80	684.0
118.90	1164.0
124.00	77.0
125.20	206.0
126.70	83.0
127.80	415.0
129.00	280.0
129.90	678.0
130.90	283.0
132.10	77.0
133.10	666.0
133.80	196.0
135.00	212.0
135.90	121.0
136.80	277.0
139.00	76.0
139.80	124.0
141.00	1818.0
142.00	216.0
143.00	1700.0
144.10	122.0
144.70	175.0
145.30	107.0

Instrument :
MSVOA_W
ClientSampleId :
BFB470

145.90	294.0
147.10	205.0
147.90	376.0
149.10	186.0
149.90	201.0
151.90	101.0
153.00	100.0
154.00	148.0
154.80	417.0
155.80	76.0
157.00	285.0
158.90	203.0
160.80	192.0
165.00	100.0
170.00	109.0
171.00	97.0
172.20	694.0
174.00	129768.0
175.00	9180.0
176.00	124800.0
177.00	7421.0
178.10	274.0
179.10	77.0
191.10	235.0
193.00	332.0
194.00	76.0
204.90	82.0
207.00	272.0
209.10	75.0
249.00	337.0
250.00	98.0
251.00	167.0
251.80	50.0
265.00	445.0
266.10	163.0
281.10	4537.0
282.00	1104.0
283.10	579.0
284.10	267.0

Instrument :
MSVOA_W
ClientSampleId :
BFB470