

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011420\
 Data File : VW014633.D
 Acq On : 14 Jan 2020 15:21
 Operator : SY/VA
 Sample : L1109-07
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GASG6

Manual Integrations
 APPROVED

MMDadoda
 1/16/2020 1:50:53 PM

Quant Time: Jan 15 02:28:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jan 15 01:48:42 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1280680	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1118810	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	500081	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	414367	22.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.80%
7) Chloroethane-d5	2.89	69	324282	24.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.52%
10) 1,1-Dichloroethene-d2	4.01	63	595864	18.04	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.16%
20) 2-Butanone-d5	7.07	46	174925	40.72	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.44%
24) Chloroform-d	7.65	84	718188	24.38	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.52%
26) 1,2-Dichloroethane-d4	8.31	65	366110m	23.94	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.76%
29) Benzene-d6	8.27	84	1575724	26.48	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.92%
33) 1,2-Dichloropropane-d6	9.27	67	471184	26.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.36%
37) Toluene-d8	10.32	98	1416934	26.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.08%
38) trans-1,3-Dichloropropene-	10.57	79	181215	24.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.12%
39) 2-Hexanone-d5	10.92	63	140449	45.92	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.84%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	314014	23.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.52%
61) 1,2-Dichlorobenzene-d4	13.85	152	456538	27.71	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.84%

Target Compounds					Ovalue
13) Acetone	4.12	43	19830m	3.334	ug/L
16) Methylene chloride	4.92	84	35350	1.693	ug/L
44) Toluene	10.38	91	81394	1.157	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW011420\
Data File : VW014633.D
Acq On : 14 Jan 2020 15:21
Operator : SY/VA
Sample : L1109-07
Misc : 5.02G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GASG6

Manual Integrations
APPROVED

MMDadoda
1/16/2020 1:50:53 PM

Quant Time: Jan 15 02:28:03 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
Quant Title : VOC Analysis
QLast Update : Wed Jan 15 01:48:42 2020
Response via : Initial Calibration

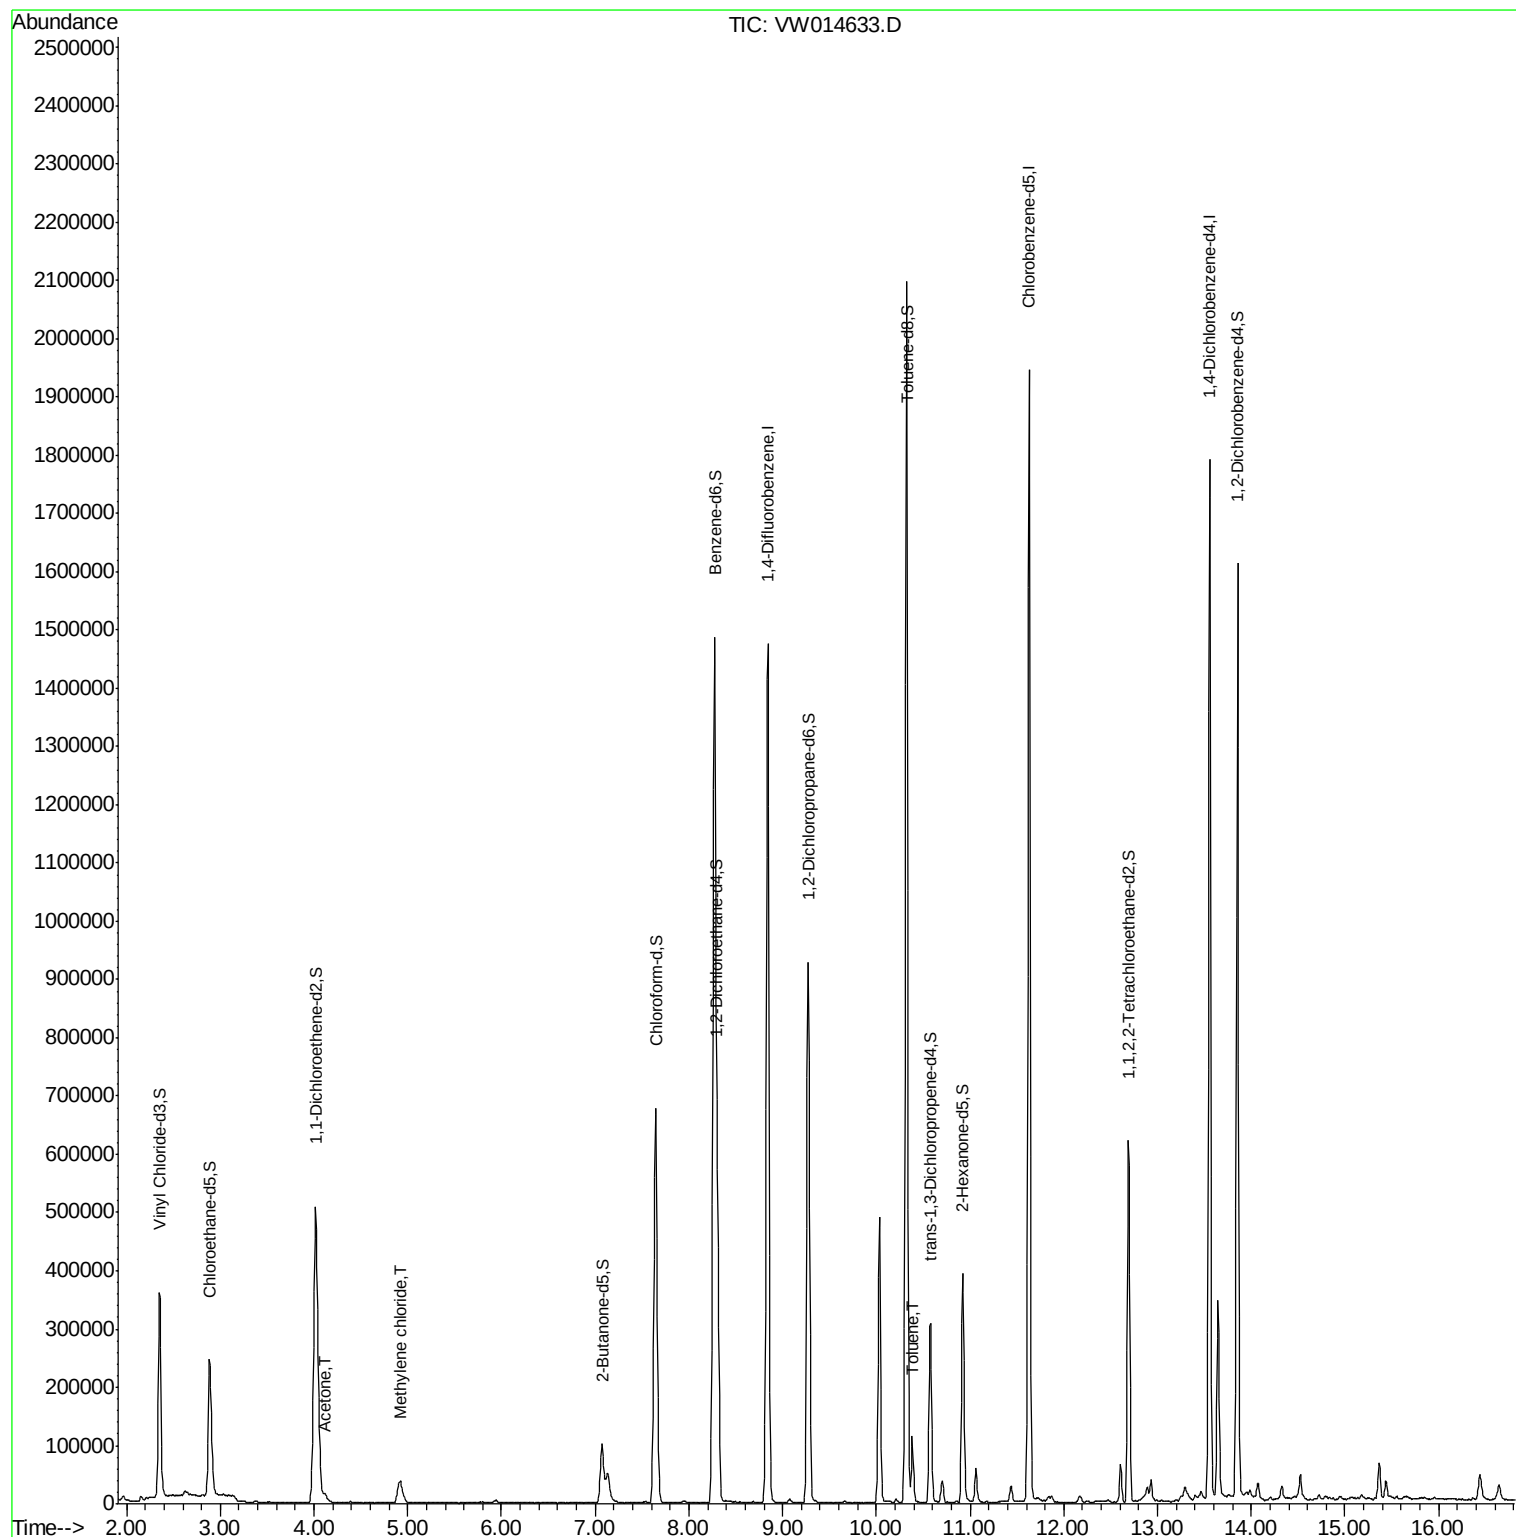

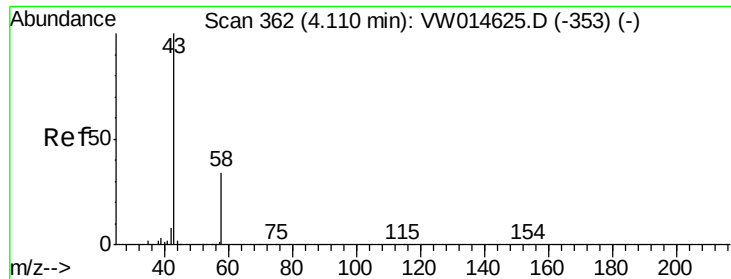





#13
Acetone
Concen: 3.334 ug/L m
RT: 4.12 min Scan# 363
Delta R.T. 0.01 min
Lab File: VW014633.D
Acq: 14 Jan 2020 15:21

Instrument :
MSVOA_W
ClientSampleId :
GASG6

Tot Ion	43	Resp	19830
Ion Ratio	43	100	Lower Upper
	58	30.9	0.0 64.0




Manual Integrations
APPROVED


MMDadoda
1/16/2020 1:50:53 PM

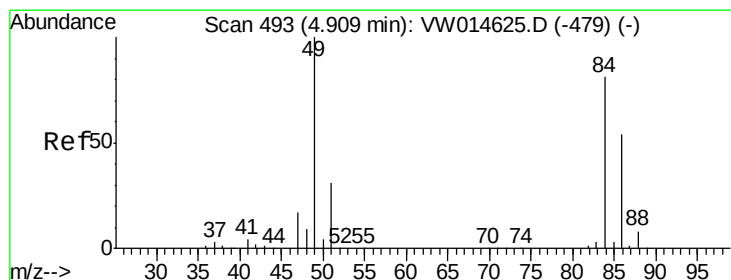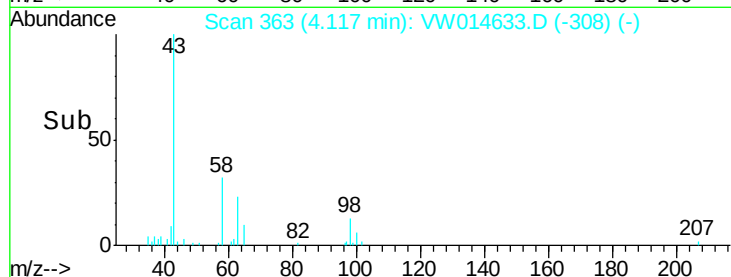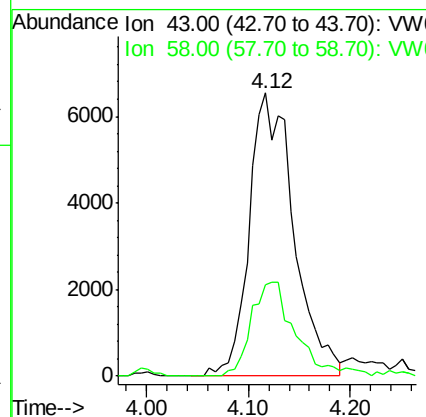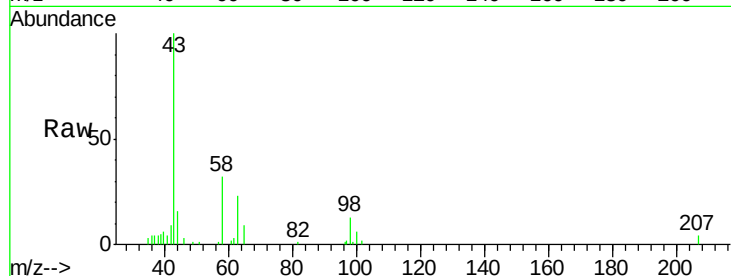

#16
Methylene chloride
Concen: 1.693 ug/L
RT: 4.92 min Scan# 495
Delta R.T. 0.01 min
Lab File: VW014633.D
Acq: 14 Jan 2020 15:21

Tgt Ion	84	Resp	35350
Ion Ratio	84	100	Lower Upper
	49	112.9	85.8 159.4
	86	61.5	44.5 82.7

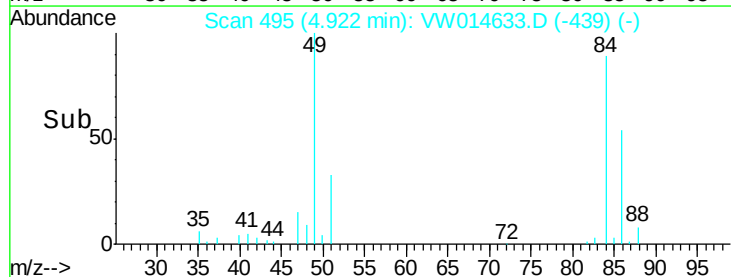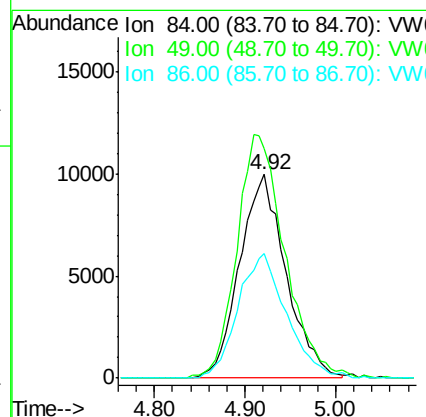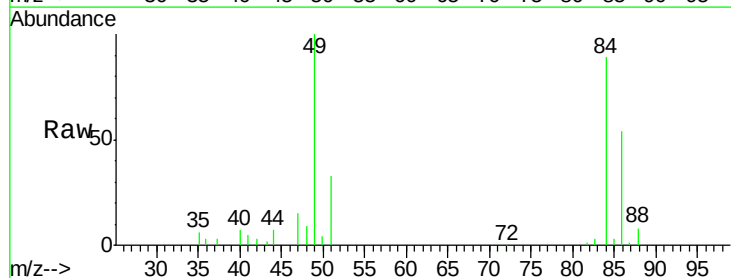

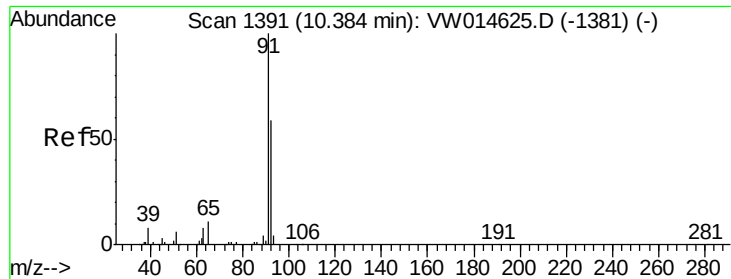

#44
Toluene
Concen: 1.157 ug/L
RT: 10.38 min Scan# 1391
Delta R.T. 0.00 min
Lab File: VW014633.D
Acq: 14 Jan 2020 15:21

Instrument :
MSVOA_W
ClientSampleId :
GASG6

Tot Ion	Ion	Ratio	Resp	Lower	Upper
91	100		81394		
92	57.6	40.2	74.6		

Manual Integrations
APPROVED

MMDadoda
1/16/2020 1:50:53 PM

