

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011620\
 Data File : VW014671.D
 Acq On : 16 Jan 2020 14:28
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK

Manual Integrations
 APPROVED

MMDadoda
 1/17/2020 1:58:52 PM

Quant Time: Jan 17 03:23:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 17 01:19:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	982895	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	890277	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	422654	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	281854	20.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.36%
7) Chloroethane-d5	2.89	69	230043	22.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.12%
10) 1,1-Dichloroethene-d2	4.02	63	425265	16.78	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.12%
20) 2-Butanone-d5	7.07	46	206137	62.52	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.04%
24) Chloroform-d	7.64	84	540467	23.90	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.60%
26) 1,2-Dichloroethane-d4	8.30	65	302179m	25.75	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.00%
29) Benzene-d6	8.27	84	1188596	25.11	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.44%
33) 1,2-Dichloropropane-d6	9.27	67	365756	25.69	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.76%
37) Toluene-d8	10.32	98	1076121	25.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.28%
38) trans-1,3-Dichloropropene-	10.57	79	143179	24.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.40%
39) 2-Hexanone-d5	10.92	63	158101	64.96	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	129.92%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	308895	28.90	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	115.60%
61) 1,2-Dichlorobenzene-d4	13.85	152	375480	26.96	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.84%

Target Compounds				Ovalue
13) Acetone	4.12	43	12349	2.705 ug/L 71

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW011620\
Data File : VW014671.D
Acq On : 16 Jan 2020 14:28
Operator : SY/VA
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VIBLK

Manual Integrations
APPROVED

MMDadoda
1/17/2020 1:58:52 PM

Quant Time: Jan 17 03:23:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 17 01:19:13 2020
Response via : Initial Calibration

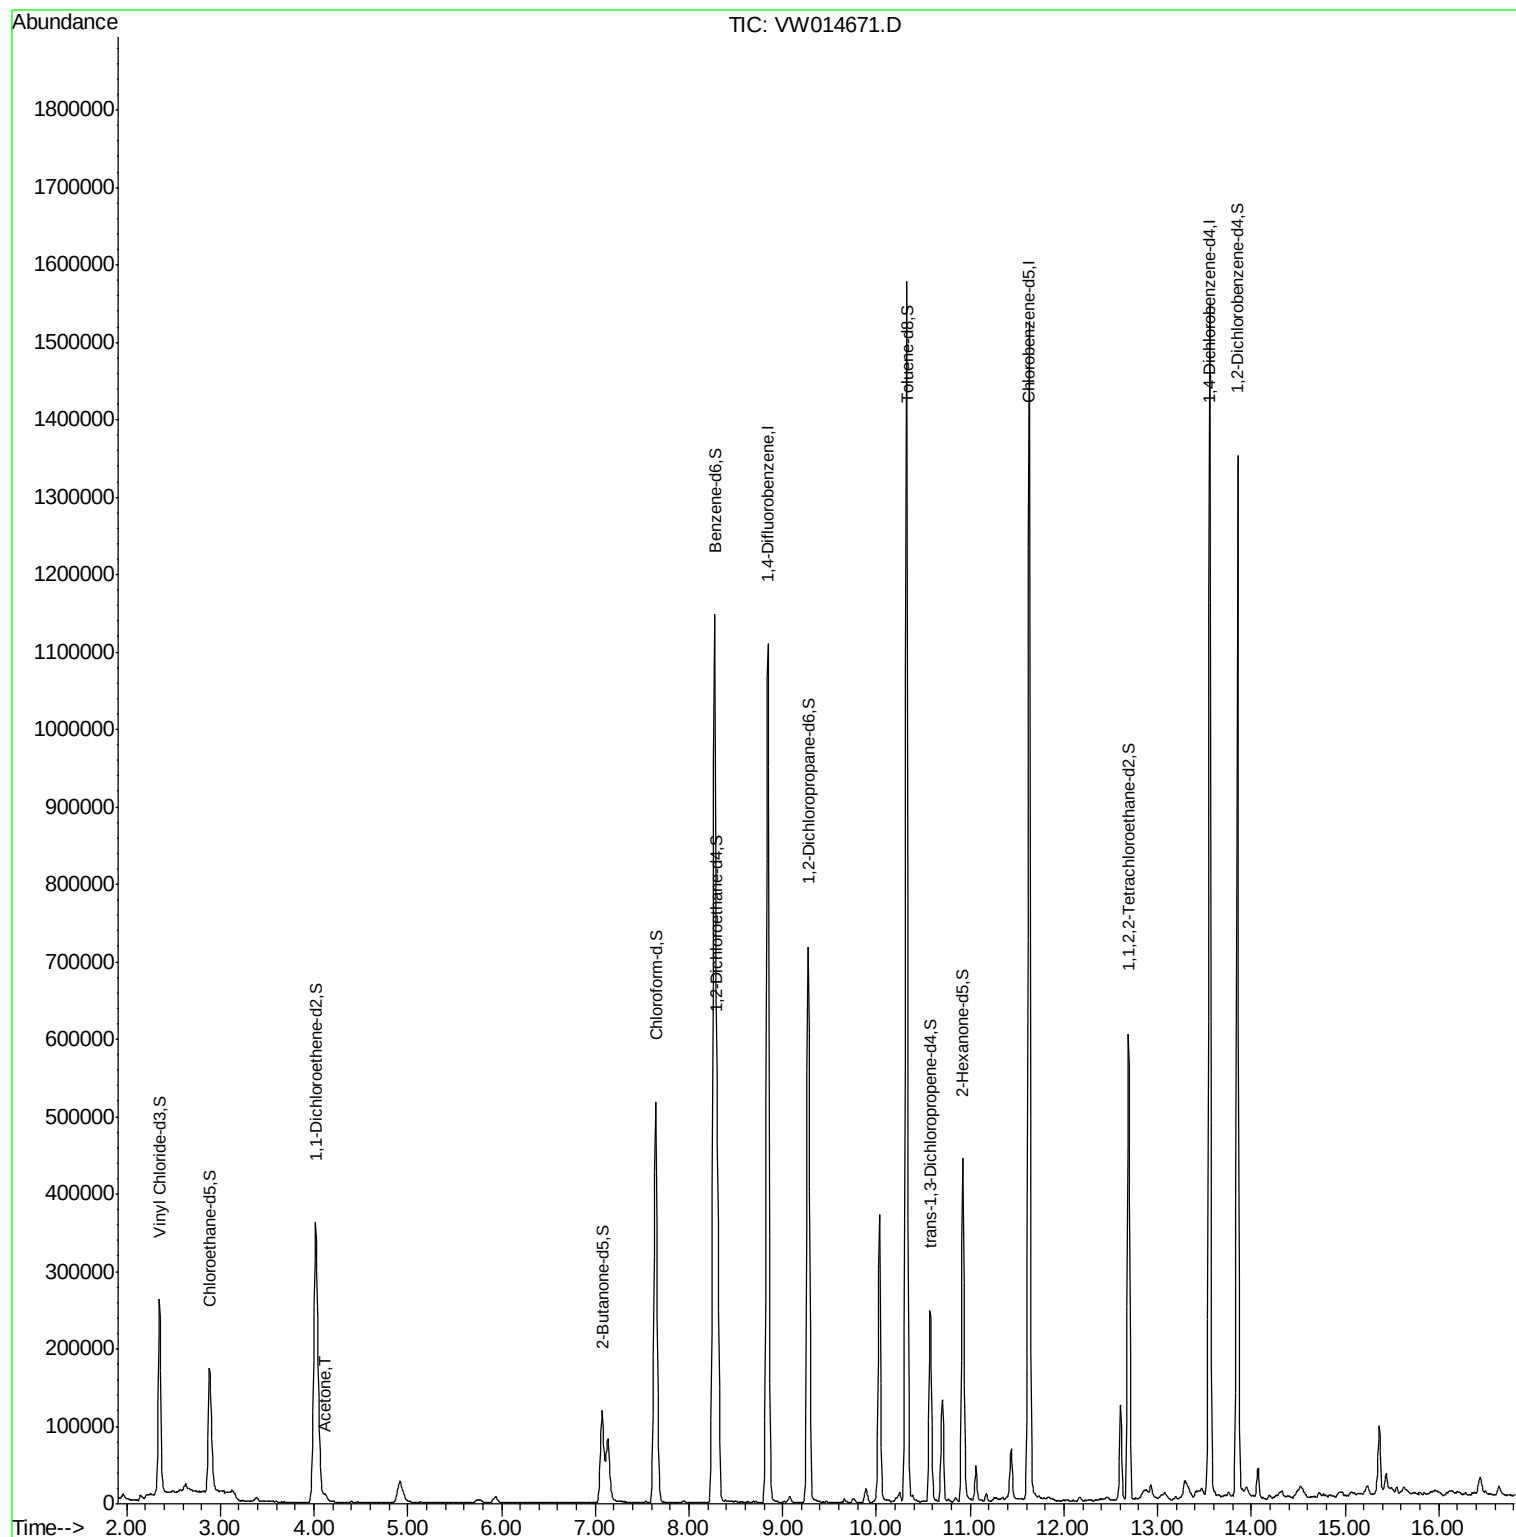

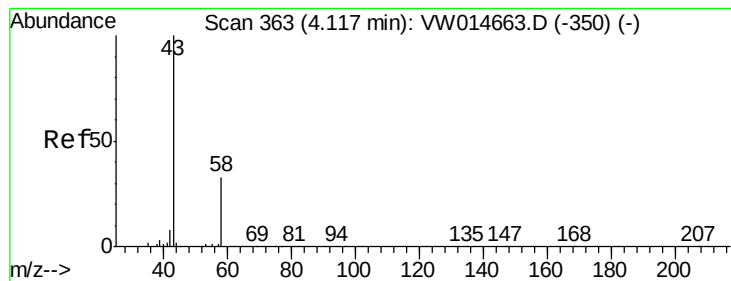

#13

Acetone

Concen: 2.705 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW014671.D

Acq: 16 Jan 2020 14:28

Instrument :

MSVOA_W

ClientSampleId :

VIBLK

Tot Ion: 43 Resp: 12349

Ion Ratio Lower Upper

43 100

58 15.9 0.0 64.0

Manual Integrations

APPROVED

MMDadoda

1/17/2020 1:58:52 PM

