

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011622\
 Data File : VW021954.D
 Acq On : 15 Jan 2022 19:03
 Operator : SY/VA
 Sample : N1168-15
 Misc : 5.60g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLX9

Quant Time: Jan 17 06:41:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 06:38:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	180125	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	177981	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	100603	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	46928	14.017	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.080%
7) Chloroethane-d5	2.885	69	36679	12.132	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	48.520%
11) 1,1-Dichloroethene-d2	4.019	63	67995	12.864	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.440%
21) 2-Butanone-d5	7.086	46	21776	46.083	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.160%
24) Chloroform-d	7.653	84	108593	18.661	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.640%
26) 1,2-Dichloroethane-d4	8.384	65	83	0.030	ug/L	0.07
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.120%#
32) Benzene-d6	8.275	84	215505	18.660	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.640%
36) 1,2-Dichloropropane-d6	9.274	67	60449	19.859	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	79.440%
41) Toluene-d8	10.323	98	211476	18.165	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.640%
43) trans-1,3-Dichloroprop...	10.579	79	23429	18.128	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.520%
47) 2-Hexanone-d5	10.927	63	18930	45.831	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.660%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	48515	20.382	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.520%
66) 1,2-Dichlorobenzene-d4	13.853	152	84765	20.491	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.960%
Target Compounds						
					Qvalue	
34) Trichloroethene	8.848	95	5217	1.648	ug/L	# 5
39) cis-1,3-Dichloropropene	10.037	75	2063	0.558	ug/L	# 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011622\
Data File : VW021954.D
Acq On : 15 Jan 2022 19:03
Operator : SY/VA
Sample : N1168-15
Misc : 5.60g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLX9

Quant Time: Jan 17 06:41:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 17 06:38:36 2022
Response via : Initial Calibration




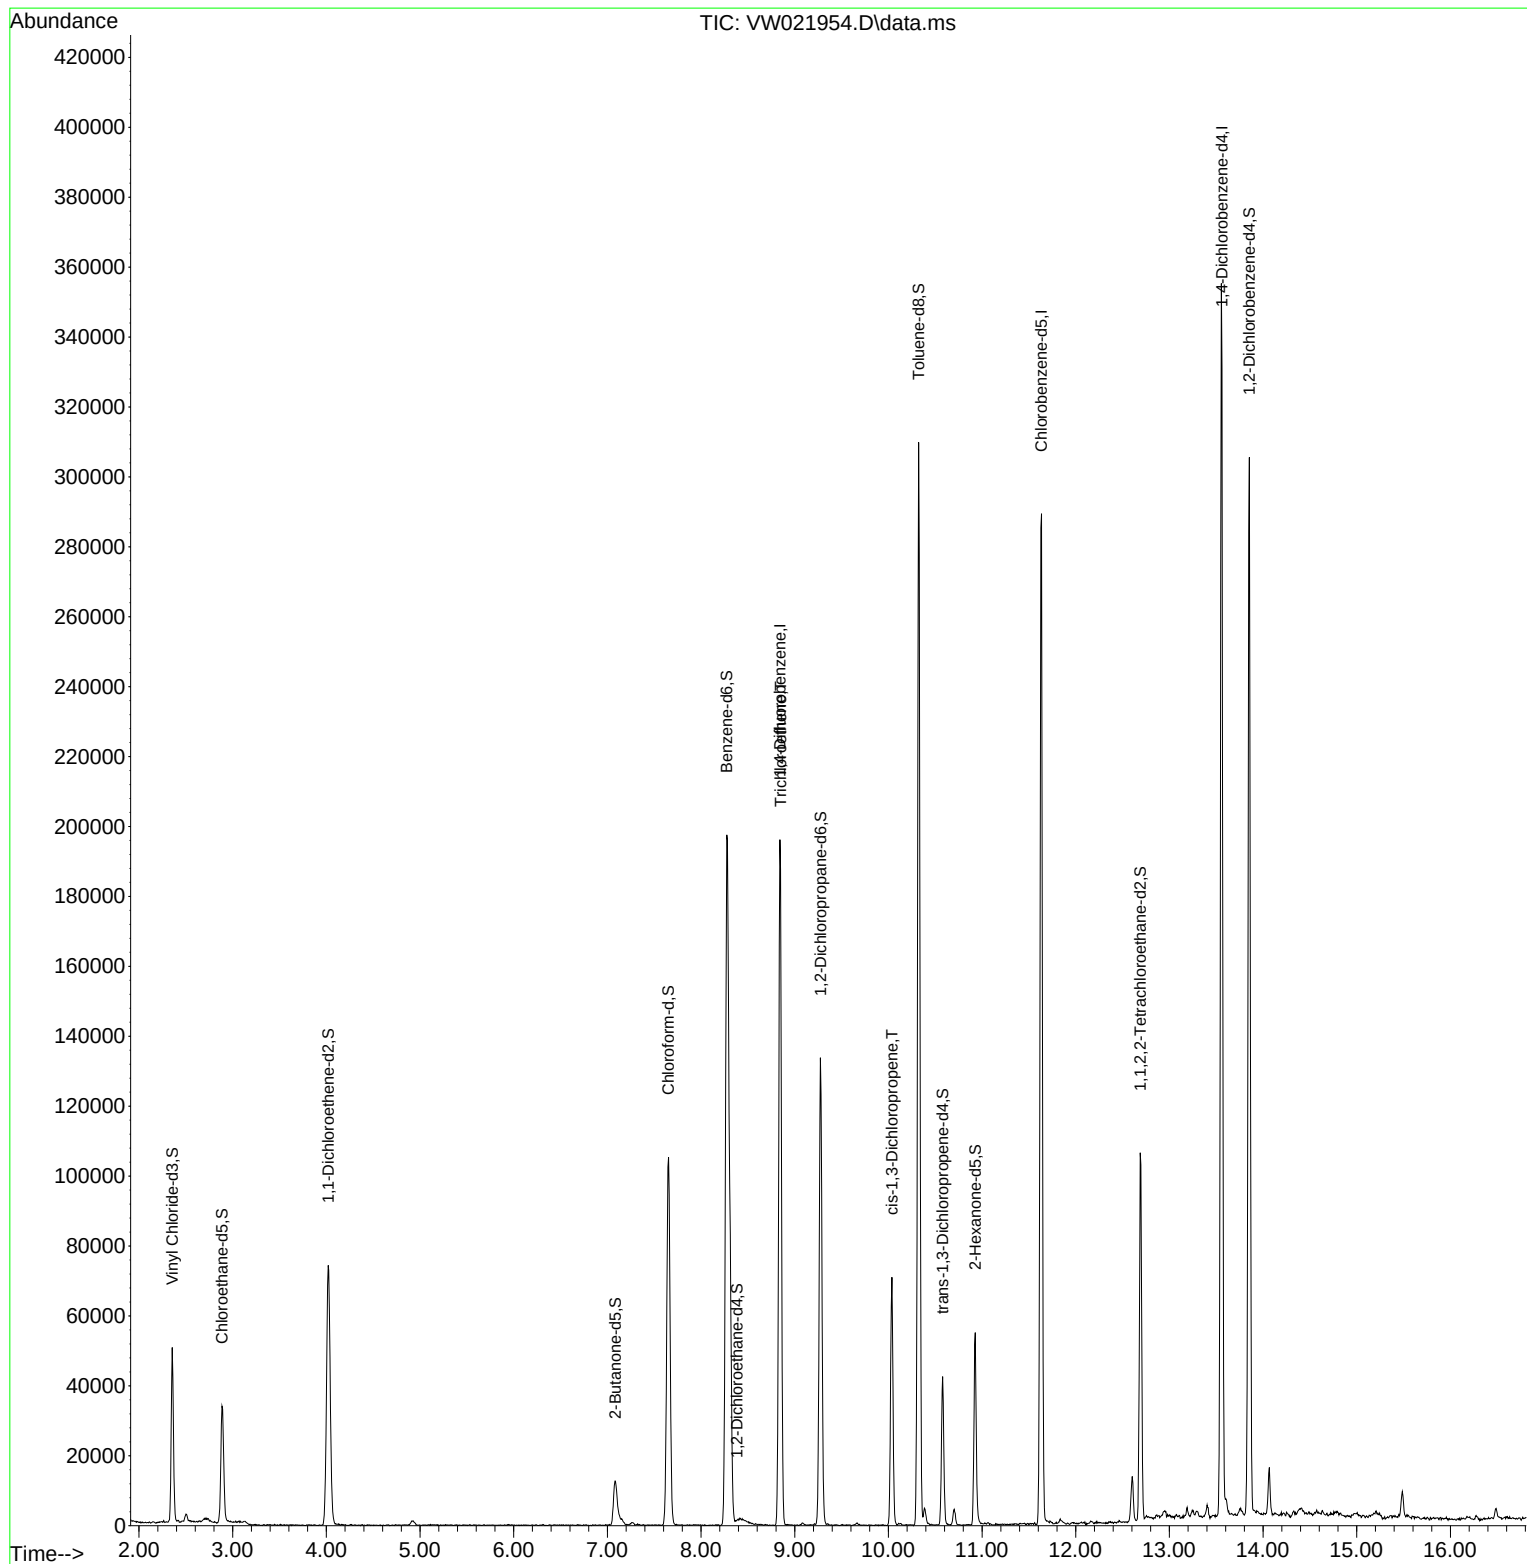


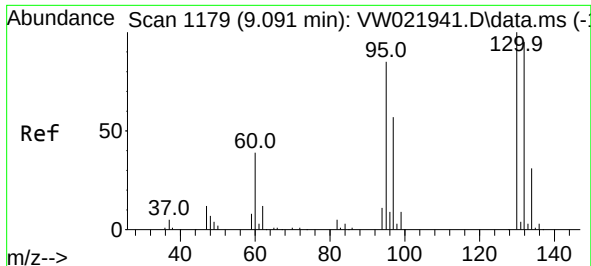

#34
Trichloroethene
Concen: 1.648 ug/L
RT: 8.848 min Scan# 1179
Delta R.T. -0.244 min
Lab File: VW021954.D
Acq: 15 Jan 2022 19:03

Instrument :
MSVOA_W
ClientSampleId :
BGLX9

Tgt Ion: 95	Resp: 5217
Ion Ratio	Lower Upper
95	100
97	0.0 47.0 87.2#
132	0.0 65.5 121.6#
130	0.0 69.4 128.8#

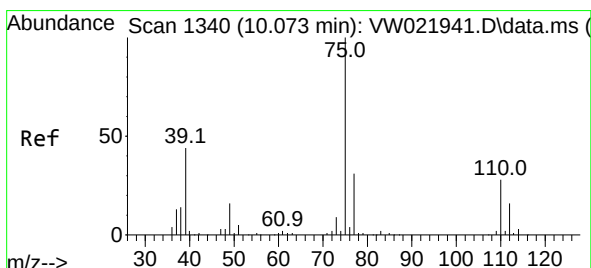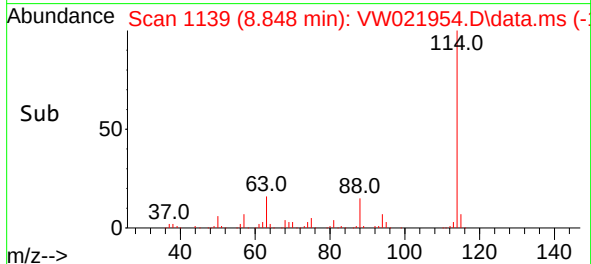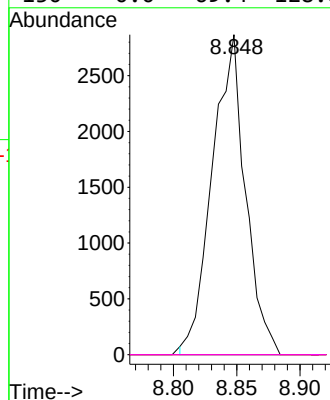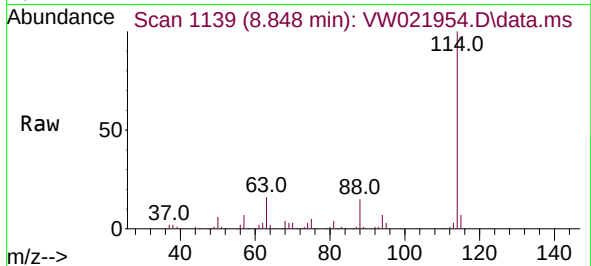

#39
cis-1,3-Dichloropropene
Concen: 0.558 ug/L
RT: 10.037 min Scan# 1334
Delta R.T. -0.036 min
Lab File: VW021954.D
Acq: 15 Jan 2022 19:03

Tgt Ion: 75	Resp: 2063
Ion Ratio	Lower Upper
75	100
77	46.3 21.8 40.6#

