

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011622\
 Data File : VW021948.D
 Acq On : 15 Jan 2022 16:40
 Operator : SY/VA
 Sample : N1168-06
 Misc : 4.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLX2

Quant Time: Jan 17 06:40:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 06:38:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	186475	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	178951	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	95363	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	46817	13.508	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	54.040%
7) Chloroethane-d5	2.885	69	36099	11.534	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	46.120%
11) 1,1-Dichloroethene-d2	4.019	63	70016	12.796	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.200%
21) 2-Butanone-d5	7.080	46	18195	37.193	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.380%
24) Chloroform-d	7.653	84	110171	18.288	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.160%
26) 1,2-Dichloroethane-d4	8.311	65	53309	18.325	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	73.280%
32) Benzene-d6	8.275	84	218337	18.803	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	75.200%
36) 1,2-Dichloropropane-d6	9.275	67	60083	19.632	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	78.520%
41) Toluene-d8	10.323	98	211551	18.073	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.280%
43) trans-1,3-Dichloroprop...	10.579	79	21702	16.701	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.800%
47) 2-Hexanone-d5	10.927	63	16100	38.768	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.540%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	44038	18.401	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	73.600%
66) 1,2-Dichlorobenzene-d4	13.853	152	78831	20.104	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.400%
Target Compounds						
					Qvalue	
46) Tetrachloroethene	10.866	164	7680	2.440	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011622\
Data File : VW021948.D
Acq On : 15 Jan 2022 16:40
Operator : SY/VA
Sample : N1168-06
Misc : 4.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLX2

Quant Time: Jan 17 06:40:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 17 06:38:36 2022
Response via : Initial Calibration

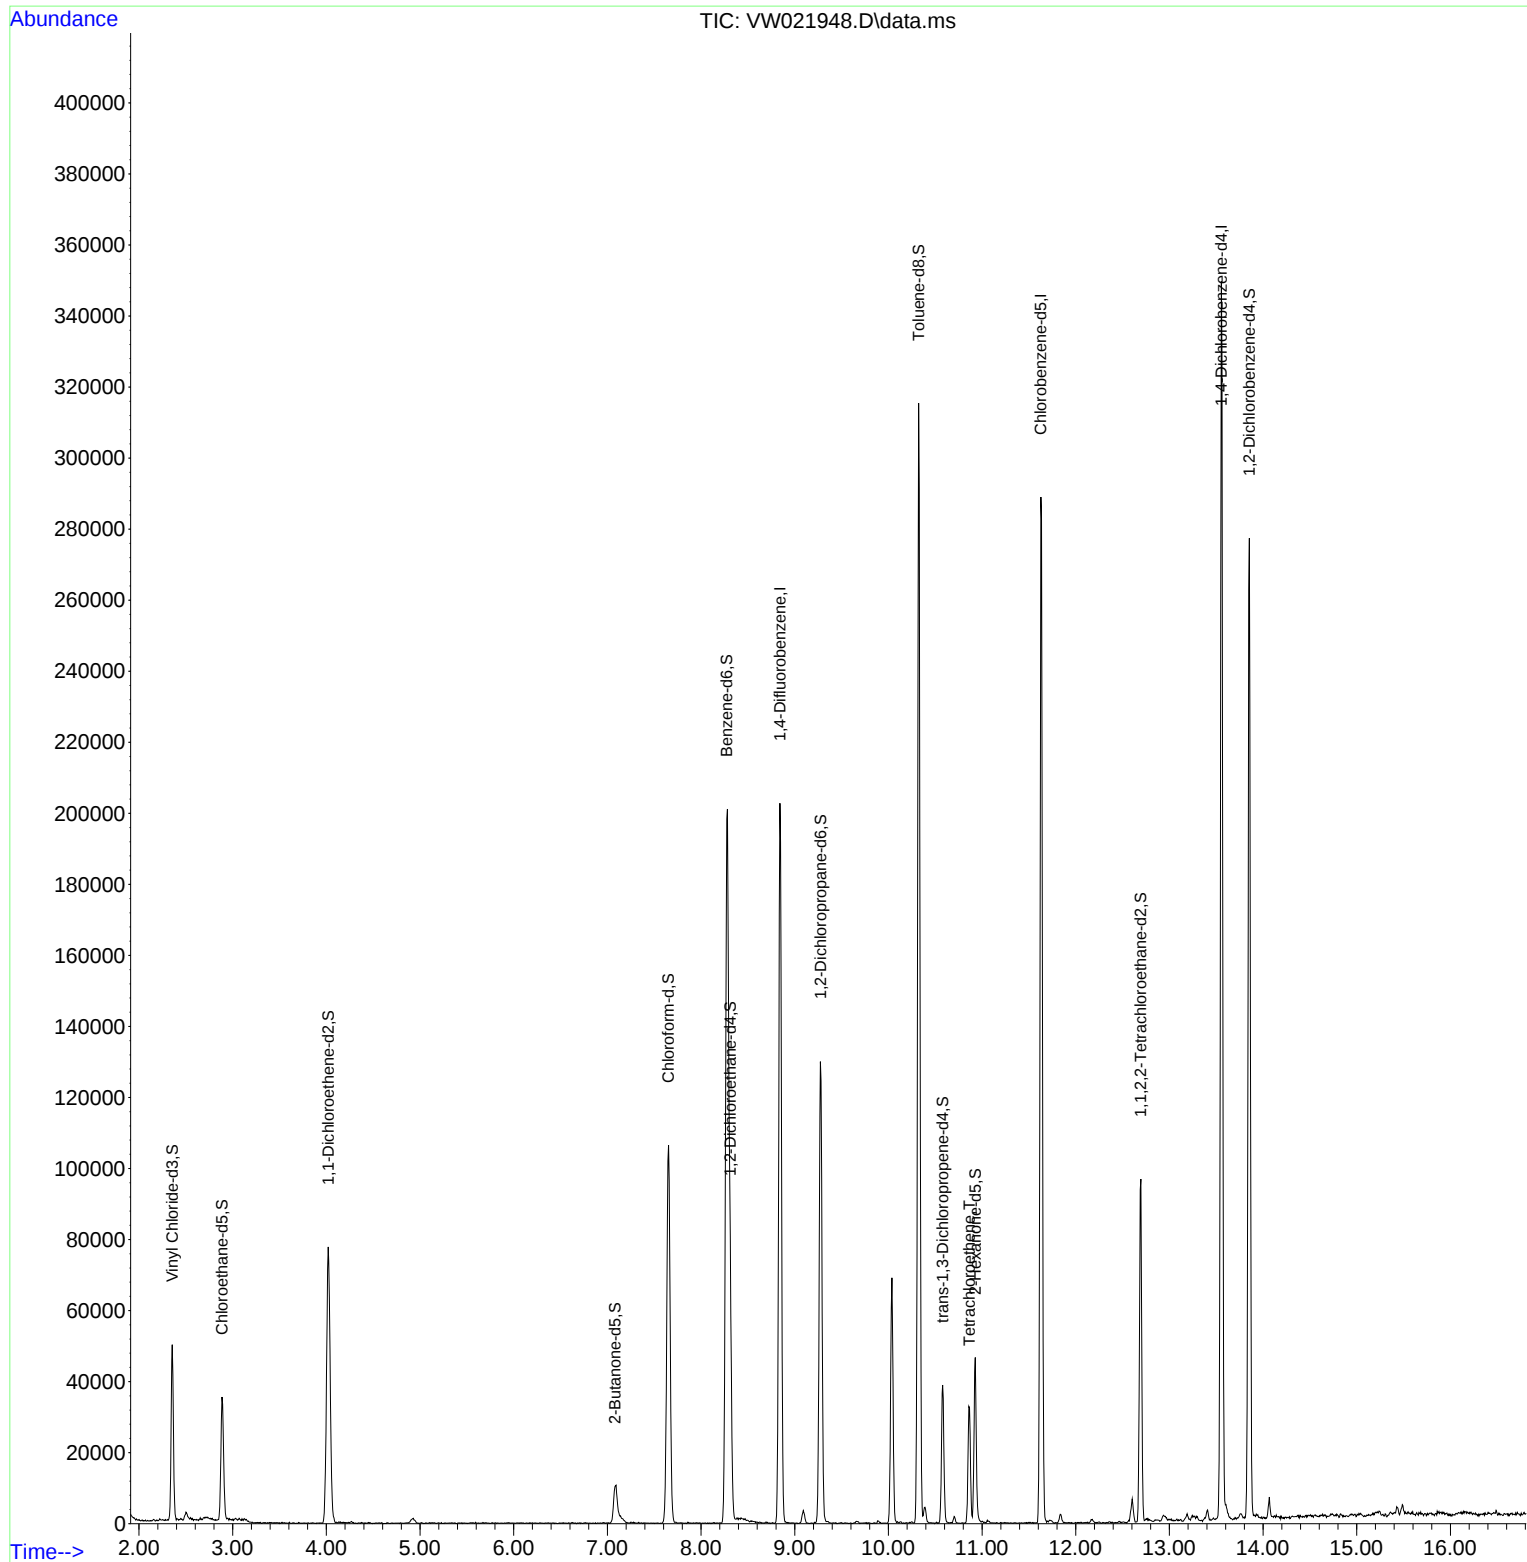

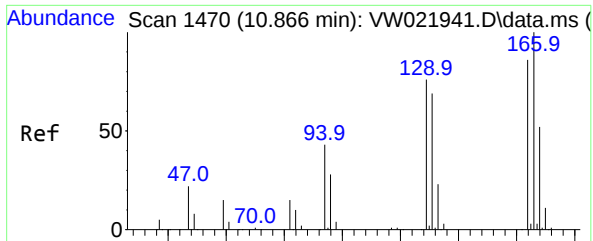

#46
 Tetrachloroethene
 Concen: 2.440 ug/L
 RT: 10.866 min Scan# 14
 Delta R.T. 0.000 min
 Lab File: VW021948.D
 Acq: 15 Jan 2022 16:40

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLX2

Tgt Ion:164 Resp: 7680

Ion	Ratio	Lower	Upper
164	100		
129	91.3	65.5	121.7
131	86.8	59.7	110.9
166	117.4	88.7	164.7

