

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011622\
 Data File : VW021950.D
 Acq On : 15 Jan 2022 17:27
 Operator : SY/VA
 Sample : N1168-08
 Misc : 5.49g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLX4

Quant Time: Jan 17 06:41:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 06:38:36 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	184703	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	179417	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	99655	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	43646	12.714	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	50.840%
7) Chloroethane-d5	2.885	69	32852	10.597	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	42.400%
11) 1,1-Dichloroethene-d2	4.019	63	65749	12.131	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	48.520%
21) 2-Butanone-d5	7.086	46	21344	44.049	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.100%
24) Chloroform-d	7.653	84	105497	17.680	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	70.720%
26) 1,2-Dichloroethane-d4	8.311	65	55086	19.117	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	76.480%
32) Benzene-d6	8.275	84	210448	18.077	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	72.320%
36) 1,2-Dichloropropane-d6	9.274	67	57679	18.797	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	75.200%
41) Toluene-d8	10.323	98	203508	17.341	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	69.360%
43) trans-1,3-Dichloroprop...	10.579	79	23125	17.750	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.000%
47) 2-Hexanone-d5	10.927	63	19139	45.966	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.940%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	47841	19.938	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.760%
66) 1,2-Dichlorobenzene-d4	13.853	152	80269	19.589	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.360%
Target Compounds						Qvalue
46) Tetrachloroethene	10.866	164	2868	0.909	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011622\
Data File : VW021950.D
Acq On : 15 Jan 2022 17:27
Operator : SY/VA
Sample : N1168-08
Misc : 5.49g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLX4

Quant Time: Jan 17 06:41:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 17 06:38:36 2022
Response via : Initial Calibration

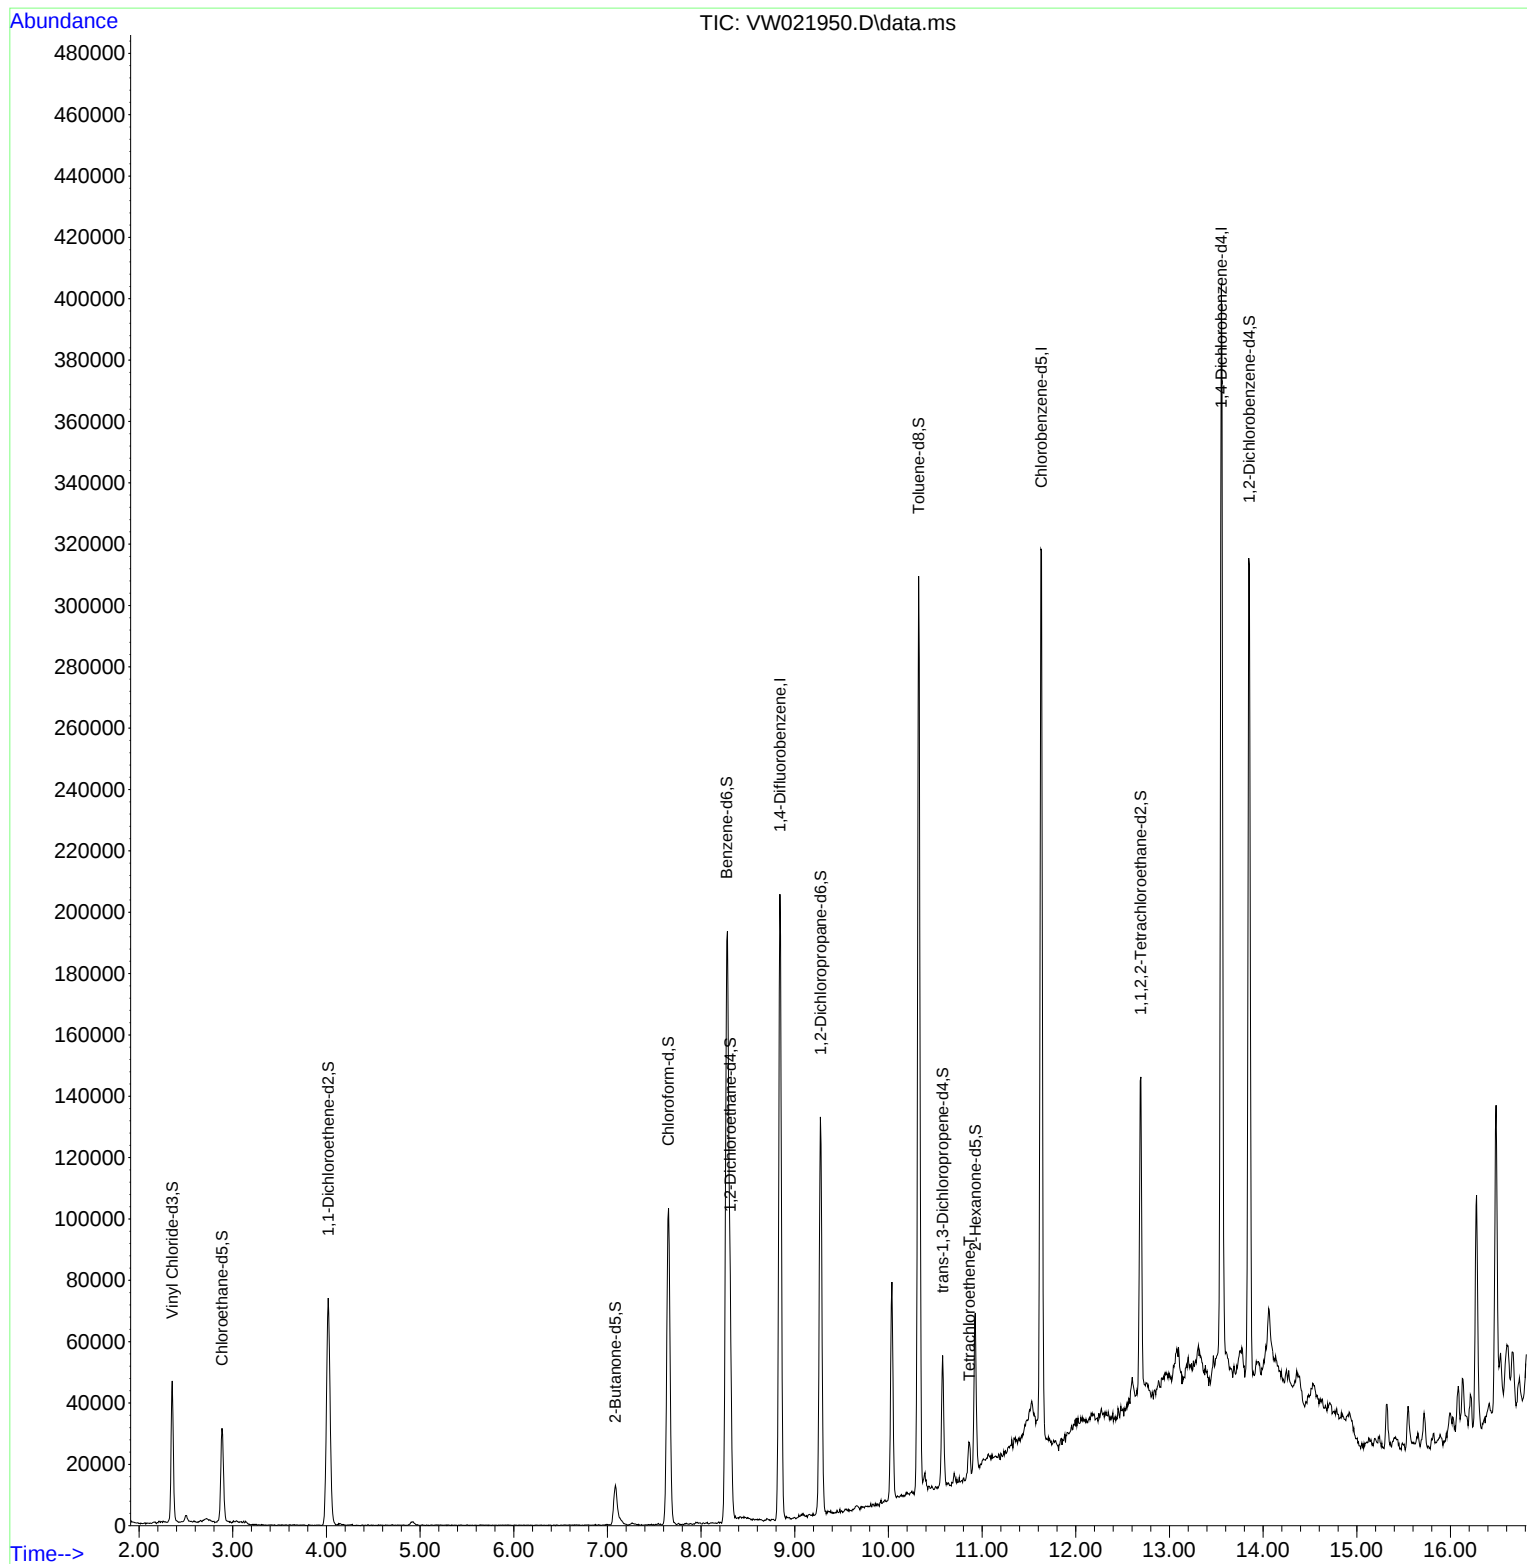

Abundance Scan 1470 (10.866 min): VW021941.D\data.ms (

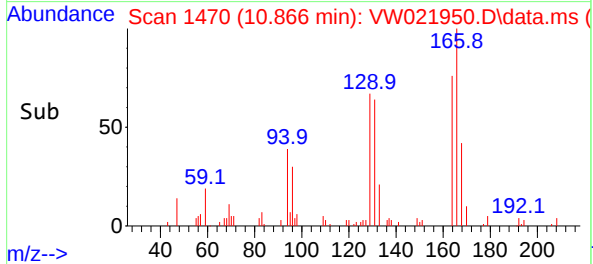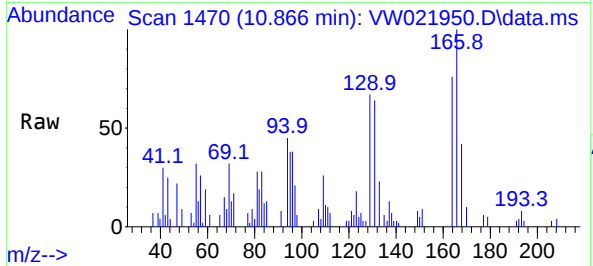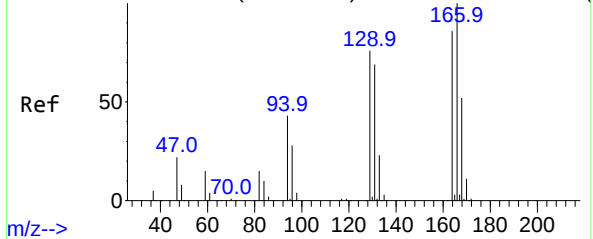

#46
Tetrachloroethene
Concen: 0.909 ug/L
RT: 10.866 min Scan# 14
Delta R.T. 0.000 min
Lab File: VW021950.D
Acq: 15 Jan 2022 17:27

Instrument :
MSVOA_W
ClientSampleId :
BGLX4

Tgt Ion:164	Resp:	2868
Ion	Ratio	Lower Upper
164	100	
129	87.1	65.5 121.7
131	83.3	59.7 110.9
166	130.8	88.7 164.7

