

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011723\
 Data File : VW025232.D
 Acq On : 17 Jan 2023 14:36
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK403

Quant Time: Jan 18 00:52:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 18 00:51:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	344475	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	300144	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	149635	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	65877	16.472	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.880%
7) Chloroethane-d5	2.885	69	42260	16.771	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.080%
11) 1,1-Dichloroethene-d2	4.013	63	136948	15.635	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.520%
21) 2-Butanone-d5	7.074	46	40140	39.603	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.200%
24) Chloroform-d	7.647	84	198340	22.973	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.880%
26) 1,2-Dichloroethane-d4	8.305	65	110967	24.952	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.800%
32) Benzene-d6	8.275	84	404262	22.430	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.720%
36) 1,2-Dichloropropane-d6	9.275	67	111278	21.107	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.440%
41) Toluene-d8	10.323	98	372361	22.701	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.800%
43) trans-1,3-Dichloroprop...	10.579	79	50122	22.202	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.800%
47) 2-Hexanone-d5	10.921	63	32880	39.578	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.160%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	81425	22.084	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	120307	22.629	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.520%
Target Compounds					Qvalue	
34) Trichloroethene	8.842	95	11197	2.366	ug/L	# 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011723\
Data File : VW025232.D
Acq On : 17 Jan 2023 14:36
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK403


Quant Time: Jan 18 00:52:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 18 00:51:50 2023
Response via : Initial Calibration

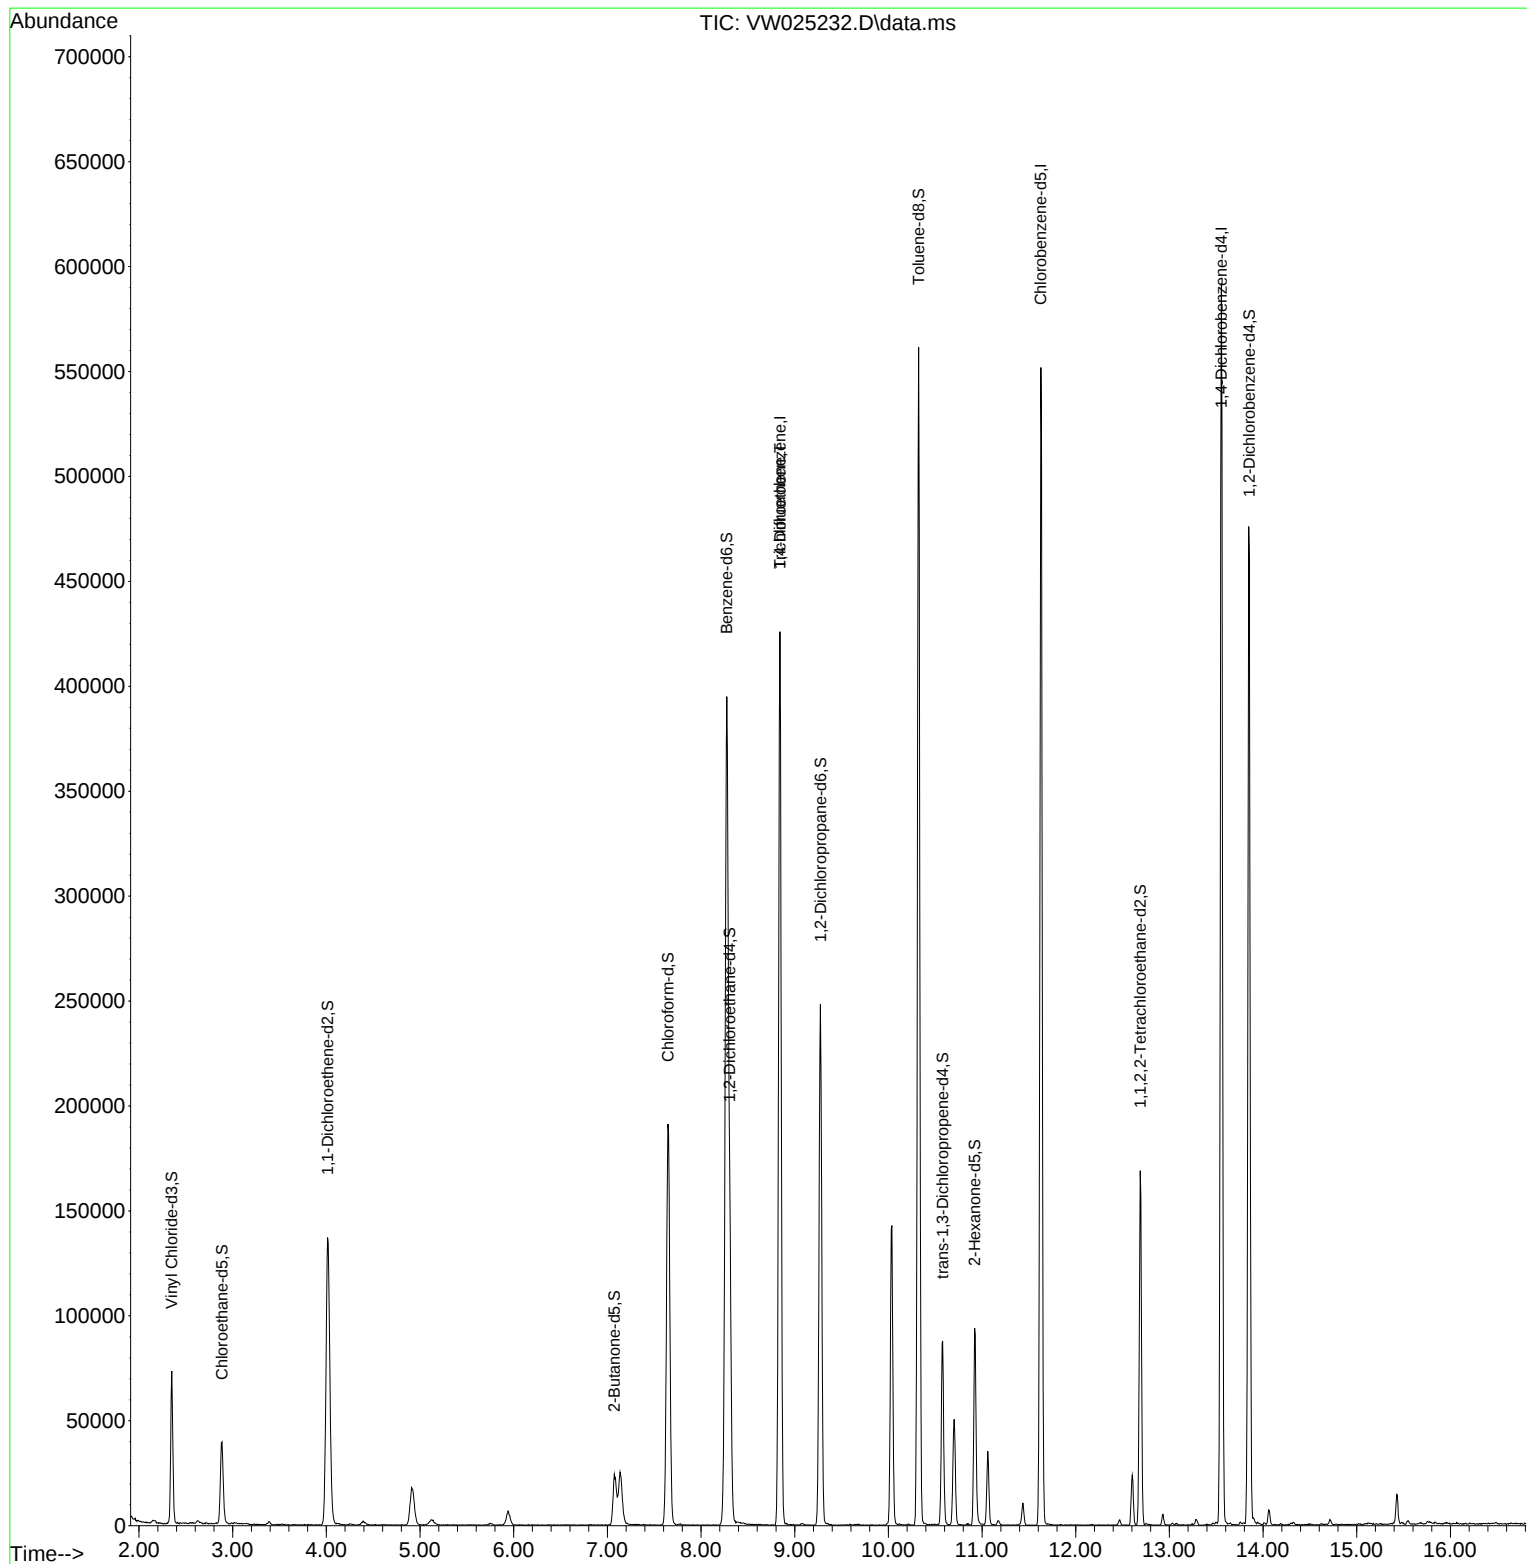

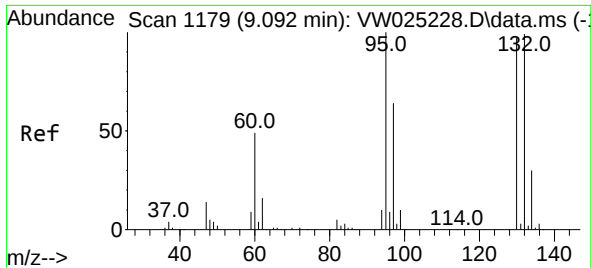

#34
 Trichloroethene
 Concen: 2.366 ug/L
 RT: 8.842 min Scan# 1179
 Delta R.T. -0.250 min
 Lab File: VW025232.D
 Acq: 17 Jan 2023 14:36

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK403

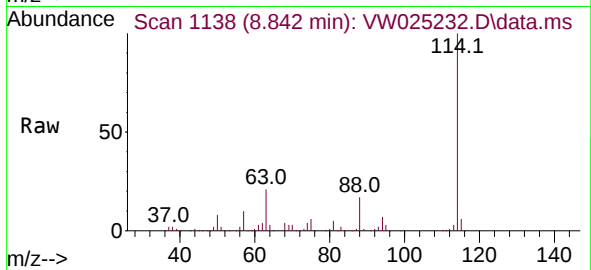

Tgt Ion: 95 Resp: 11197

Ion	Ratio	Lower	Upper
95	100		
97	0.0	44.4	82.4#
132	0.0	64.5	119.7#
130	0.0	66.8	124.0#

