

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011723\
 Data File : VW025232.D
 Acq On : 17 Jan 2023 14:36
 Operator : SY/MD
 Sample : VIBLK403
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK403

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
 Title : SFAM01.0

Signal : TIC: VW025232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.349	67	73	82	rVB	72582	113803	9.69%	1.336%
2	2.885	154	161	173	rVB	39088	83781	7.13%	0.984%
3	3.013	180	182	184	rBV2	647	583	0.05%	0.007%
4	3.367	237	240	241	rBV3	663	736	0.06%	0.009%
5	3.519	263	265	268	rBV3	393	447	0.04%	0.005%
6	3.769	305	306	307	rBV	337	130	0.01%	0.002%
7	3.922	329	331	332	rBV	234	168	0.01%	0.002%
8	4.013	335	346	361	rVV	136928	390529	33.25%	4.586%
9	4.391	401	408	410	rBV	1763	3034	0.26%	0.036%
10	4.507	426	427	428	rBV	278	135	0.01%	0.002%
11	4.525	428	430	434	rVB	323	310	0.03%	0.004%
12	4.909	483	493	511	rVV	17765	57033	4.86%	0.670%
13	5.123	515	528	545	rBV2	2613	10455	0.89%	0.123%
14	5.275	551	553	554	rVB	258	138	0.01%	0.002%
15	5.623	609	610	613	rBV	258	308	0.03%	0.004%
16	5.806	639	640	643	rBV	190	226	0.02%	0.003%
17	5.940	653	662	671	rVB4	6642	18203	1.55%	0.214%
18	6.141	694	695	697	rBV	198	179	0.02%	0.002%
19	6.196	702	704	706	rBV	249	146	0.01%	0.002%
20	6.373	731	733	735	rBV	225	145	0.01%	0.002%
21	6.580	765	767	768	rBV	224	174	0.01%	0.002%
22	6.781	798	800	801	rBV	216	155	0.01%	0.002%
23	6.812	801	805	806	rVV	248	288	0.02%	0.003%
24	6.854	810	812	813	rBV	234	140	0.01%	0.002%
25	6.946	824	827	830	rVB	245	246	0.02%	0.003%
26	6.976	830	832	836	rBV2	334	353	0.03%	0.004%
27	7.074	841	848	853	rBV	23955	60609	5.16%	0.712%
28	7.452	906	910	911	rVV2	174	170	0.01%	0.002%
29	7.647	932	942	956	rBV	191097	476454	40.57%	5.595%
30	7.805	967	968	971	rVB2	223	184	0.02%	0.002%
31	7.909	982	985	987	rVB2	235	218	0.02%	0.003%
32	7.958	989	993	994	rBV2	176	255	0.02%	0.003%
33	8.006	999	1001	1005	rVV	177	176	0.01%	0.002%
34	8.159	1025	1026	1029	rVB	273	217	0.02%	0.003%
35	8.275	1031	1045	1061	rBV2	394814	1174476	100.00%	13.792%
36	8.842	1130	1138	1149	rBV	425728	827630	70.47%	9.719%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011723\
 Data File : VW025232.D
 Acq On : 17 Jan 2023 14:36
 Operator : SY/MD
 Sample : VIBLK403
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK403

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
 Title : SFAM01.0

37	8.958	1155	1157	1158	rVB	382	227	0.02%	0.003%
38	8.976	1158	1160	1161	rBV	197	207	0.02%	0.002%
39	9.049	1170	1172	1173	rBV	253	186	0.02%	0.002%
40	9.067	1173	1175	1176	rBV	633	555	0.05%	0.007%

41	9.275	1198	1209	1219	rBV	248193	501501	42.70%	5.889%
42	9.470	1238	1241	1242	rBV	227	201	0.02%	0.002%
43	9.488	1242	1244	1246	rBV2	158	159	0.01%	0.002%
44	9.592	1258	1261	1265	rBV3	465	599	0.05%	0.007%
45	9.659	1266	1272	1273	rBV2	381	659	0.06%	0.008%

46	9.951	1317	1320	1322	rBV2	199	233	0.02%	0.003%
47	10.037	1323	1334	1342	rBV	142688	260837	22.21%	3.063%
48	10.323	1372	1381	1390	rBV	561280	991227	84.40%	11.640%
49	10.463	1402	1404	1405	rBV2	403	243	0.02%	0.003%
50	10.579	1415	1423	1433	rVB	87558	154178	13.13%	1.811%

51	10.701	1436	1443	1451	rVB2	50159	91101	7.76%	1.070%
52	10.841	1461	1466	1467	rBV2	729	830	0.07%	0.010%
53	10.921	1472	1479	1492	rVV	93899	162766	13.86%	1.911%
54	11.061	1496	1502	1512	rVV2	35194	55848	4.76%	0.656%
55	11.171	1515	1520	1525	rBV4	2145	3624	0.31%	0.043%

56	11.439	1554	1564	1570	rBV	10423	17832	1.52%	0.209%
57	11.542	1577	1581	1583	rBV2	219	434	0.04%	0.005%
58	11.628	1587	1595	1606	rBV	551620	934291	79.55%	10.972%
59	11.835	1627	1629	1634	rVB2	432	564	0.05%	0.007%
60	11.890	1634	1638	1639	rBV2	169	207	0.02%	0.002%

61	11.933	1644	1645	1647	rBV	269	223	0.02%	0.003%
62	12.000	1655	1656	1658	rBV2	229	129	0.01%	0.002%
63	12.079	1668	1669	1671	rBV	191	136	0.01%	0.002%
64	12.152	1680	1681	1682	rBV	246	170	0.01%	0.002%
65	12.317	1706	1708	1710	rBV	212	152	0.01%	0.002%

66	12.347	1710	1713	1714	rBV	285	231	0.02%	0.003%
67	12.469	1728	1733	1740	rVV3	2551	3980	0.34%	0.047%
68	12.603	1748	1755	1761	rBV2	23831	39596	3.37%	0.465%
69	12.689	1762	1769	1777	rBV	168835	277243	23.61%	3.256%
70	12.750	1777	1779	1781	rBV3	678	691	0.06%	0.008%

71	12.865	1796	1798	1801	rBV2	176	176	0.01%	0.002%
72	12.932	1804	1809	1816	rVB2	5158	7706	0.66%	0.090%
73	13.030	1822	1825	1829	rBV5	916	1267	0.11%	0.015%
74	13.079	1829	1833	1835	rVB3	729	766	0.07%	0.009%
75	13.188	1849	1851	1856	rBV2	224	404	0.03%	0.005%

76	13.243	1858	1860	1862	rVV	731	625	0.05%	0.007%
----	--------	------	------	------	-----	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011723\
 Data File : VW025232.D
 Acq On : 17 Jan 2023 14:36
 Operator : SY/MD
 Sample : VIBLK403
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK403

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
 Title : SFAM01.0

77	13.280	1862	1866	1873	rVB4	2652	4717	0.40%	0.055%
78	13.402	1882	1886	1887	rBV3	407	416	0.04%	0.005%
79	13.463	1893	1896	1899	rBV2	956	1398	0.12%	0.016%
80	13.493	1899	1901	1904	rVV3	1190	1702	0.14%	0.020%
81	13.554	1904	1911	1922	rVB	591291	940027	80.04%	11.039%
82	13.755	1940	1944	1947	rBV5	1400	1907	0.16%	0.022%
83	13.847	1952	1959	1966	rBV	475169	783183	66.68%	9.197%
84	14.011	1983	1986	1989	rBV3	785	1066	0.09%	0.013%
85	14.060	1989	1994	2001	rVB2	7110	11676	0.99%	0.137%
86	14.188	2013	2015	2020	rVB4	790	918	0.08%	0.011%
87	14.243	2022	2024	2026	rBV2	275	234	0.02%	0.003%
88	14.268	2026	2028	2029	rVB	311	142	0.01%	0.002%
89	14.292	2030	2032	2035	rBV3	670	849	0.07%	0.010%
90	14.414	2051	2052	2055	rBV	289	260	0.02%	0.003%
91	14.481	2062	2063	2064	rBV	419	157	0.01%	0.002%
92	14.499	2064	2066	2067	rBV2	545	395	0.03%	0.005%
93	14.621	2083	2086	2090	rBV3	530	653	0.06%	0.008%
94	14.713	2097	2101	2108	rVB4	2399	3672	0.31%	0.043%
95	14.969	2141	2143	2146	rBV3	263	275	0.02%	0.003%
96	15.024	2150	2152	2153	rBV2	502	482	0.04%	0.006%
97	15.121	2166	2168	2176	rVV4	720	1389	0.12%	0.016%
98	15.176	2176	2177	2180	rVB2	458	205	0.02%	0.002%
99	15.426	2214	2218	2224	rVB3	13972	22229	1.89%	0.261%
100	15.548	2233	2238	2242	rBV4	1841	3196	0.27%	0.038%




Sum of corrected areas: 8515386

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011723\
Data File : VW025232.D
Acq On : 17 Jan 2023 14:36
Operator : SY/MD
Sample : VIBLK403
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK403

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

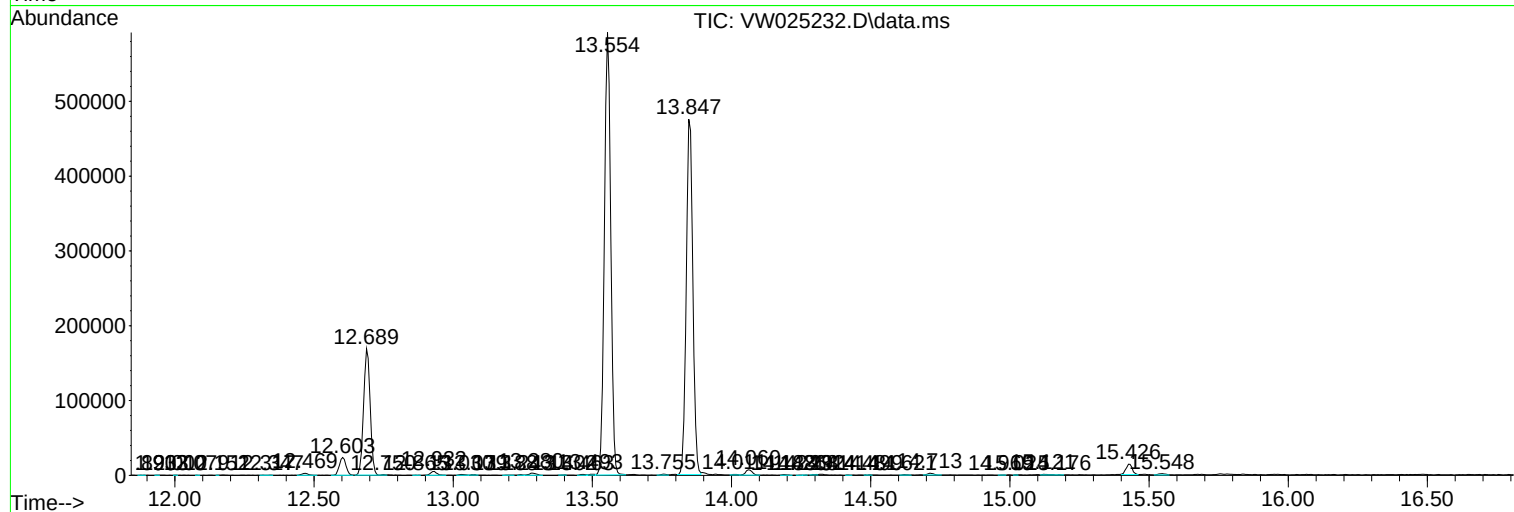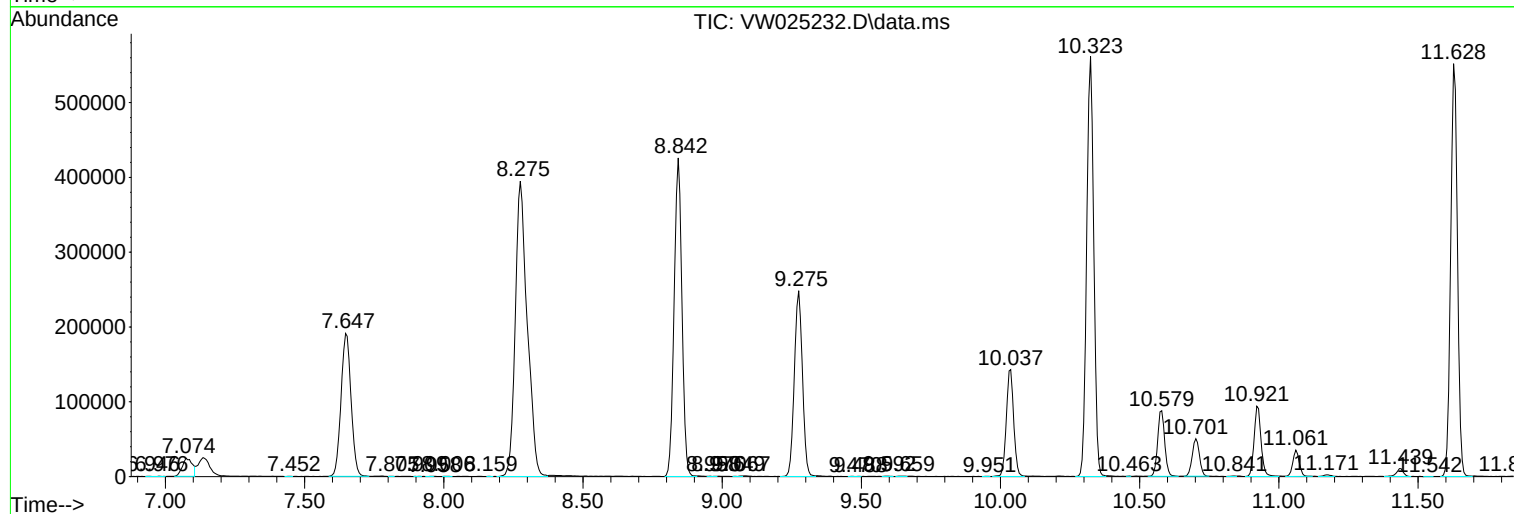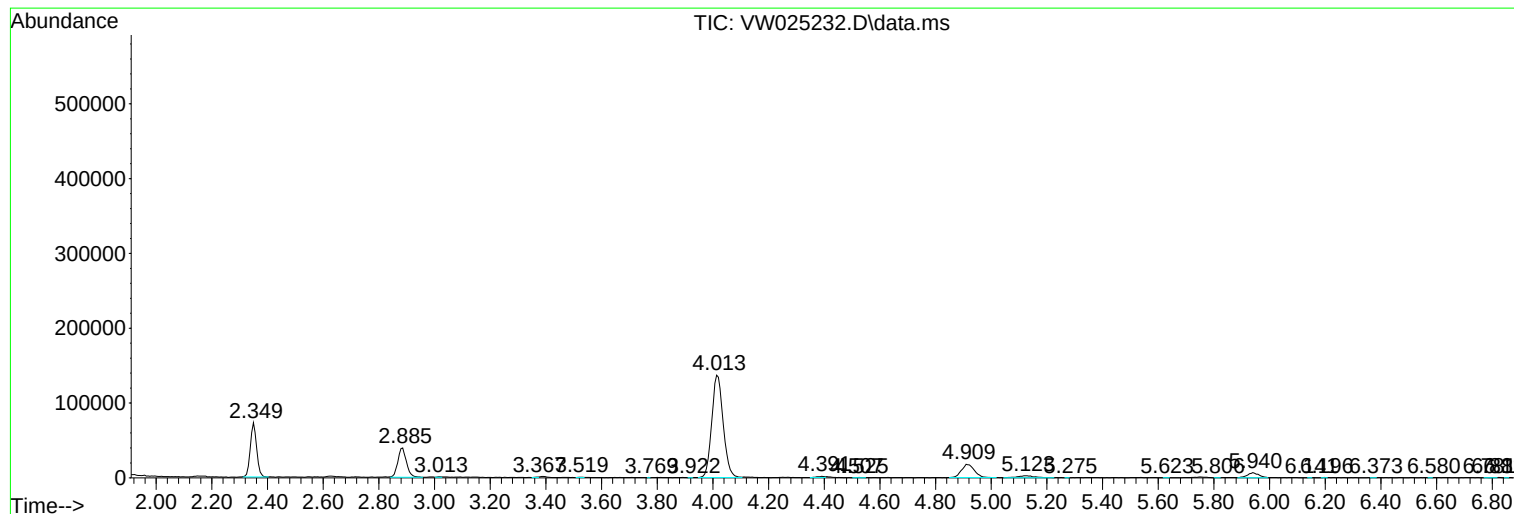

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011723\
Data File : VW025232.D
Acq On : 17 Jan 2023 14:36
Operator : SY/MD
Sample : VIBLK403
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK403

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011723\
Data File : VW025232.D
Acq On : 17 Jan 2023 14:36
Operator : SY/MD
Sample : VIBLK403
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK403

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
Quant Title : SFAM01.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc