

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011725\
 Data File : VW031564.D
 Acq On : 17 Jan 2025 10:39
 Operator : SY/MD
 Sample : Q1108-09
 Misc : 3.28g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jan 18 00:37:35 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jan 18 00:35:19 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1057463	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	840736	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	232815	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	351289	21.170	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.680%
7) Chloroethane-d5	2.899	69	244416	20.625	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.520%
11) 1,1-Dichloroethene-d2	4.015	65	155802	21.103	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.400%
21) 2-Butanone-d5	7.093	46	96309	36.106	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.220%
24) Chloroform-d	7.648	84	543139	19.846	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.400%
26) 1,2-Dichloroethane-d4	8.300	65	263908	19.592	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	78.360%
32) Benzene-d6	8.276	84	1172611	22.204	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.800%
36) 1,2-Dichloropropane-d6	9.270	67	329995	21.164	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.640%
41) Toluene-d8	10.318	98	1016191	21.316	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.280%
43) trans-1,3-Dichloroprop...	10.574	79	128210	20.023	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.080%
47) 2-Hexanone-d5	10.922	63	61228	38.479	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.960%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	181665	19.052	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	76.200%
66) 1,2-Dichlorobenzene-d4	13.848	152	174360	21.353	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.400%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	9575	0.421	ug/L	# 54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011725\
Data File : VW031564.D
Acq On : 17 Jan 2025 10:39
Operator : SY/MD
Sample : Q1108-09
Misc : 3.28g/10mL/MSVOA_W/SOIL/A
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jan 18 00:37:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jan 18 00:35:19 2025
Response via : Initial Calibration

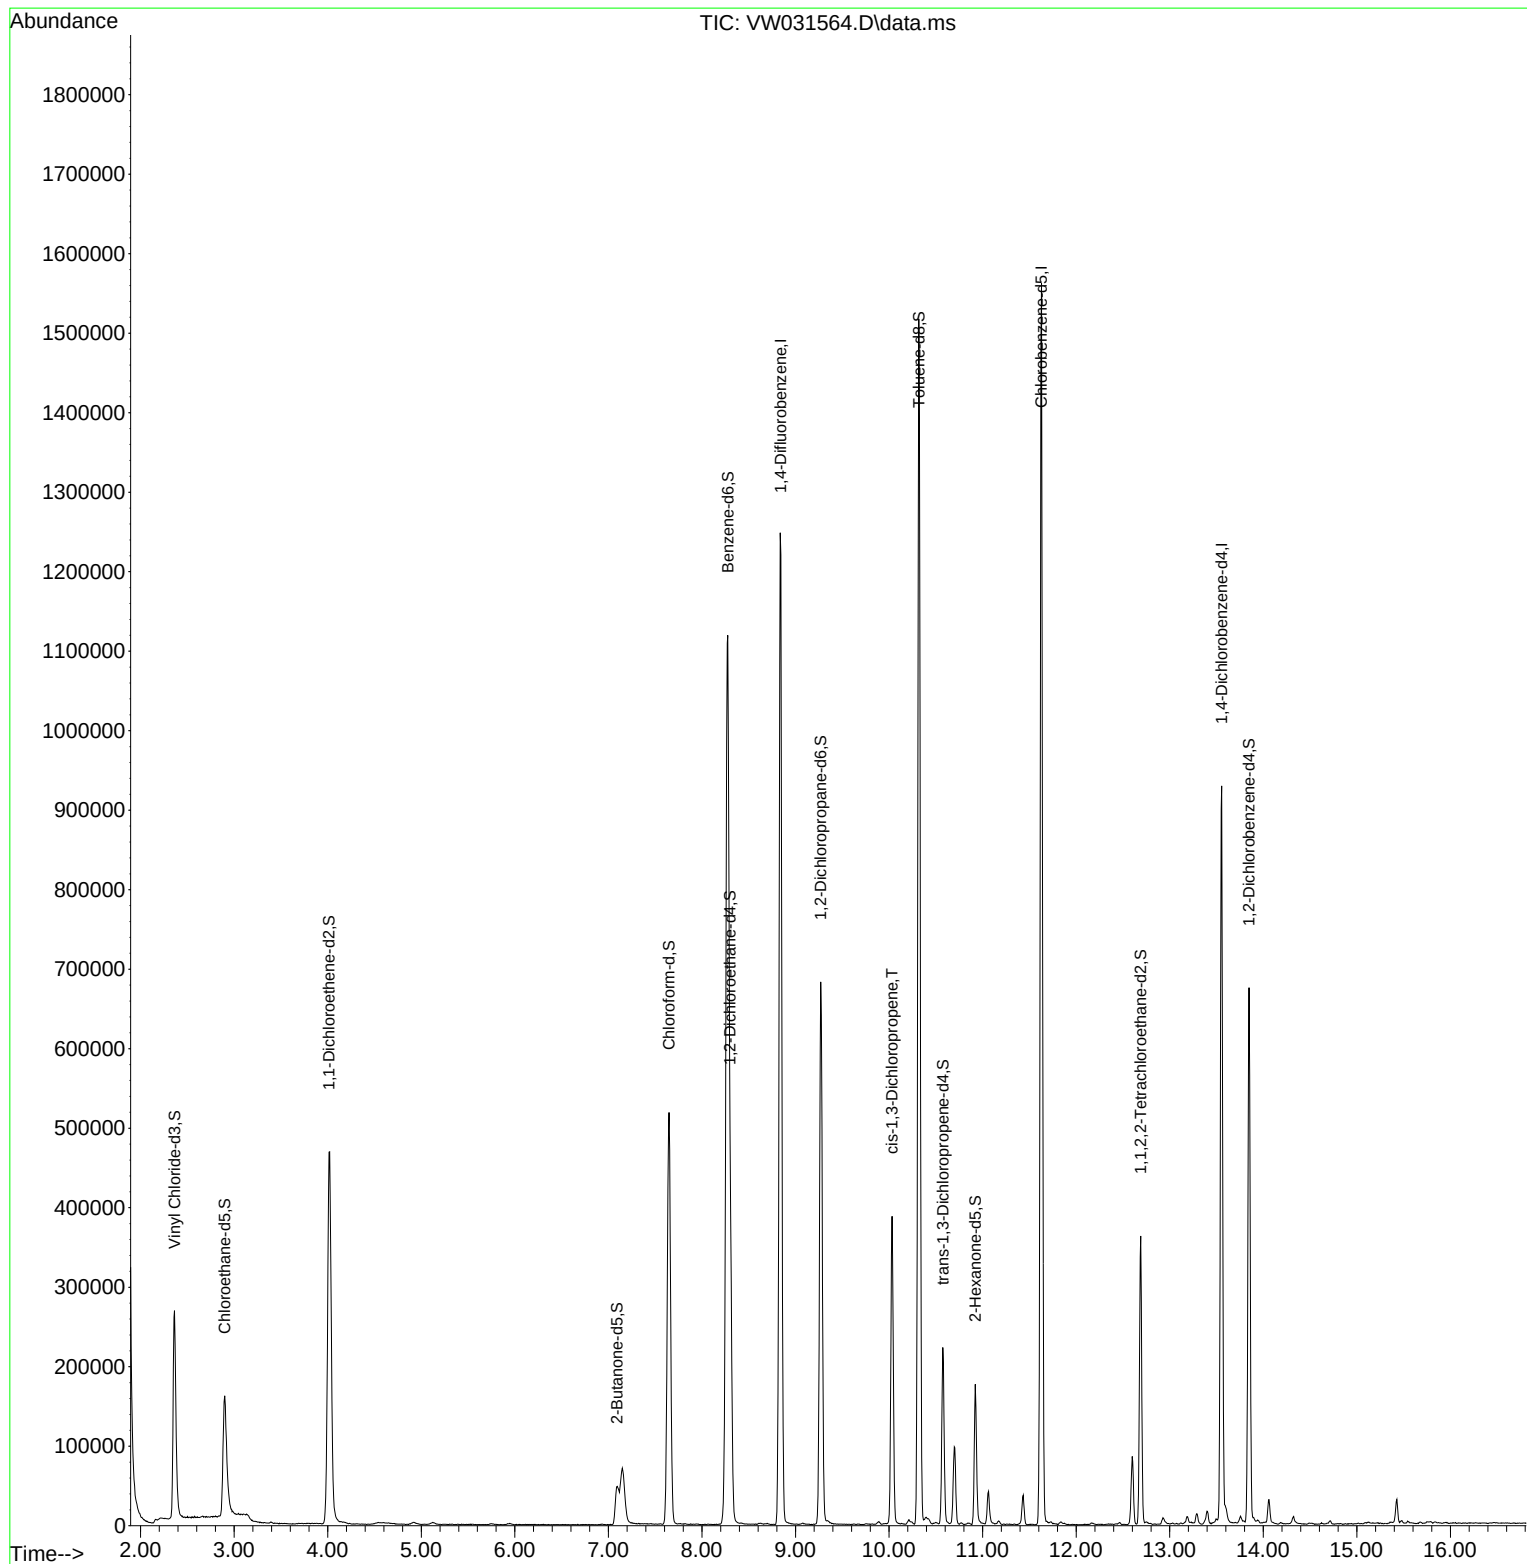

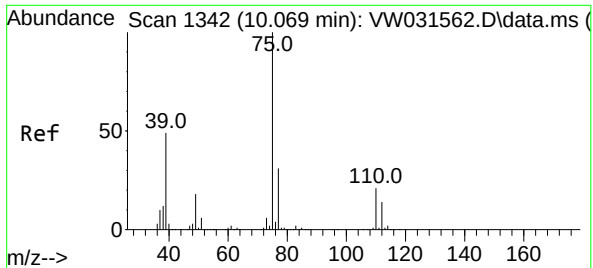

#39
 cis-1,3-Dichloropropene
 Concen: 0.421 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW031564.D
 Acq: 17 Jan 2025 10:39

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 9575
 Ion Ratio Lower Upper
 75 100
 77 56.1 21.6 40.2#

