




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011822\
Data File : VW021990.D
Acq On : 18 Jan 2022 11:00
Operator : SY/VA
Sample : N1129-06RE
Misc : 6.13g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBLZ9RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/19/2022
Supervised By :Mahesh Dadoda 01/19/2022

Quant Time: Jan 19 00:31:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 19 00:30:45 2022
Response via : Initial Calibration

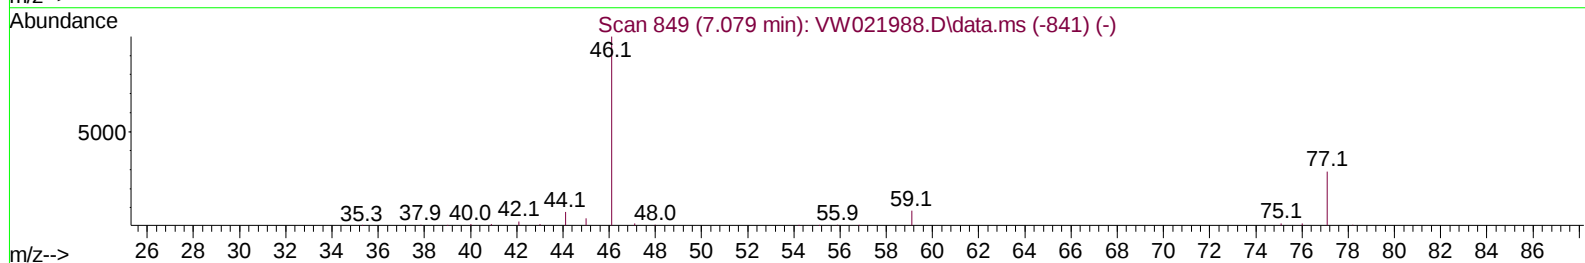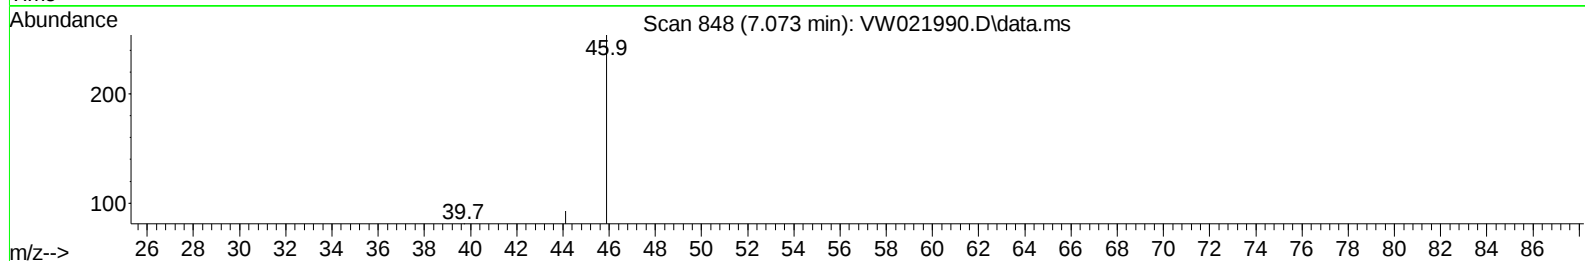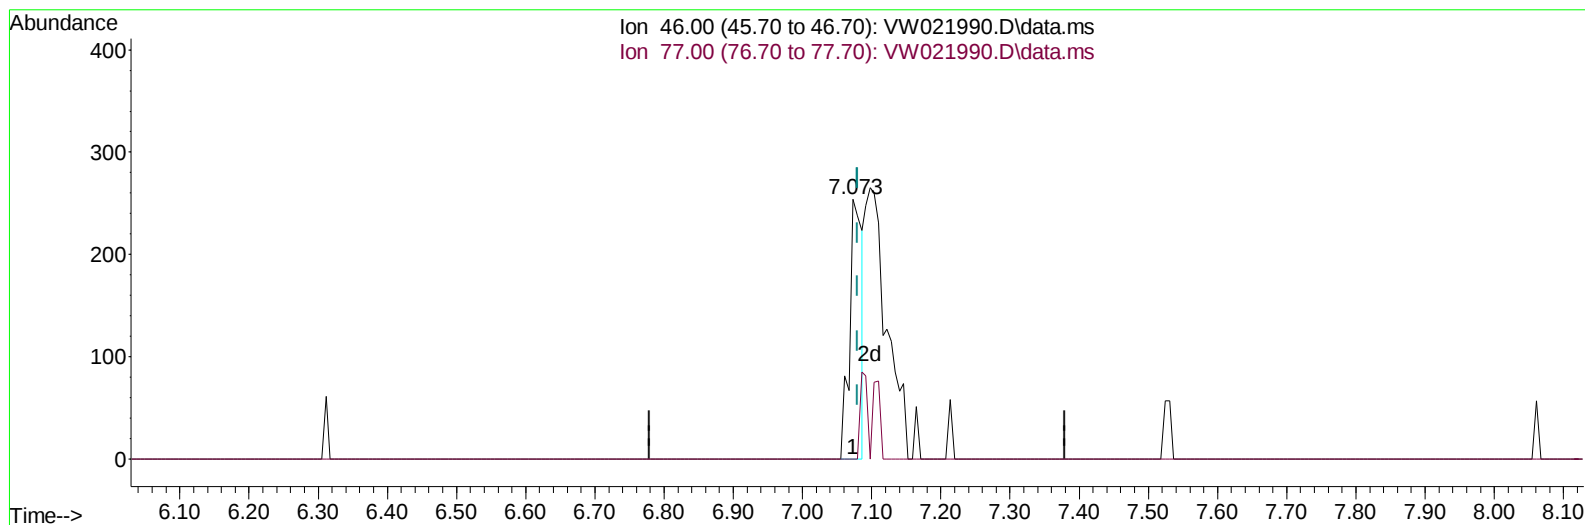

TIC: VW021990.D\data.ms

(21) 2-Butanone-d5 (S)

7.073min (-0.006) 12.94 ug/L

response 316

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	19.30
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011822\
 Data File : VW021990.D
 Acq On : 18 Jan 2022 11:00
 Operator : SY/VA
 Sample : N1129-06RE
 Misc : 6.13g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBLZ9RE

Manual IntegrationsAPPROVED

Quant Time: Jan 19 00:31:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 19 00:30:45 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/19/2022
 Supervised By :Mahesh Dadoda 01/19/2022

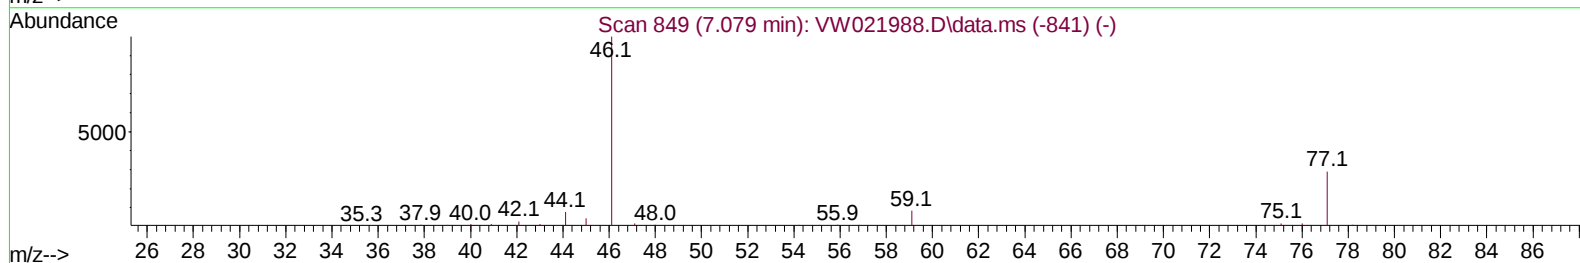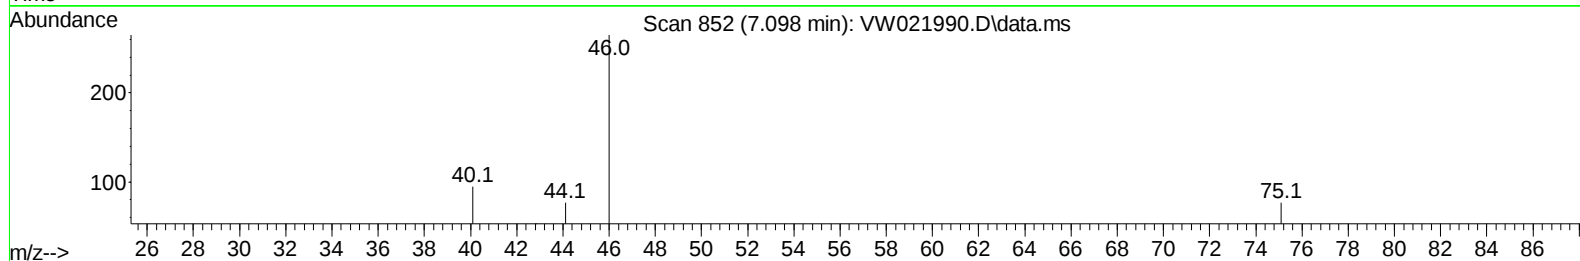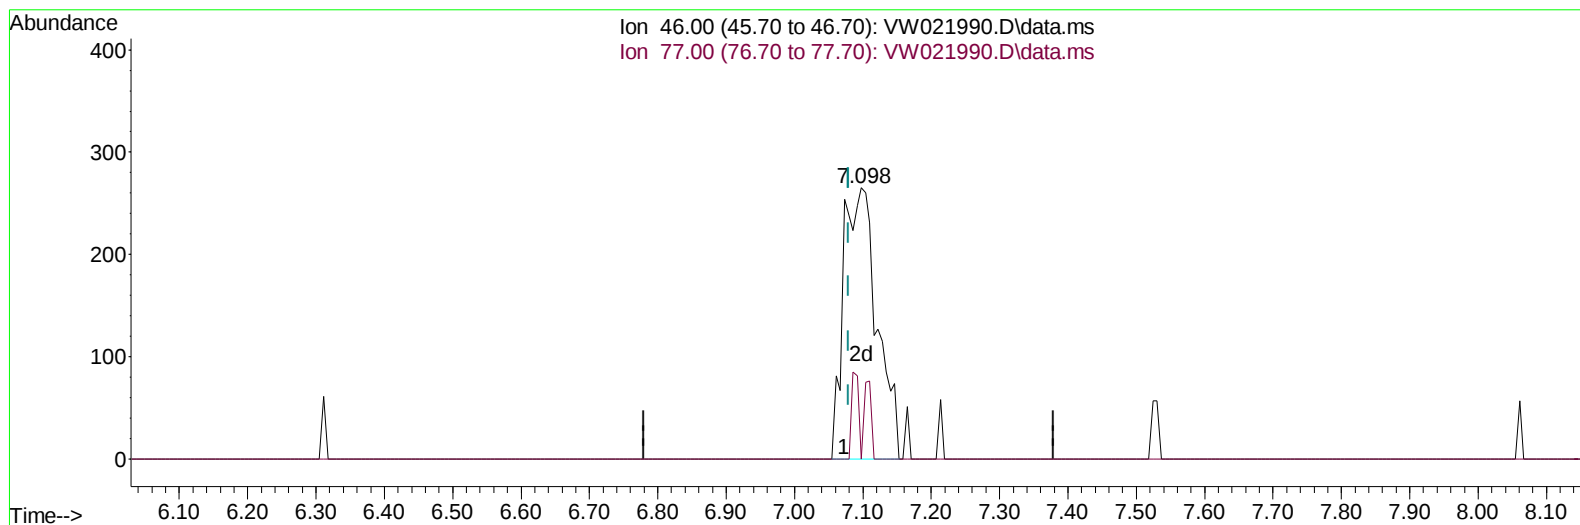

TIC: VW021990.D\data.ms

(21) 2-Butanone-d5 (S)

7.098min (+ 0.018) 36.78 ug/L m

response 898

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	6.79#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011822\
Data File : VW021990.D
Acq On : 18 Jan 2022 11:00
Operator : SY/VA
Sample : N1129-06RE
Misc : 6.13g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBLZ9RE

Manual IntegrationsAPPROVED

Quant Time: Jan 19 00:31:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 19 00:30:45 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/19/2022
Supervised By :Mahesh Dadoda 01/19/2022

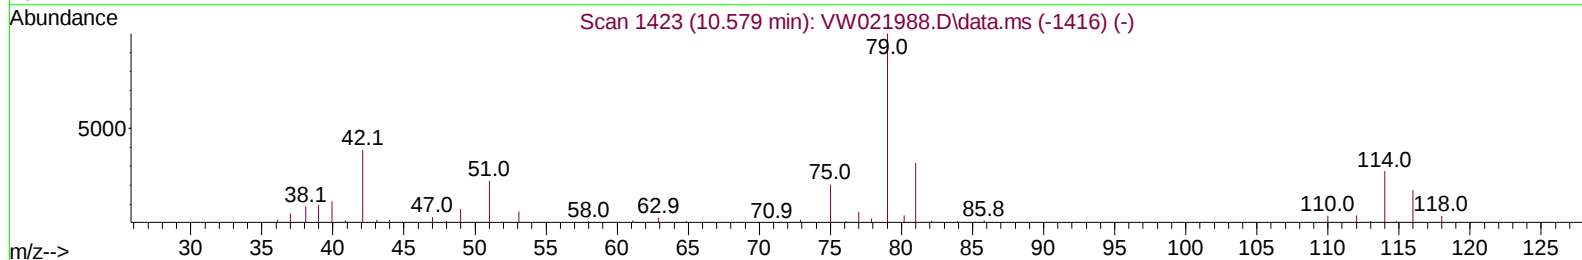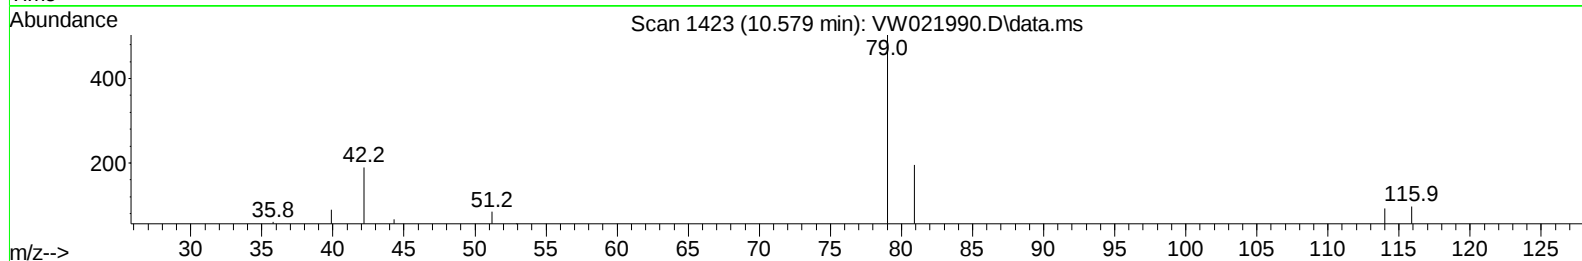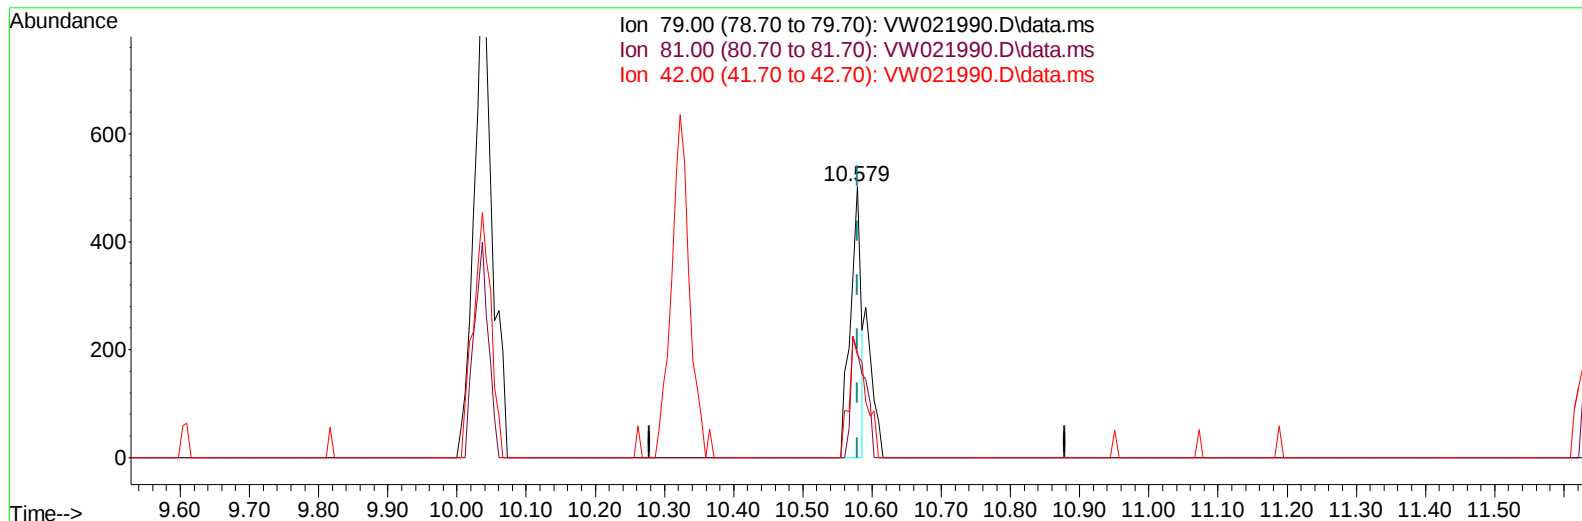

TIC: VW021990.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

10.579min (-0.000) 9.59 ug/L

response 525

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	32.00	60.95#
42.00	54.80	65.90
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011822\
Data File : VW021990.D
Acq On : 18 Jan 2022 11:00
Operator : SY/VA
Sample : N1129-06RE
Misc : 6.13g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBLZ9RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/19/2022
Supervised By :Mahesh Dadoda 01/19/2022

Quant Time: Jan 19 00:31:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 19 00:30:45 2022
Response via : Initial Calibration

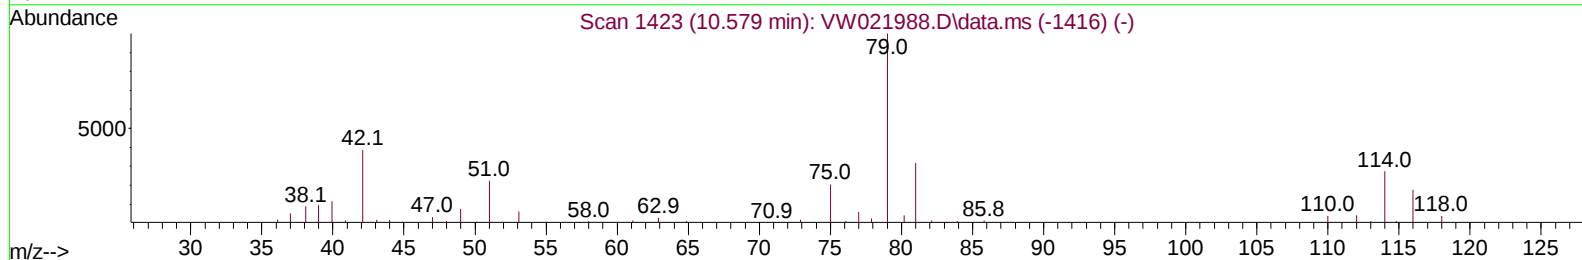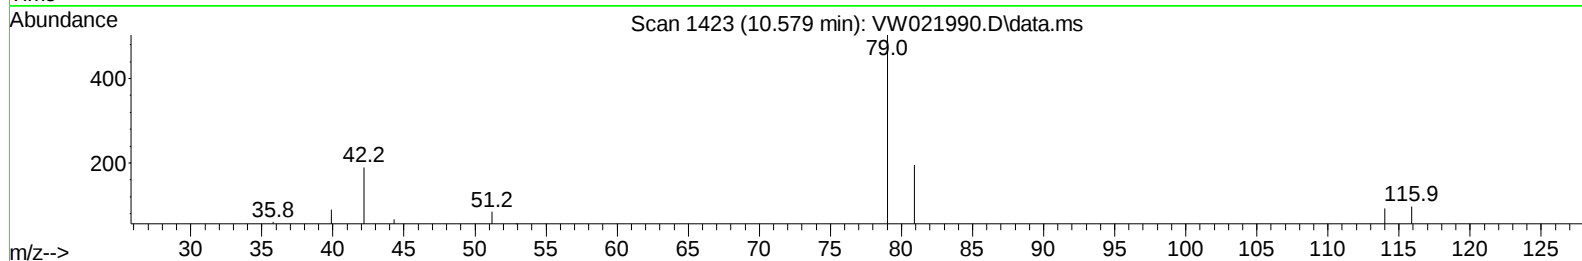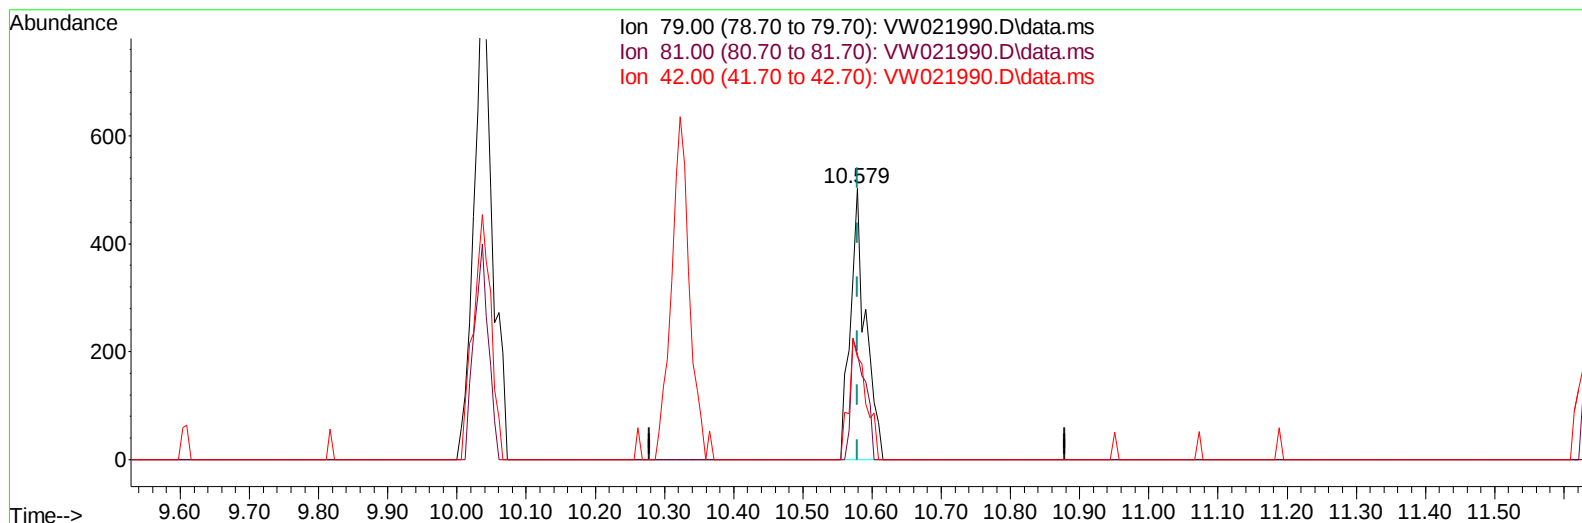

TIC: VW021990.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)**10.579min (-0.000) 13.90 ug/L m****response 761**

Ion	Exp%	Act%
79.00	100.00	100.00
81.00	32.00	42.05#
42.00	54.80	45.47
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011822\
 Data File : VW021990.D
 Acq On : 18 Jan 2022 11:00
 Operator : SY/VA
 Sample : N1129-06RE
 Misc : 6.13g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBLZ9RE

Manual IntegrationsAPPROVED

Quant Time: Jan 19 00:31:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 19 00:30:45 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/19/2022
 Supervised By :Mahesh Dadoda 01/19/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	9306	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.633	117	7538	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	2382	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	2900	16.766	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.080%	
7) Chloroethane-d5	2.891	69	2318	14.841	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	59.360%	
11) 1,1-Dichloroethene-d2	4.037	63	4125	15.106	ug/L	0.02
Spiked Amount 25.000	Range 45	- 110	Recovery	=	60.440%	
21) 2-Butanone-d5	7.098	46	898m	36.783	ug/L	0.02
Spiked Amount 50.000	Range 20	- 135	Recovery	=	73.560%	
24) Chloroform-d	7.652	84	6402	21.295	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	85.160%	
26) 1,2-Dichloroethane-d4	8.305	65	3457	23.812	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	95.240%	
32) Benzene-d6	8.280	84	12222	24.988	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	99.960%	
36) 1,2-Dichloropropane-d6	9.274	67	3524	27.335	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	109.320%	
41) Toluene-d8	10.323	98	9806	19.888	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	79.560%	
43) trans-1,3-Dichloroprop...	10.579	79	761m	13.903	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	55.600%	
47) 2-Hexanone-d5	10.926	63	183	10.461	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	20.920%	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	1874	18.589	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	74.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	1706	17.418	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	69.680%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011822\
Data File : VW021990.D
Acq On : 18 Jan 2022 11:00
Operator : SY/VA
Sample : N1129-06RE
Misc : 6.13g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBLZ9RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/19/2022
Supervised By :Mahesh Dadoda 01/19/2022

Quant Time: Jan 19 00:31:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 19 00:30:45 2022
Response via : Initial Calibration

