

Data Path : W:\HPCHEM1\MSVOA W\DATA\VW012418\
 Data File : VW000946.D
 Acq On : 24 Jan 2018 14:27
 Operator : JC/SY
 Sample : J1187-07RE
 Misc : 5.77G/5.0ML/MSVOA W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EPE-106-4A(65-67)RE

Quant Time: Jan 24 15:26:06 2018
 Quant Method : W:\HPCHEM1\MSVOA_W\METHOD\82W012318S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jan 23 13:31:00 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	146698	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	220601	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.65	117	188226	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.58	152	75450	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	88887	63.22	ug/l	0.00
Spiked Amount 50.000			Recovery	=	126.44%	
35) Dibromofluoromethane	7.88	113	62617	46.33	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.66%	
50) Toluene-d8	10.34	98	278982	52.36	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.72%	
62) 4-Bromofluorobenzene	12.63	95	79740	41.10	ug/l	0.00
Spiked Amount 50.000			Recovery	=	82.20%	
Target Compounds						
16) Acetone	4.14	43	6435	27.67	ug/l	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA W\DATA\VW012418\
Data File : VW000946.D
Acq On : 24 Jan 2018 14:27
Operator : JC/SY
Sample : J1187-07RE
Misc : 5.77G/5.0ML/MSVOA W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EPE-106-4A(65-67)RE

Quant Time: Jan 24 15:26:06 2018
Quant Method : W:\HPCHEM1\MSVOA_W\METHOD\82W012318S.M
Quant Title : SW846 8260
QLast Update : Tue Jan 23 13:31:00 2018
Response via : Initial Calibration

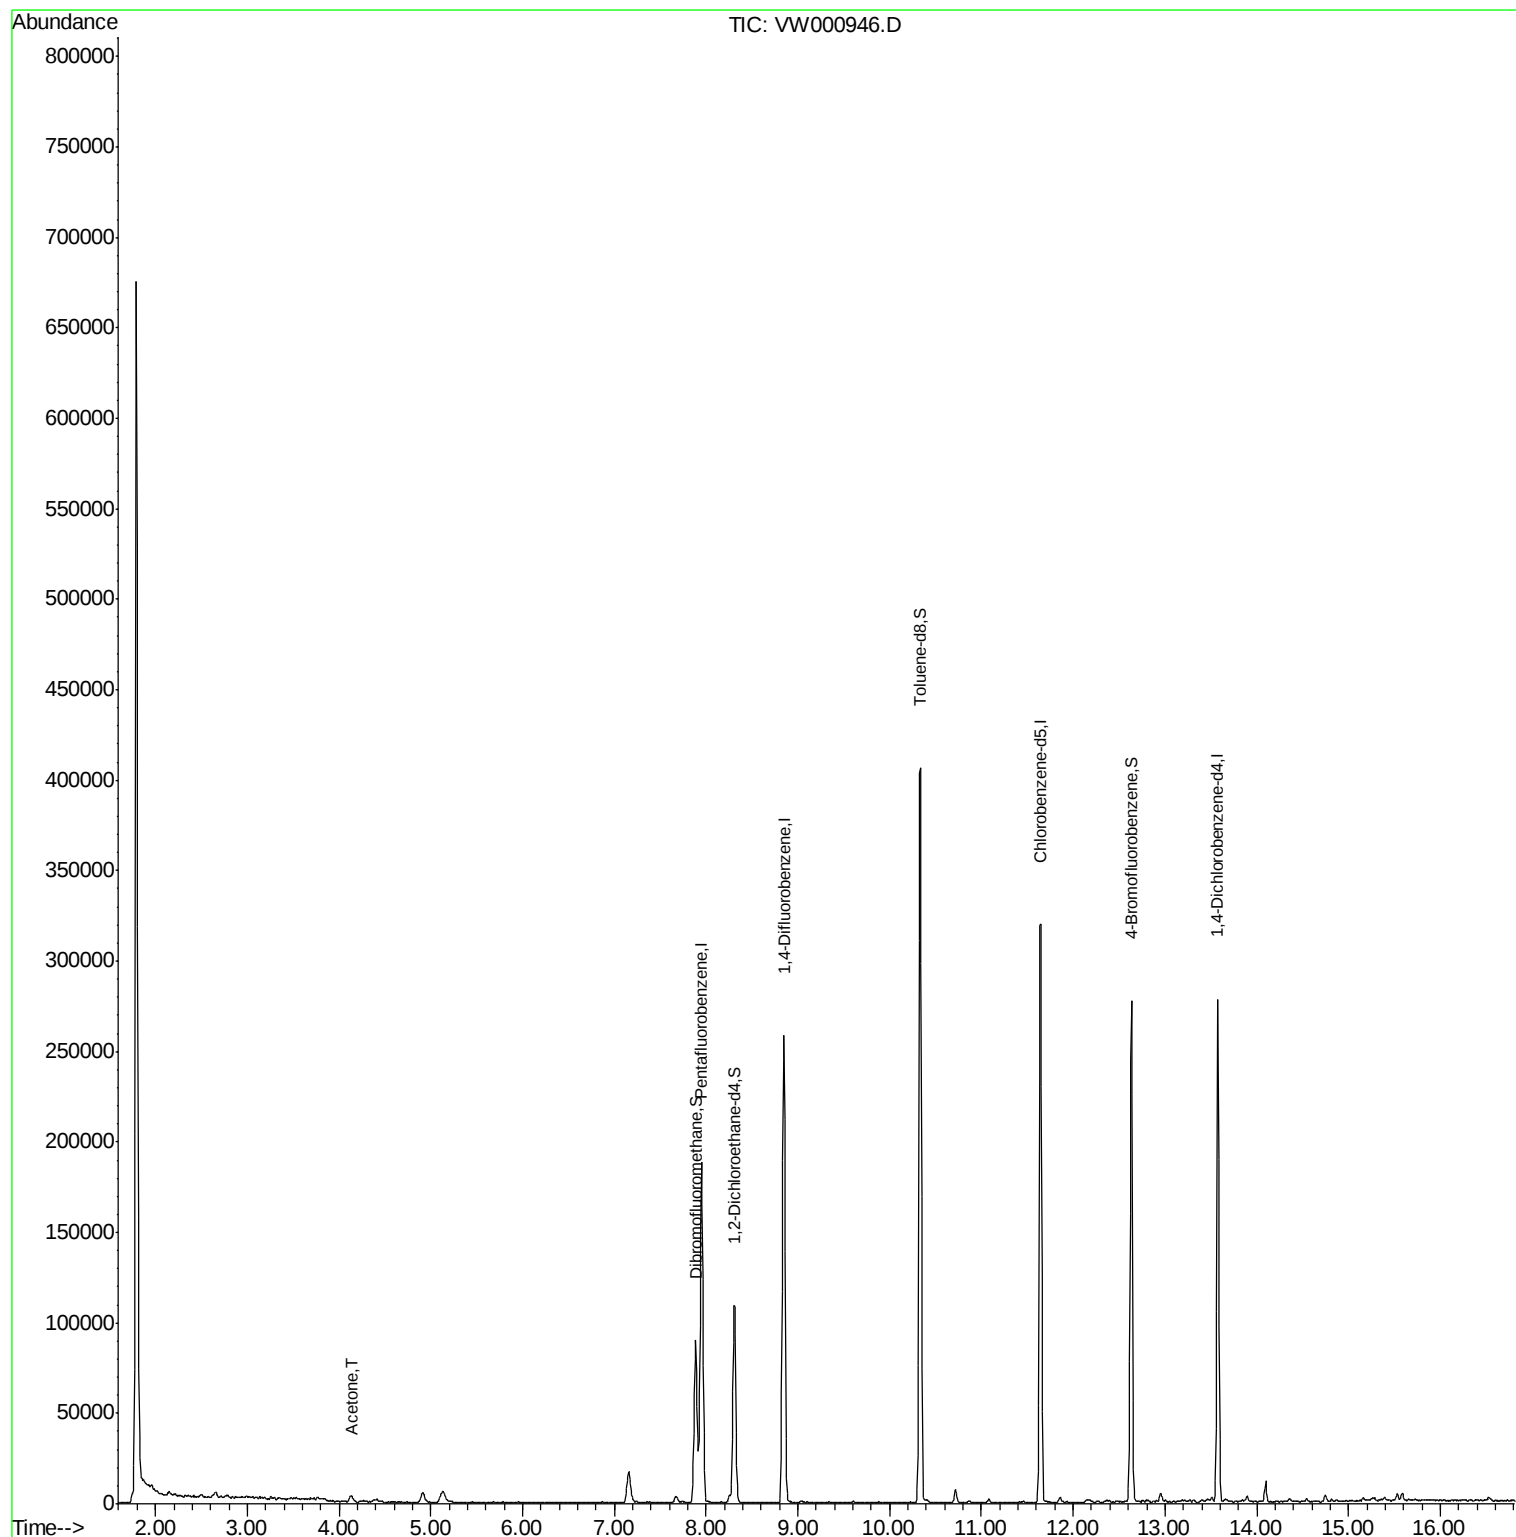

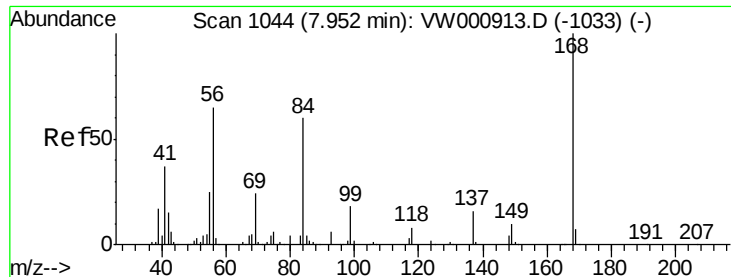

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.95 min Scan# 1044

Delta R.T. 0.00 min

Lab File: VW000946.D

Acq: 24 Jan 2018 14:27

Instrument :

MSVOA_W

ClientSampleId :


EPE-106-4A(65-67)RE

Tot Ion:168 Resp: 146698

Ion Ratio Lower Upper

168 100

99 53.4 40.6 61.0

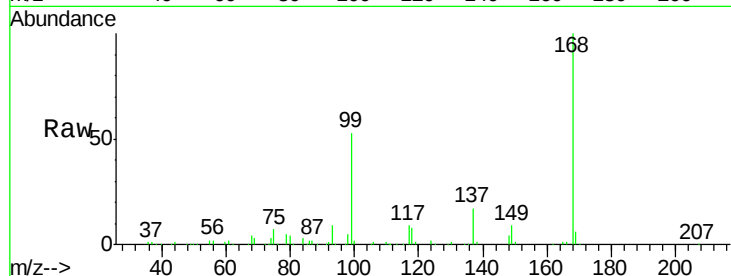

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

60000



40000

20000

0

7.90 8.00 8.10

Time-->

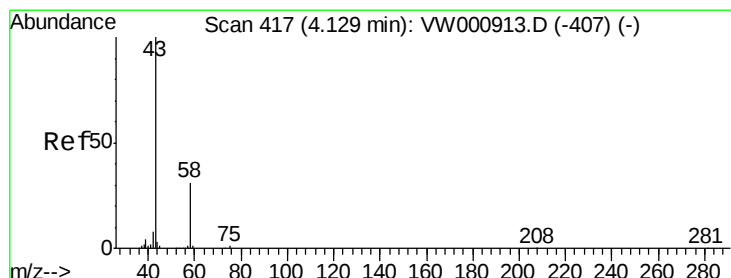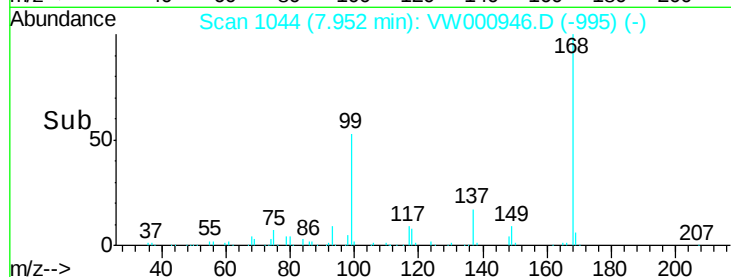

#16

Acetone

Concen: 27.67 ug/l

RT: 4.14 min Scan# 418

Delta R.T. 0.01 min

Lab File: VW000946.D


Acq: 24 Jan 2018 14:27

Tgt Ion: 43 Resp: 6435

Ion Ratio Lower Upper

43 100

58 25.4 24.9 37.3

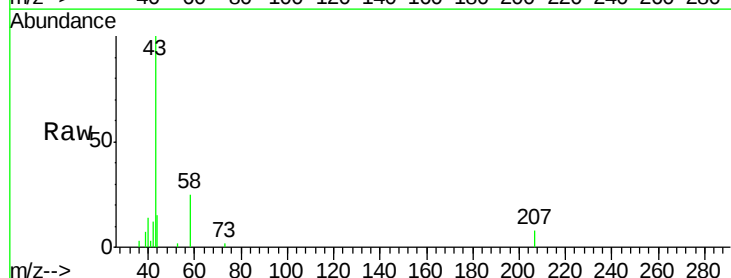

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

4.14

2500

2000

1500


1000


500

0

4.00 4.10 4.20

Time-->




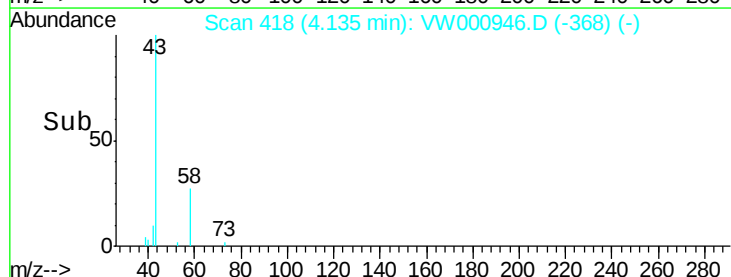


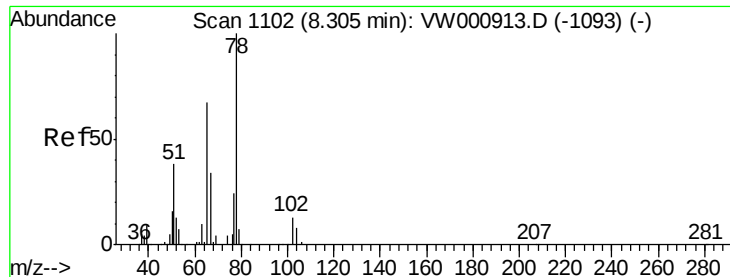

#33
 1,2-Dichloroethane-d4
 Concen: 63.22 ug/l
 RT: 8.31 min Scan# 1103
 Delta R.T. 0.01 min
 Lab File: VW000946.D
 Acq: 24 Jan 2018 14:27




Instrument :
 MSVOA_W
 ClientSampleId :
 EPE-106-4A(65-67)RE


Tot Ion: 65 Resp: 88887
 Ion Ratio Lower Upper
 65 100
 67 51.6 0.0 105.8

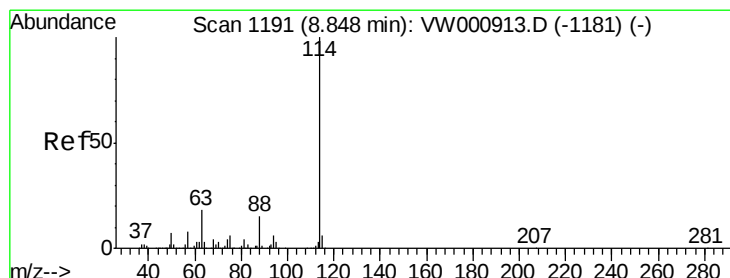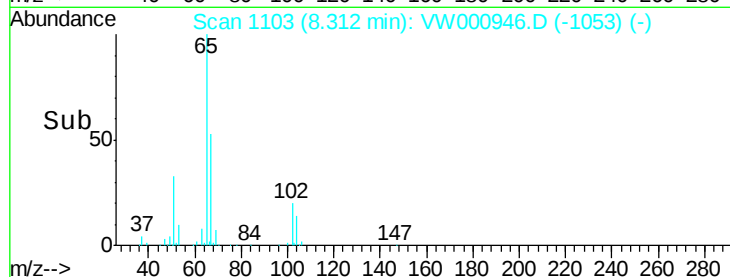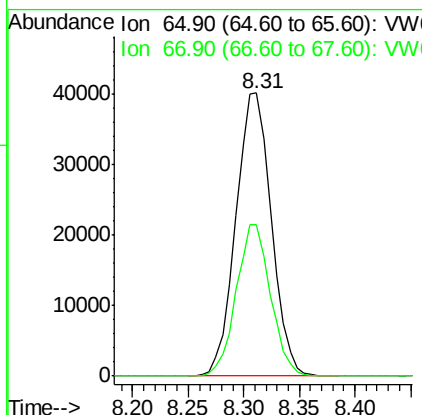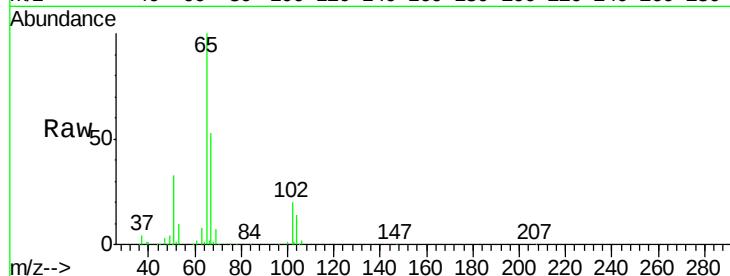

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.85 min Scan# 1191
 Delta R.T. 0.00 min
 Lab File: VW000946.D
 Acq: 24 Jan 2018 14:27

Tgt Ion: 114 Resp: 220601
 Ion Ratio Lower Upper
 114 100
 63 18.9 0.0 36.8
 88 14.5 0.0 29.8

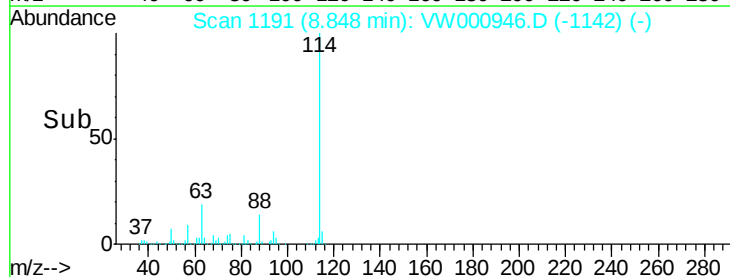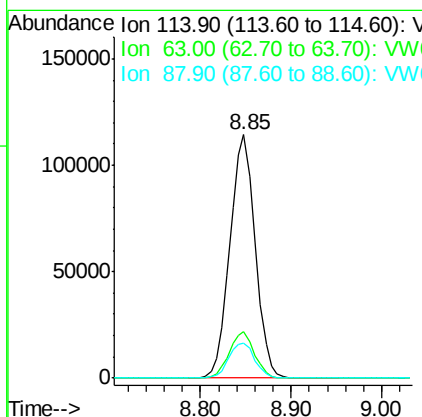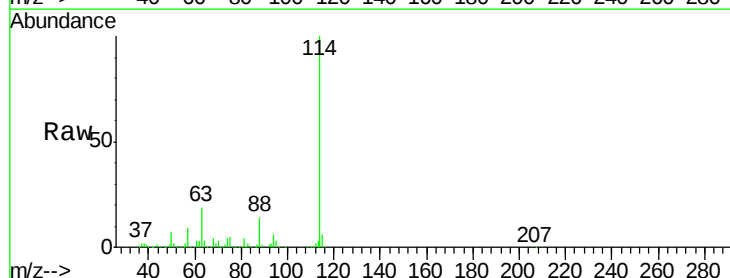

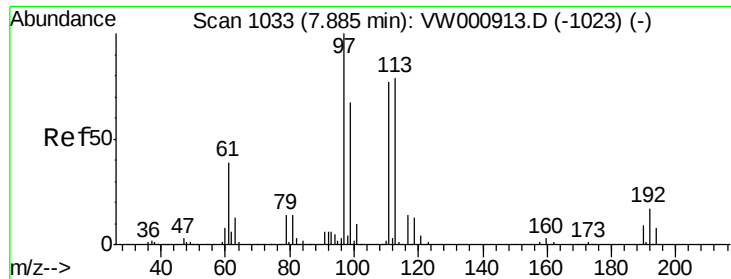

#35

Dibromofluoromethane

Concen: 46.33 ug/l

RT: 7.88 min Scan# 1033

Delta R.T. 0.00 min

Lab File: VW000946.D

Acq: 24 Jan 2018 14:27

Instrument :

MSVOA_W

ClientSampleId :

EPE-106-4A(65-67)RE


Tot Ion:113 Resp: 62617

Ion Ratio Lower Upper

113 100

111 104.4 80.4 120.6




192 22.7 17.0 25.4

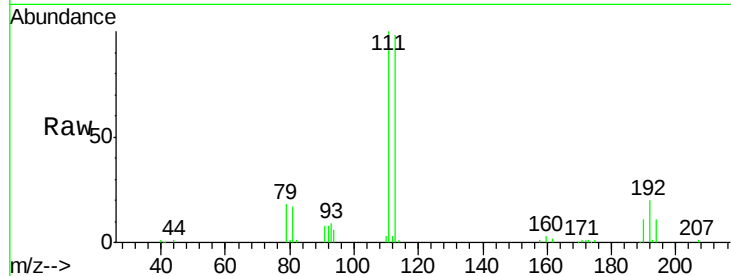

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

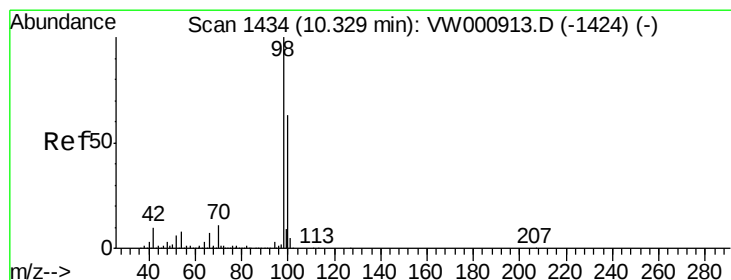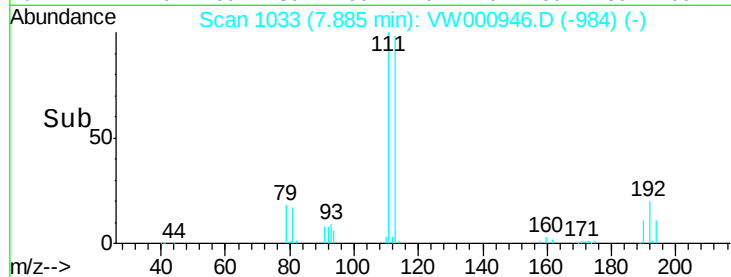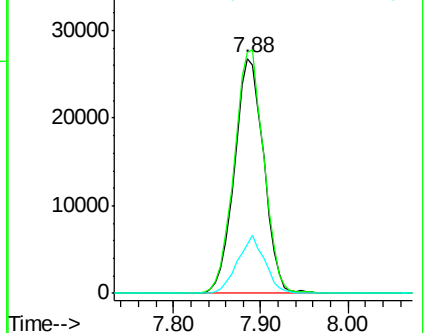

#50

Toluene-d8

Concen: 52.36 ug/l

RT: 10.34 min Scan# 1435

Delta R.T. 0.01 min

Lab File: VW000946.D


Acq: 24 Jan 2018 14:27

Tgt Ion: 98 Resp: 278982

Ion Ratio Lower Upper



98 100


100 63.3 50.8 76.2

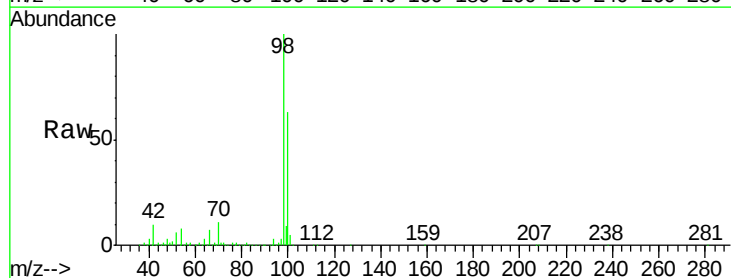

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW



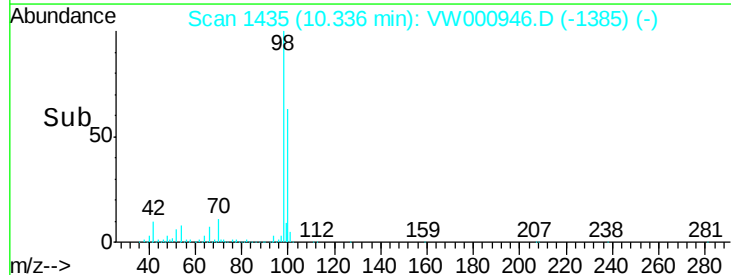
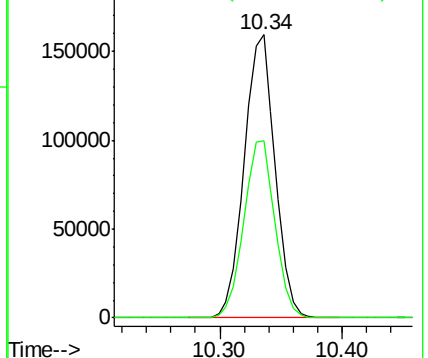


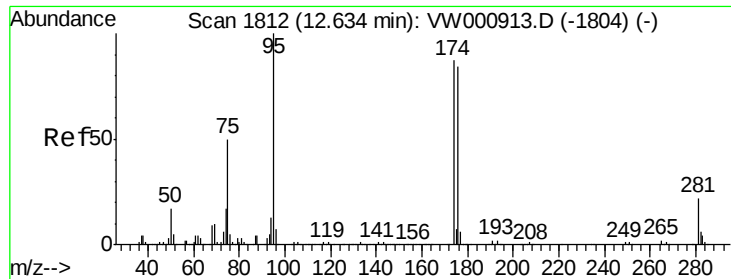

#62
4-Bromofluorobenzene
Concen: 41.10 ug/l
RT: 12.63 min Scan# 1812
Delta R.T. 0.00 min
Lab File: VW000946.D
Acq: 24 Jan 2018 14:27




Instrument :
MSVOA_W
ClientSampleId :
EPE-106-4A(65-67)RE


Tot Ion: 95 Resp: 79740
Ion Ratio Lower Upper
95 100
174 89.3 0.0 176.8
176 85.9 0.0 171.8

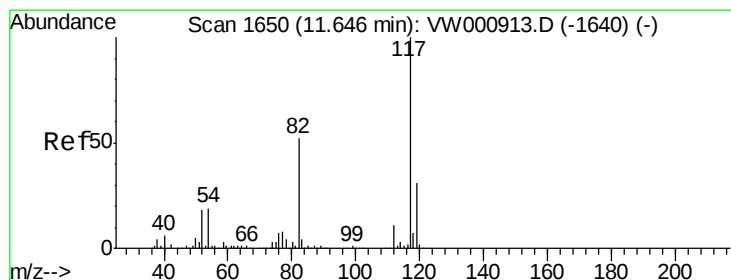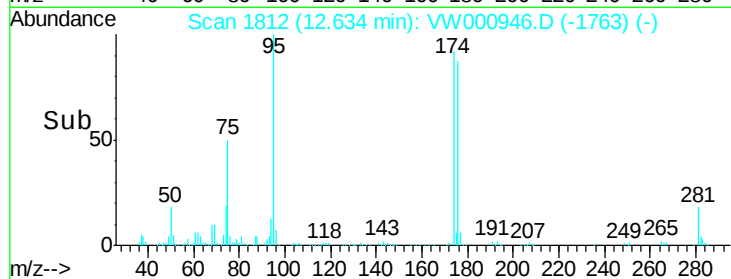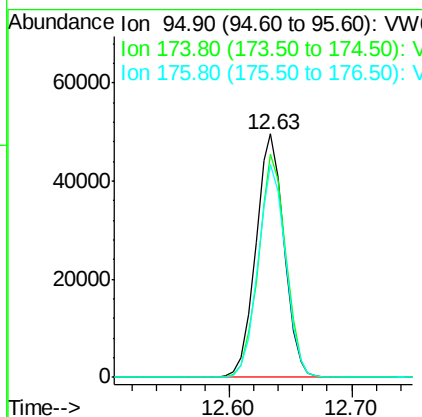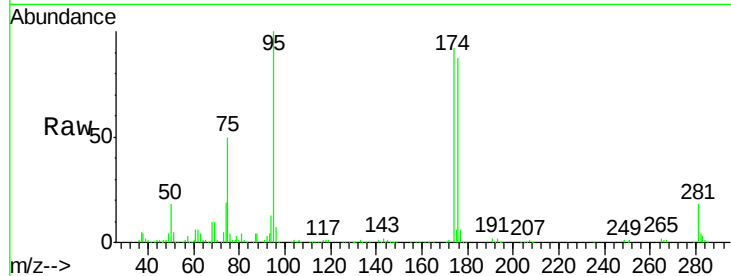

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.65 min Scan# 1650
Delta R.T. 0.00 min
Lab File: VW000946.D
Acq: 24 Jan 2018 14:27

Tgt Ion: 117 Resp: 188226
Ion Ratio Lower Upper
117 100
82 51.4 41.8 62.6
119 32.3 25.2 37.8

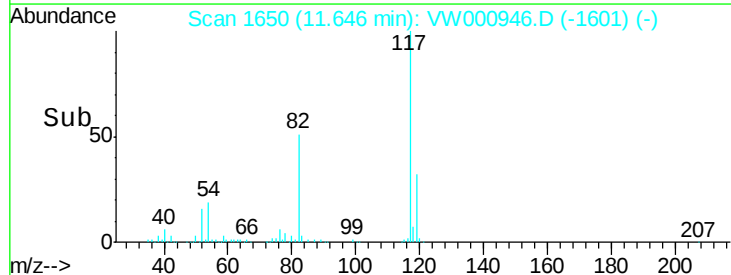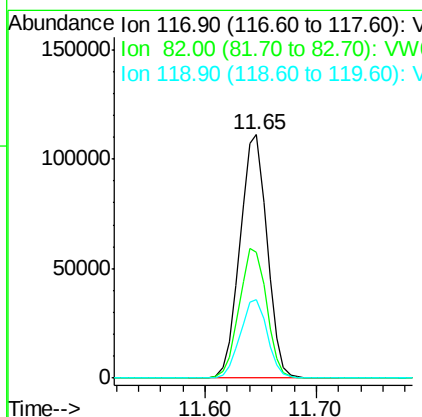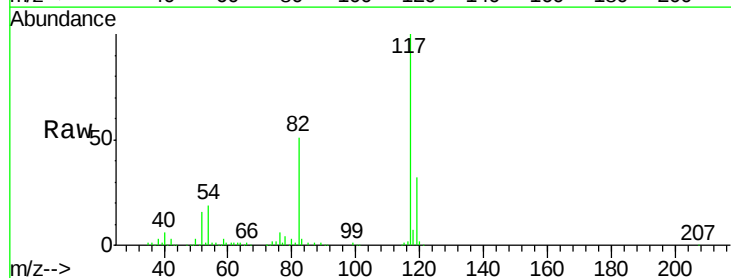

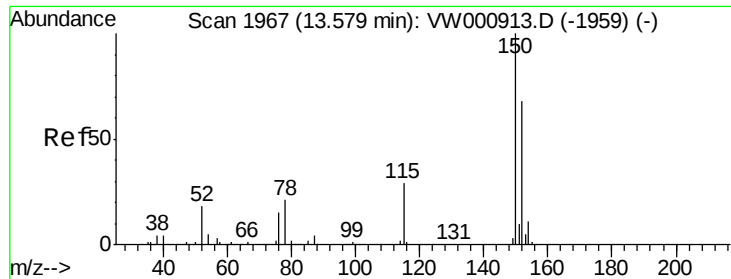

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.58 min Scan# 1967

Delta R.T. 0.00 min

Lab File: VW000946.D

Acq: 24 Jan 2018 14:27

Instrument :

MSVOA_W

ClientSampleId :

EPE-106-4A(65-67)RE


Tot Ion:152 Resp: 75450

Ion Ratio Lower Upper

152 100

115 57.9 28.5 85.5

150 158.4 0.0 342.0

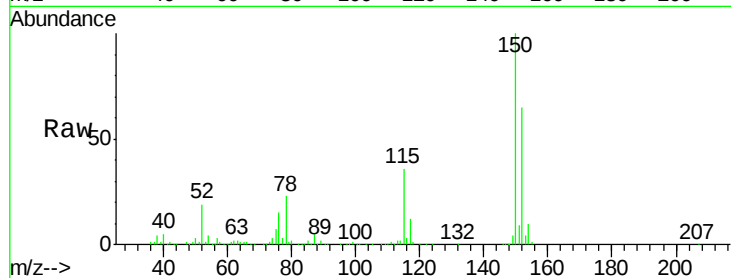

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

