


Data Path : W:\HPCHEM1\MSVOA W\Data\VW012418\
Data File : VW000962.D
Acq On : 24 Jan 2018 21:56
Operator : JC/SY
Sample : BFB
Misc : 5.0G/5.0ML/MSVOA W/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_W\METHOD\82W012318S.M
Title : SW846 8260
Last Update : Tue Jan 23 13:31:00 2018

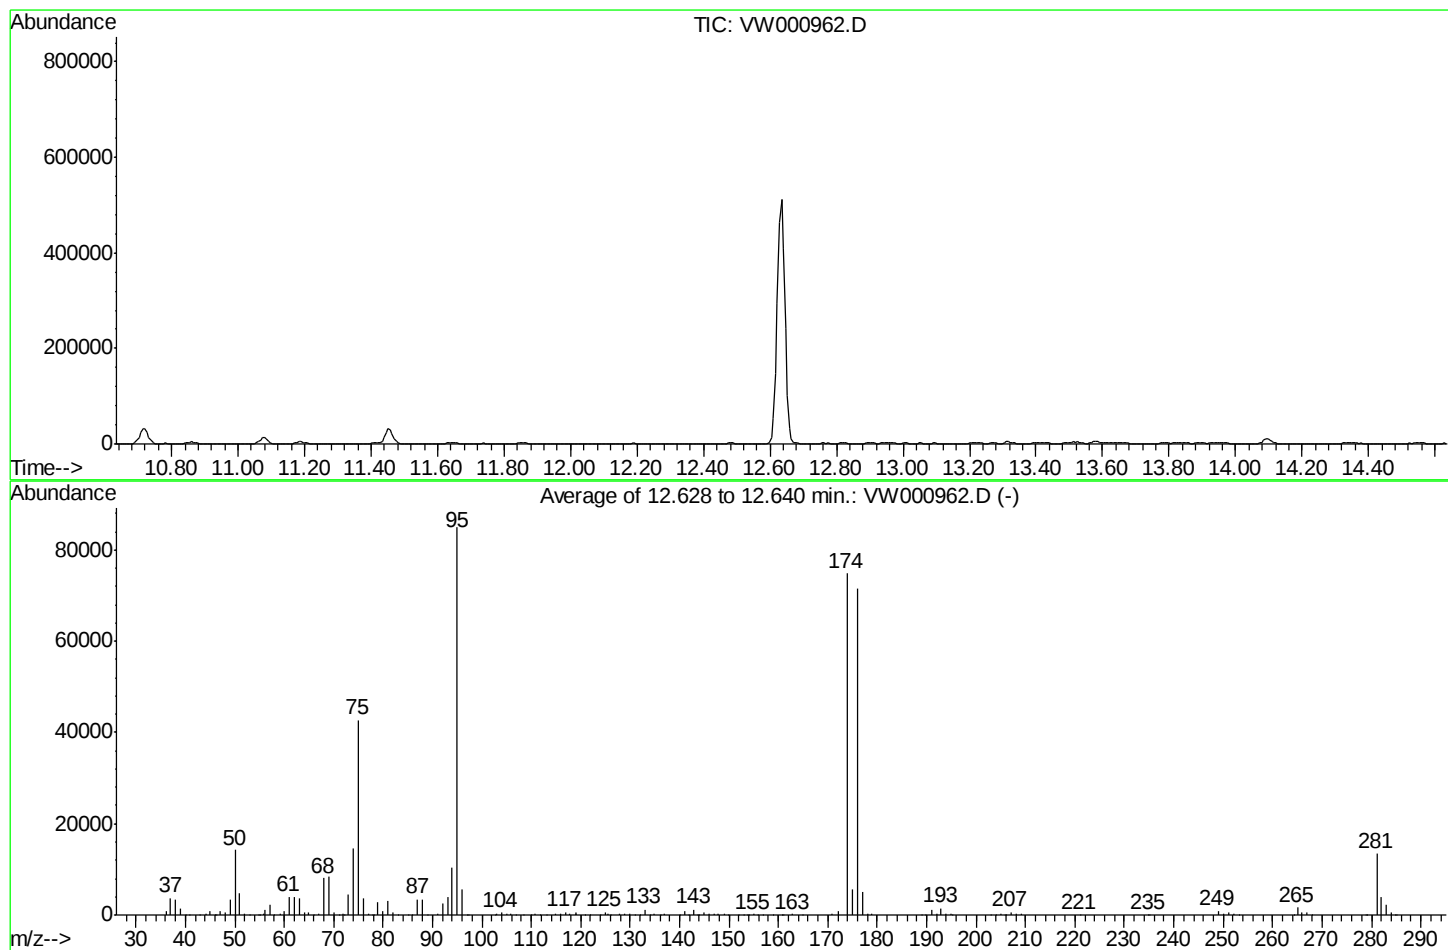

AutoFind: Scans 1811, 1812, 1813; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	14229	PASS
75	95	30	60	50.4	42770	PASS
95	95	100	100	100.0	84938	PASS
96	95	5	9	6.7	5692	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.1	74872	PASS
175	174	5	9	7.7	5739	PASS
176	174	95	101	95.6	71581	PASS
177	176	5	9	7.2	5187	PASS