

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012623\
 Data File : VW025236.D
 Acq On : 26 Jan 2023 10:21
 Operator : SY/MD
 Sample : VW0126SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK455

Quant Time: Jan 27 00:37:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 27 00:36:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	404000	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	363284	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	174796	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	92316	19.682	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.720%
7) Chloroethane-d5	2.885	69	65261	22.083	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.320%
11) 1,1-Dichloroethene-d2	4.019	63	170264	16.574	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.280%
21) 2-Butanone-d5	7.080	46	64761	54.480	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.960%
24) Chloroform-d	7.647	84	253109	24.997	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.000%
26) 1,2-Dichloroethane-d4	8.305	65	139320	26.711	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.840%
32) Benzene-d6	8.275	84	521298	23.897	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.600%
36) 1,2-Dichloropropane-d6	9.275	67	152941	23.967	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.880%
41) Toluene-d8	10.323	98	469925	23.669	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.680%
43) trans-1,3-Dichloroprop...	10.579	79	66777	24.438	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.760%
47) 2-Hexanone-d5	10.921	63	50919	50.639	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.280%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	118333	26.516	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.080%
66) 1,2-Dichlorobenzene-d4	13.853	152	155532	25.043	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.160%
Target Compounds						Qvalue
34) Trichloroethene	8.842	95	12572	2.195	ug/L	# 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012623\
Data File : VW025236.D
Acq On : 26 Jan 2023 10:21
Operator : SY/MD
Sample : VW0126SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK455

Quant Time: Jan 27 00:37:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 27 00:36:30 2023
Response via : Initial Calibration

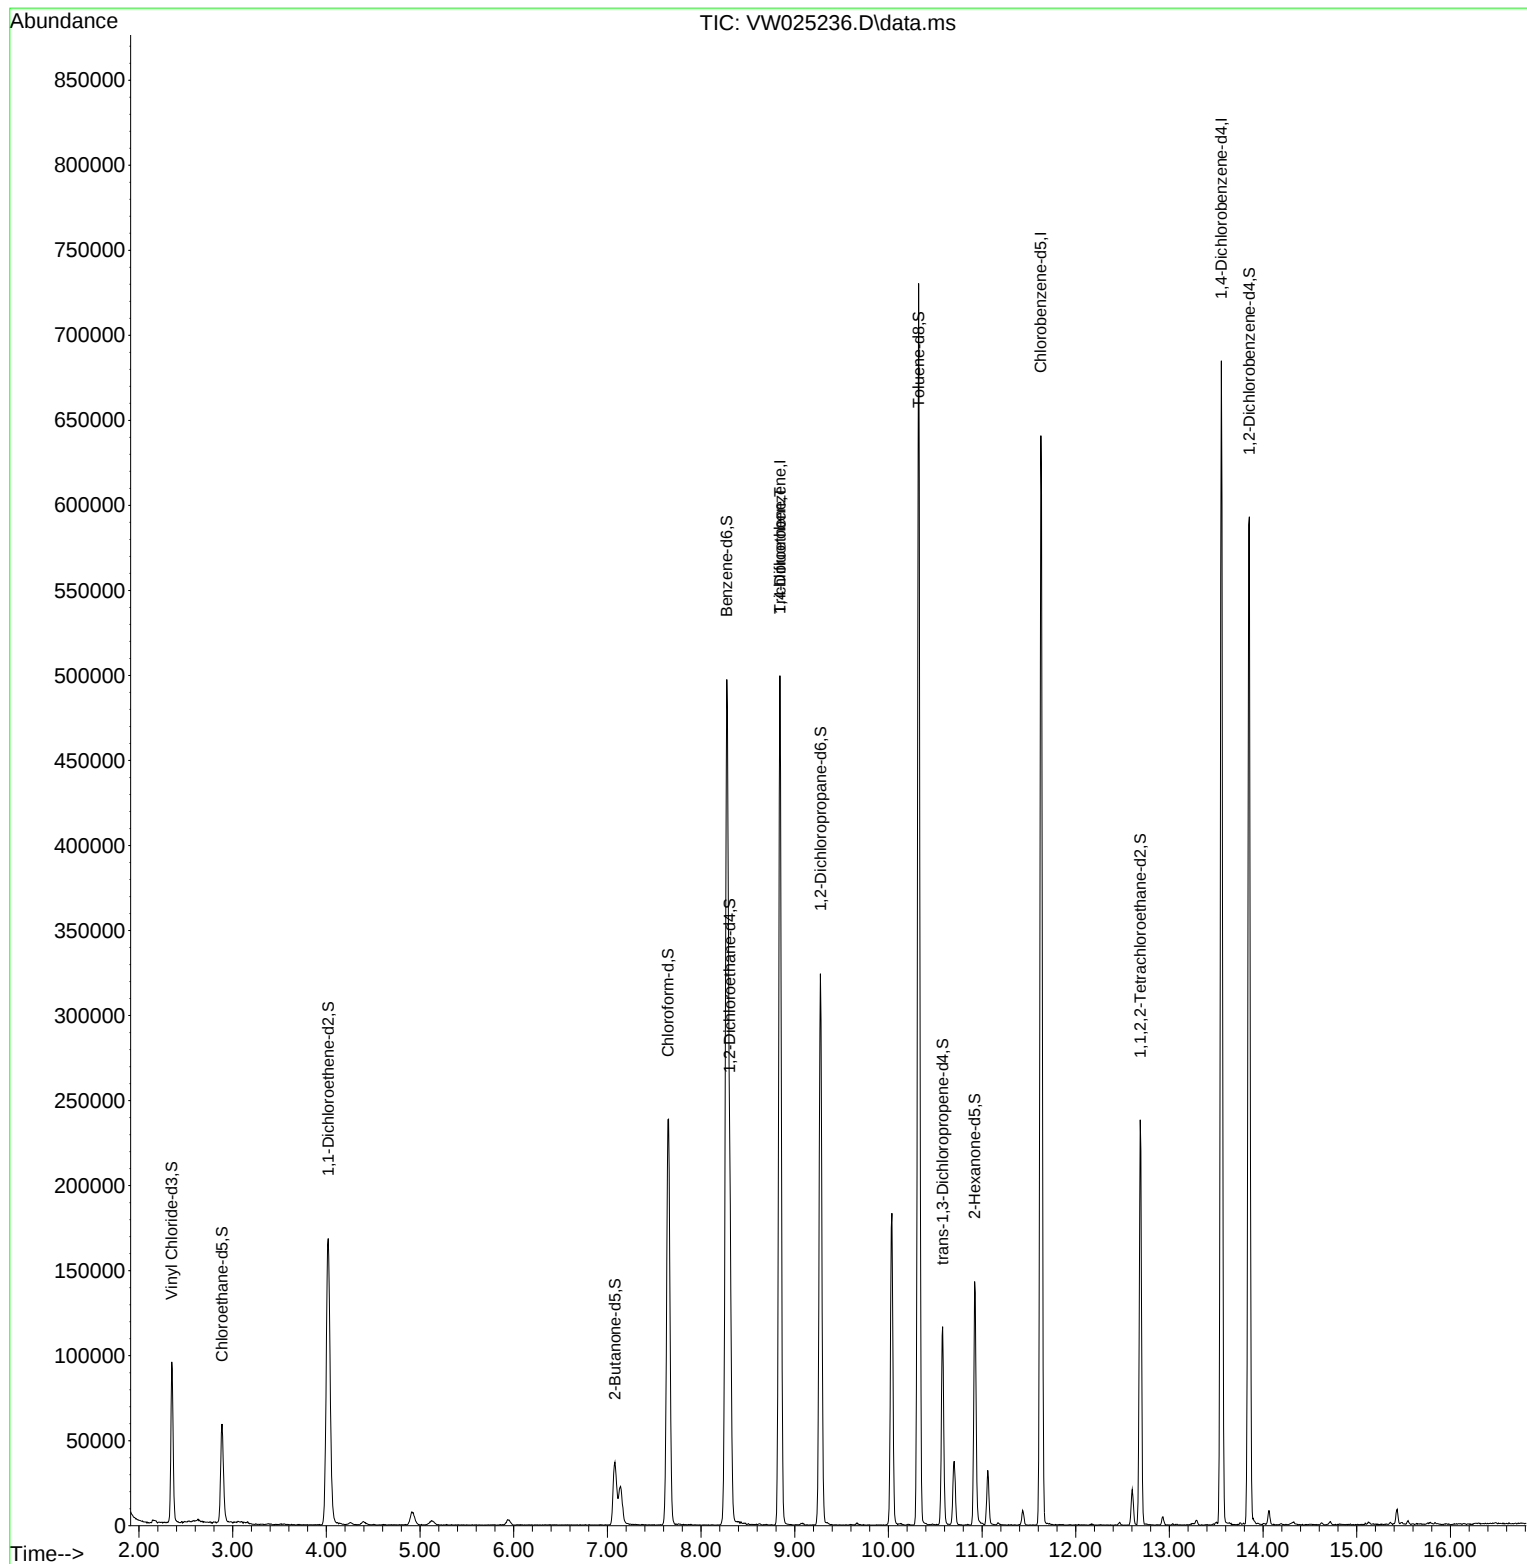

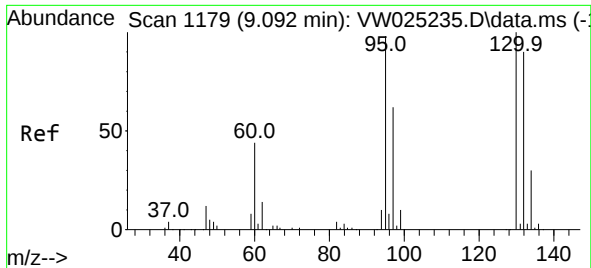

#34

Trichloroethene

Concen: 2.195 ug/L

RT: 8.842 min Scan# 11

Delta R.T. -0.250 min

Lab File: VW025236.D


Acq: 26 Jan 2023 10:21

Instrument :

MSVOA_W

ClientSampleId :

VBLK455

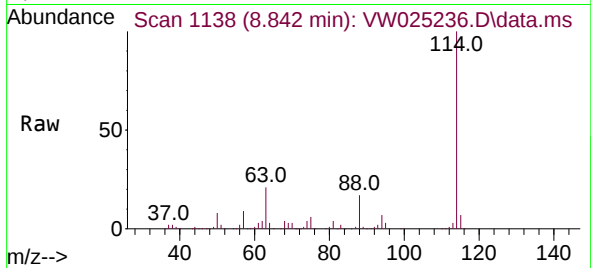

Tgt Ion: 95 Resp: 12572

Ion Ratio Lower Upper

95 100

97 0.0 44.4 82.4#

132 0.0 64.5 119.7#

130 0.0 66.8 124.0#

