

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012623\
 Data File : VW025238.D
 Acq On : 26 Jan 2023 13:36
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK404

Quant Time: Jan 27 00:37:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 27 00:36:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	430525	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	380217	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	182537	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	87171	17.440	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.760%
7) Chloroethane-d5	2.885	69	61952	19.672	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.680%
11) 1,1-Dichloroethene-d2	4.019	63	161308	14.735	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.960%
21) 2-Butanone-d5	7.080	46	48041	37.925	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.840%
24) Chloroform-d	7.653	84	232723	21.568	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.280%
26) 1,2-Dichloroethane-d4	8.305	65	122505	22.040	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.160%
32) Benzene-d6	8.275	84	480884	21.062	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.240%
36) 1,2-Dichloropropane-d6	9.274	67	138985	20.810	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.240%
41) Toluene-d8	10.323	98	444218	21.378	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.520%
43) trans-1,3-Dichloroprop...	10.579	79	57395	20.069	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.280%
47) 2-Hexanone-d5	10.927	63	39968	37.978	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.960%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	98617	21.114	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	141887	21.877	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.520%
Target Compounds					Qvalue	
34) Trichloroethene	8.842	95	13646	2.277	ug/L	# 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012623\
Data File : VW025238.D
Acq On : 26 Jan 2023 13:36
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK404


Quant Time: Jan 27 00:37:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 27 00:36:30 2023
Response via : Initial Calibration

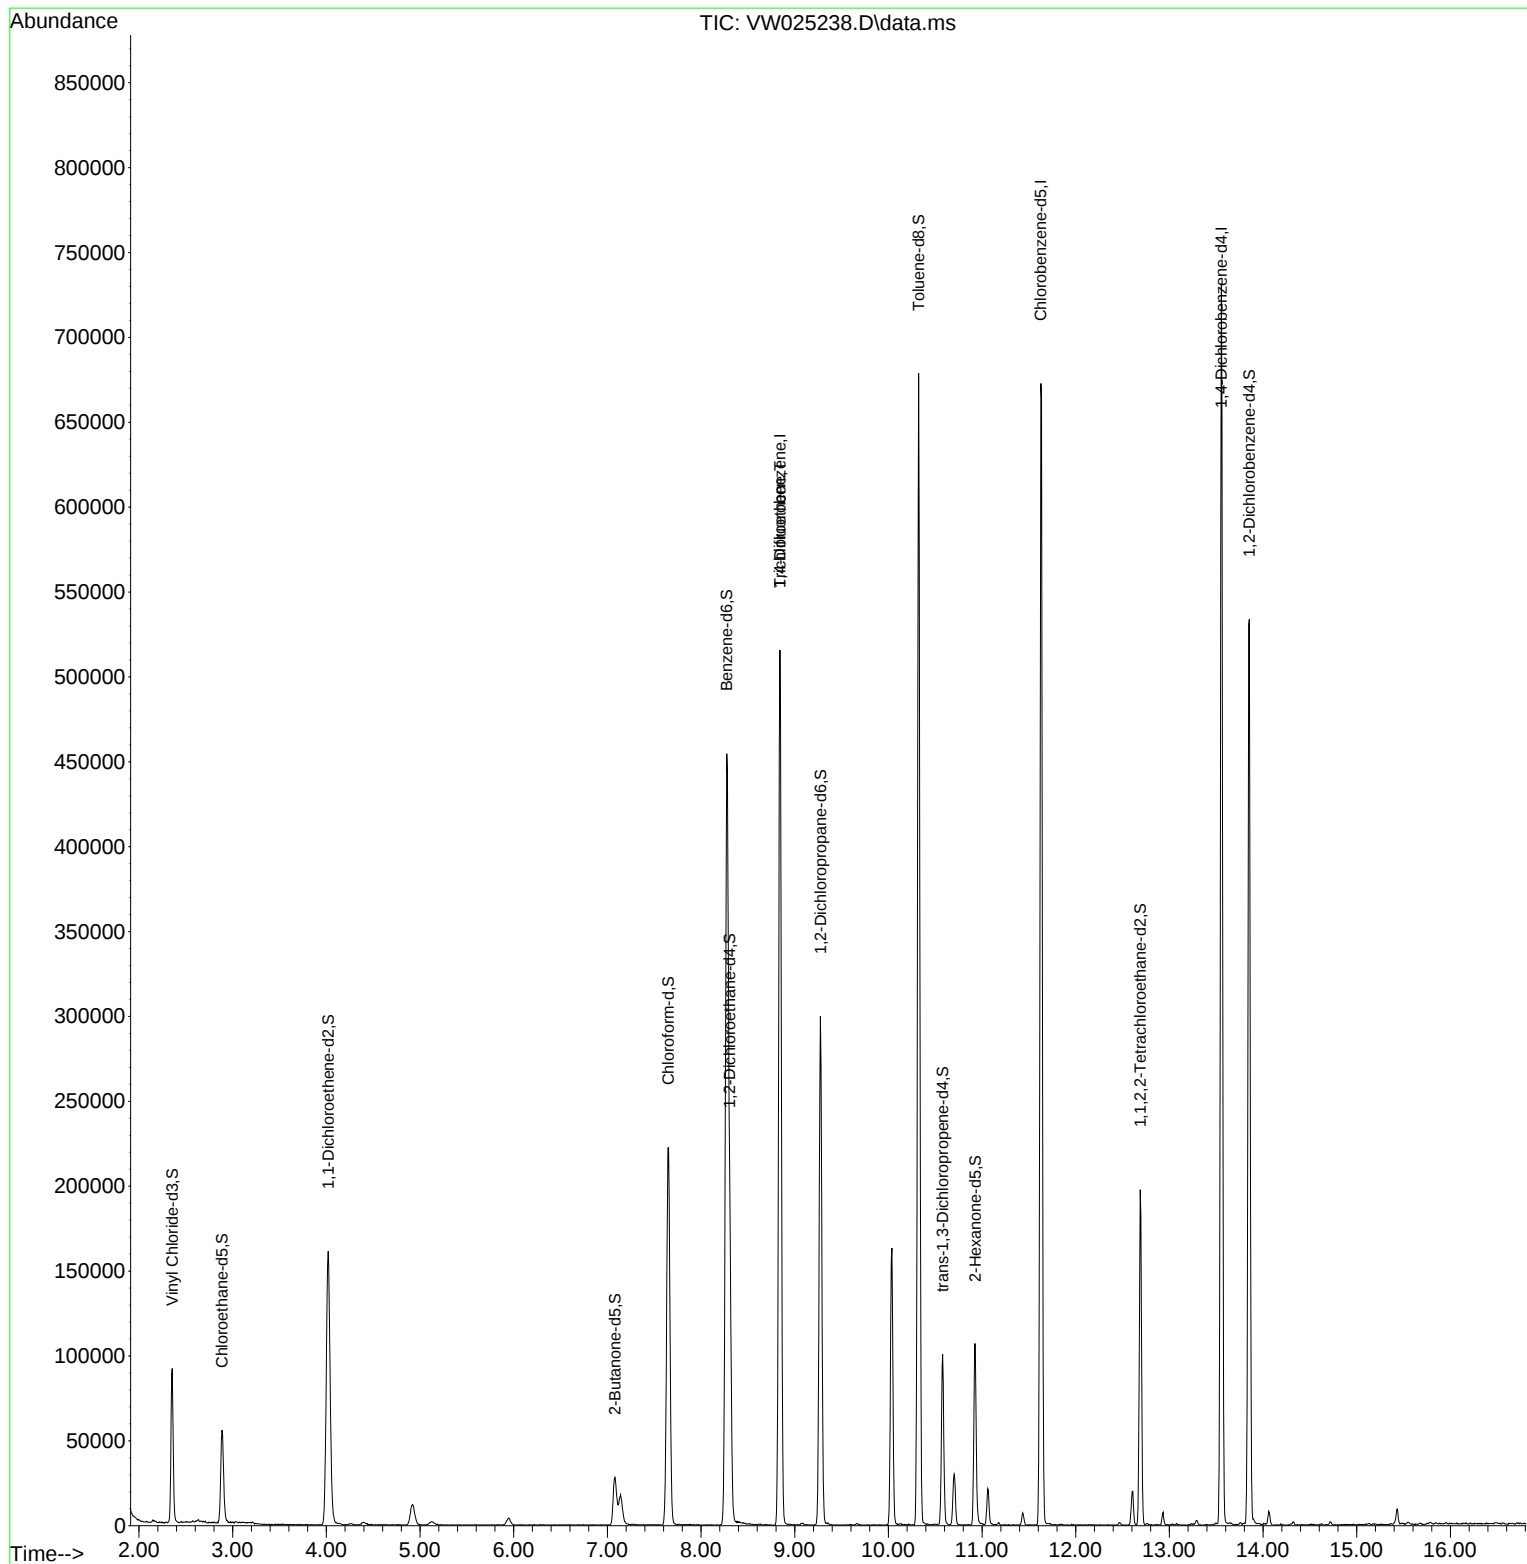

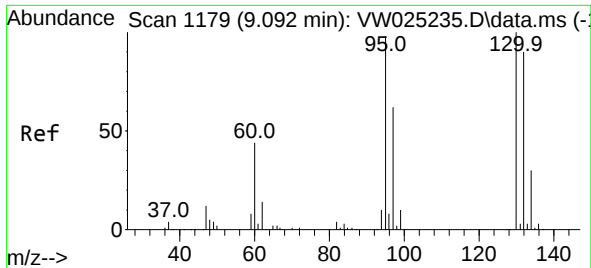

#34
 Trichloroethene
 Concen: 2.277 ug/L
 RT: 8.842 min Scan# 11
 Delta R.T. -0.250 min
 Lab File: VW025238.D
 Acq: 26 Jan 2023 13:36

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK404

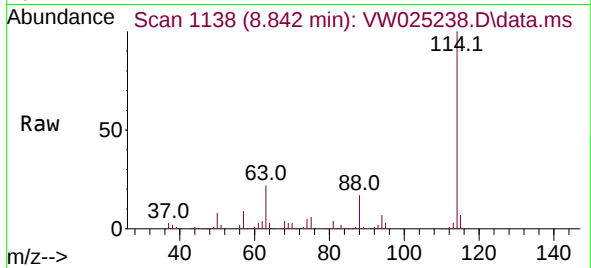

Tgt Ion: 95	Resp: 13646
Ion Ratio	Lower Upper
95	100
97	0.0 44.4 82.4#
132	0.0 64.5 119.7#
130	0.0 66.8 124.0#

