

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012623\
 Data File : VW025240.D
 Acq On : 26 Jan 2023 14:51
 Operator : SY/MD
 Sample : 01315-06
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Jan 27 00:37:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jan 27 00:36:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	446241	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	379478	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	157083	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	91963	17.751	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.000%
7) Chloroethane-d5	2.879	69	63107	19.333	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.320%
11) 1,1-Dichloroethene-d2	4.013	63	173617	15.301	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.200%
21) 2-Butanone-d5	7.074	46	57349	43.678	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.360%
24) Chloroform-d	7.647	84	246921	22.078	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.320%
26) 1,2-Dichloroethane-d4	8.305	65	135563	23.531	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.120%
32) Benzene-d6	8.275	84	510470	22.402	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.600%
36) 1,2-Dichloropropane-d6	9.274	67	147511	22.130	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.520%
41) Toluene-d8	10.323	98	464138	22.380	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.520%
43) trans-1,3-Dichloroprop...	10.579	79	62267	21.815	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.280%
47) 2-Hexanone-d5	10.920	63	45053	42.893	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.780%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	110154	23.630	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.520%
66) 1,2-Dichlorobenzene-d4	13.847	152	125598	22.504	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.000%
Target Compounds						Qvalue
34) Trichloroethene	8.841	95	13951	2.332	ug/L #	7
37) 1,2-Dichloropropane	9.268	63	16880	2.992	ug/L #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012623\
Data File : VW025240.D
Acq On : 26 Jan 2023 14:51
Operator : SY/MD
Sample : 01315-06
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Jan 27 00:37:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jan 27 00:36:30 2023
Response via : Initial Calibration




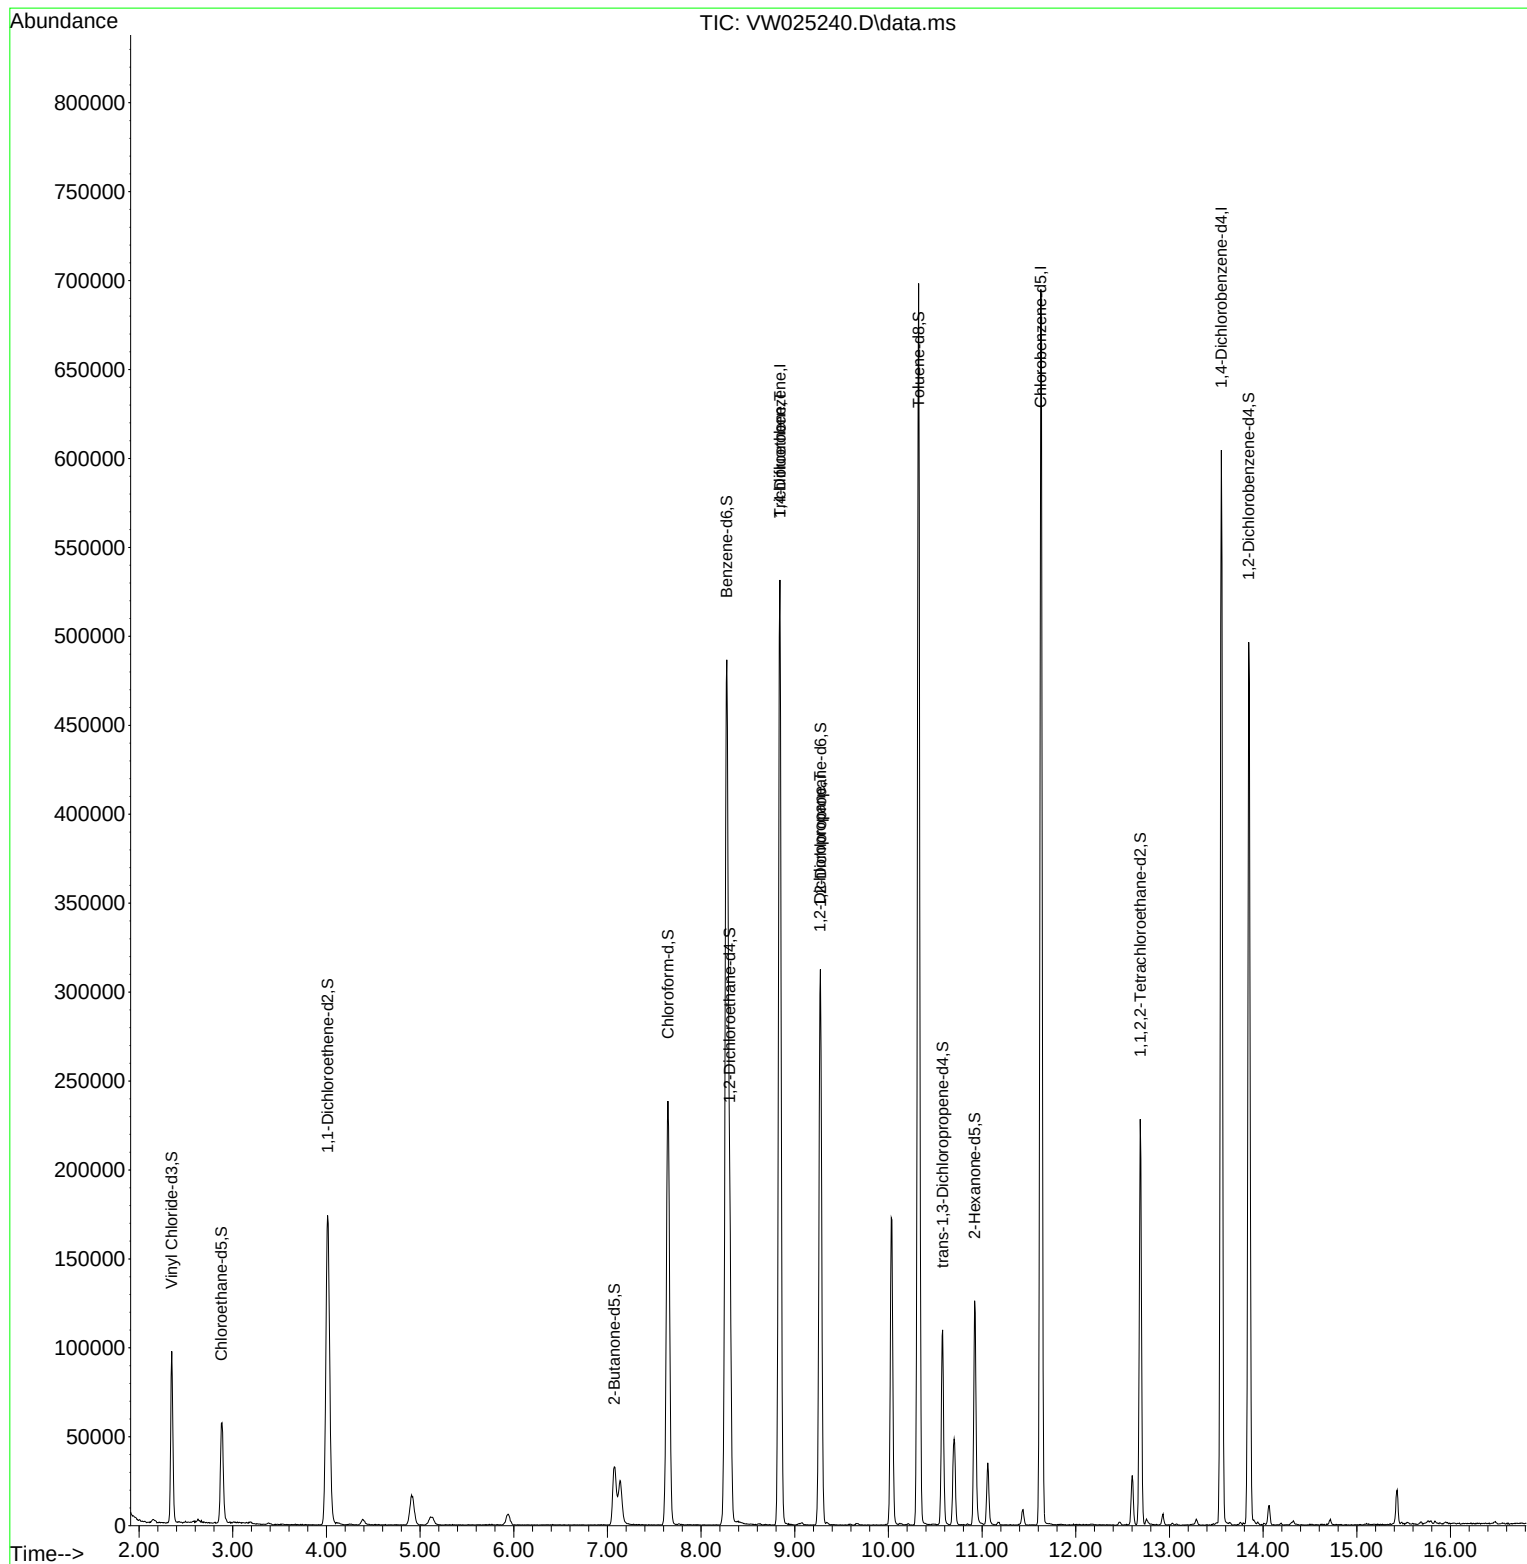


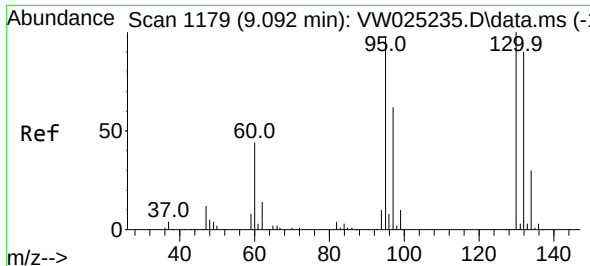

#34
Trichloroethene
Concen: 2.332 ug/L
RT: 8.841 min Scan# 1138
Delta R.T. -0.250 min
Lab File: VW025240.D
Acq: 26 Jan 2023 14:51

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Tgt Ion:	95	Resp:	13951
Ion	Ratio	Lower	Upper
95	100		
97	0.0	44.4	82.4#
132	0.0	64.5	119.7#
130	0.0	66.8	124.0#

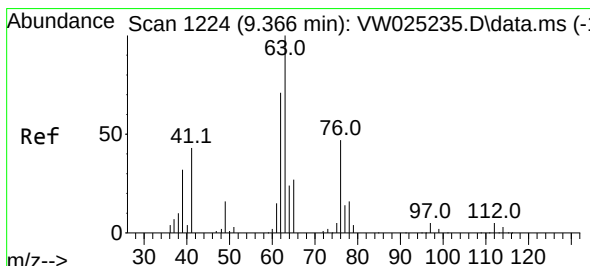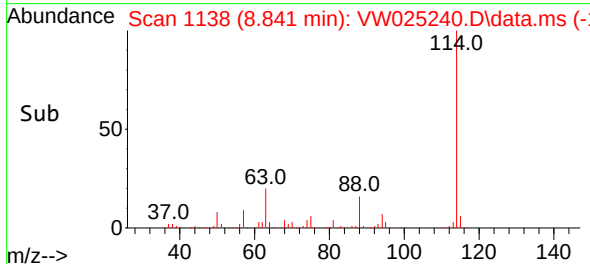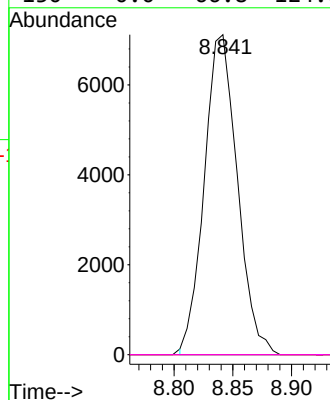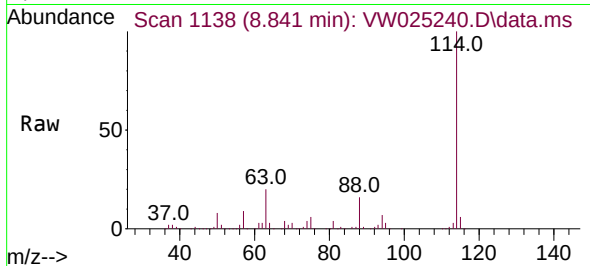

#37
1,2-Dichloropropane
Concen: 2.992 ug/L
RT: 9.268 min Scan# 1208
Delta R.T. -0.098 min
Lab File: VW025240.D
Acq: 26 Jan 2023 14:51

Tgt Ion:	63	Resp:	16880
Ion	Ratio	Lower	Upper
63	100		
112	0.3	3.7	5.5#

