
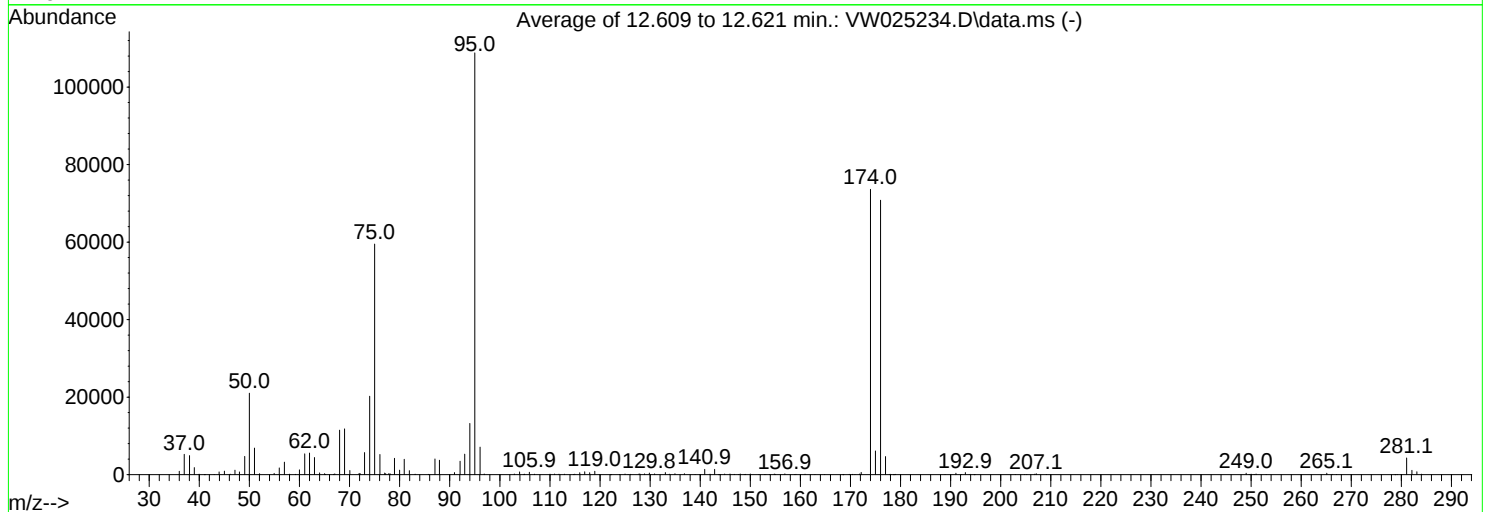


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012623\
Data File : VW025234.D
Acq On : 26 Jan 2023 08:41
Operator : SY/MD
Sample : BFB472
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB472

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010323SMA.M
Title : SFAM01.0
Last Update : Fri Jan 27 00:36:30 2023

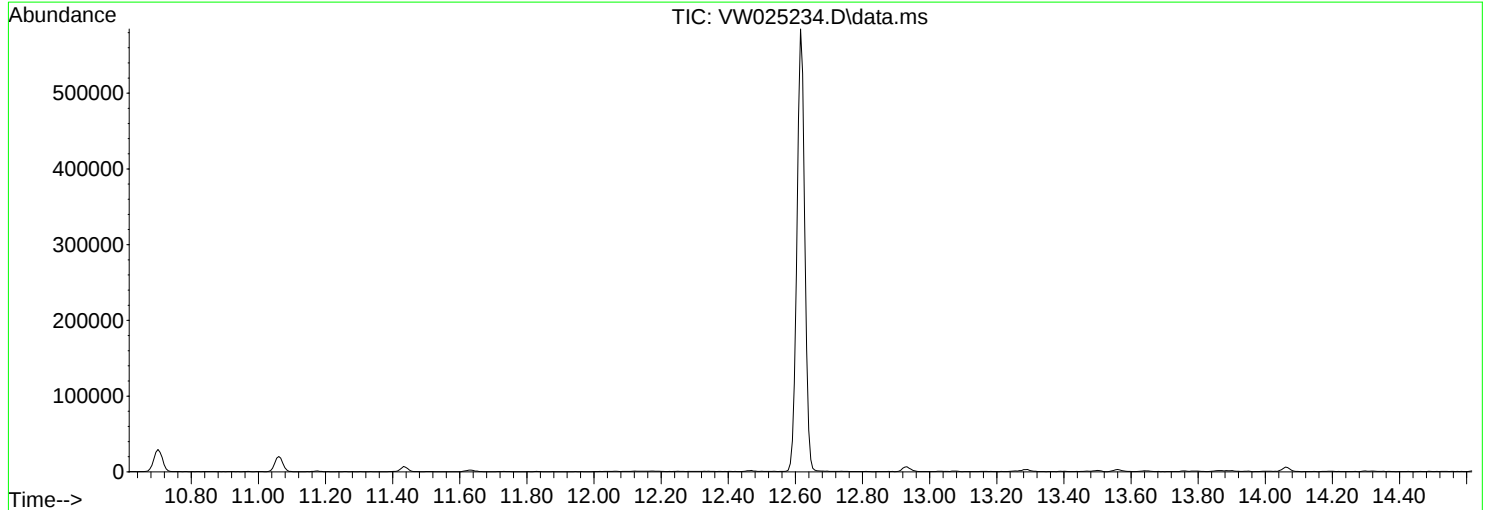

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	21021	PASS
75	95	30	80	54.7	59475	PASS
95	95	100	100	100.0	108824	PASS
96	95	5	9	6.5	7122	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	67.7	73627	PASS
175	174	5	9	8.3	6105	PASS
176	174	95	105	96.1	70784	PASS
177	176	5	10	6.6	4673	PASS

m/z	Abundance
35.90	225.0
39.00	50.0
39.90	138.0
43.00	69.0
43.30	70.0
57.00	65.0

Instrument :
MSVOA_W
ClientSampleId :
BFB472

m/z	Abundance
36.00	1056.0
37.00	4938.0
38.00	4704.0
39.10	1935.0
40.00	277.0
41.00	56.0
43.00	115.0
43.90	647.0
45.00	972.0
46.10	175.0
47.10	1170.0
48.00	653.0
49.00	4106.0
50.00	19104.0
51.00	6496.0
52.10	273.0
54.90	368.0
55.90	1490.0
57.10	2783.0
58.10	127.0
59.20	180.0
60.00	978.0
61.00	4898.0
62.00	4936.0
63.00	3772.0
64.00	441.0
65.00	408.0
67.10	271.0
68.00	10041.0
69.00	10673.0
70.10	930.0
71.90	489.0
73.00	5531.0
74.00	17536.0
75.00	51928.0
76.00	4720.0
77.00	661.0
77.80	427.0
79.00	3873.0
80.00	990.0
80.90	3422.0
82.00	900.0
83.20	180.0
87.00	3730.0
88.00	3514.0
91.00	526.0
92.00	3202.0
93.00	5030.0
94.00	11939.0
95.00	97208.0
96.00	6218.0
102.90	298.0
104.00	488.0
104.80	230.0
105.90	421.0
106.90	72.0
109.90	162.0
111.00	153.0
111.80	124.0
112.90	111.0
114.70	137.0
115.10	96.0
116.00	524.0
116.90	574.0
118.10	469.0
118.90	858.0
119.90	69.0
125.00	282.0
125.60	124.0
126.30	86.0
127.80	260.0
128.80	219.0
129.90	313.0
131.00	197.0
133.10	728.0
133.90	226.0
135.00	212.0
136.80	213.0
139.00	75.0
140.90	1061.0
142.00	192.0
142.90	1193.0
145.00	162.0
146.00	140.0
146.80	127.0
147.70	172.0
148.80	114.0
150.10	127.0
154.80	192.0
156.90	173.0
158.90	130.0
161.00	157.0

Instrument :
MSVOA_W
ClientSampleId :
BFB472

162.90	91.0
164.80	54.0
170.40	82.0
171.80	477.0
172.30	579.0
174.00	61904.0
175.00	5089.0
176.00	56384.0
177.00	3909.0
177.90	236.0
179.00	158.0
188.90	81.0
191.10	454.0
193.00	688.0
193.90	231.0
194.70	66.0
202.90	94.0
204.80	106.0
205.20	93.0
206.80	404.0
207.10	378.0
209.10	116.0
249.00	682.0
250.00	109.0
250.60	153.0
251.10	196.0
253.00	70.0
265.10	493.0
266.10	209.0
267.10	75.0
279.20	74.0
281.00	5983.0
282.10	1617.0
283.10	1210.0
284.00	206.0

Instrument :
MSVOA_W
ClientSampleId :
BFB472

m/z	Abundance
36.10	1175.0
37.00	5932.0
38.10	5419.0
39.10	2135.0
40.10	284.0
42.80	124.0
44.00	803.0
45.10	880.0
46.20	153.0
47.20	983.0
48.00	707.0
49.10	5276.0
50.00	23224.0
51.00	7807.0
52.00	245.0
55.00	338.0
56.00	1902.0
57.00	3585.0
58.00	111.0
59.20	90.0
60.00	1509.0
61.00	6263.0
62.00	6278.0
63.00	5108.0
64.00	569.0
65.00	371.0
66.80	286.0
68.00	13373.0
69.00	13799.0
70.10	1109.0
72.10	837.0
73.00	6114.0
74.00	22640.0
75.00	66296.0
76.10	5434.0
77.20	710.0
78.10	599.0
78.90	4454.0
80.00	1176.0
80.90	4080.0
81.90	1127.0
83.00	141.0
85.80	100.0
87.00	4407.0
87.90	4374.0
91.00	527.0
92.00	3666.0
93.00	5820.0
94.00	13902.0
95.00	122104.0
96.00	8142.0
96.90	302.0
102.80	93.0
103.90	784.0
105.00	208.0
105.90	719.0
106.90	184.0
110.00	149.0
110.90	190.0
111.90	115.0
113.00	124.0
114.90	206.0
115.90	504.0
117.00	845.0
117.90	567.0
118.90	935.0
119.80	51.0
122.10	63.0
123.90	96.0
125.00	168.0
126.10	113.0
128.00	357.0
128.90	255.0
129.80	605.0
130.90	298.0
133.10	586.0
133.70	102.0
134.90	299.0
136.90	311.0
139.90	55.0
140.90	1498.0
141.90	168.0
142.90	1426.0
144.10	116.0
144.90	206.0
146.00	149.0
146.70	83.0
148.10	231.0
149.00	186.0
149.90	140.0
151.70	60.0
152.90	85.0

Instrument :
MSVOA_W
ClientSampleId :
BFB472

155.00	257.0
156.90	258.0
159.10	164.0
160.90	173.0
162.90	71.0
164.90	92.0
169.80	110.0
170.40	129.0
172.10	467.0
174.00	84096.0
175.00	6860.0
176.00	77312.0
177.00	4816.0
178.10	167.0
179.00	90.0
191.00	454.0
192.10	74.0
192.90	629.0
202.90	86.0
205.20	67.0
207.10	241.0
249.00	358.0
249.60	120.0
250.00	106.0
250.90	148.0
253.00	92.0
265.10	418.0
266.20	99.0
267.00	65.0
278.70	56.0
281.10	4815.0
282.10	949.0
283.10	699.0
284.10	137.0

Instrument :
MSVOA_W
ClientSampleId :
BFB472

m/z	Abundance
36.00	1040.0
37.00	4828.0
38.00	4628.0
39.00	1522.0
39.90	234.0
43.00	102.0
44.00	675.0
44.90	923.0
46.10	97.0
47.00	1297.0
48.00	723.0
49.00	4792.0
50.00	20736.0
51.00	6263.0
52.00	253.0
55.00	294.0
56.00	1796.0
57.00	3504.0
58.00	95.0
60.00	1243.0
61.10	4967.0
62.00	5454.0
63.00	4421.0
64.00	418.0
65.20	269.0
67.00	369.0
68.00	11013.0
69.00	10921.0
70.00	1159.0
71.90	563.0
73.00	5413.0
74.00	20464.0
75.00	60200.0
76.00	5453.0
77.00	558.0
77.90	474.0
78.90	4302.0
80.00	1339.0
80.90	4417.0
81.90	1029.0
83.10	75.0
85.80	105.0
87.10	4026.0
88.00	3327.0
90.90	520.0
92.10	3599.0
93.00	5051.0
94.00	13750.0
95.00	107160.0
96.10	7005.0
96.90	164.0
102.90	89.0
104.00	892.0
104.90	199.0
105.90	716.0
106.90	71.0
110.10	68.0
110.90	150.0
111.70	110.0
112.80	123.0
114.90	82.0
116.00	419.0
116.90	804.0
117.90	435.0
119.00	800.0
123.90	77.0
126.00	121.0
127.80	395.0
129.00	218.0
129.90	330.0
130.80	107.0
132.90	256.0
133.80	73.0
135.00	236.0
136.80	236.0
140.00	66.0
140.90	1552.0
142.90	1438.0
143.70	51.0
144.10	60.0
144.80	143.0
145.90	158.0
146.90	112.0
147.90	287.0
149.10	88.0
150.00	197.0
151.80	80.0
153.10	100.0
153.80	99.0
154.80	281.0
156.90	149.0
159.10	127.0

Instrument :
MSVOA_W
ClientSampleId :
BFB472

160.90	106.0
168.50	57.0
169.70	107.0
170.90	117.0
172.10	683.0
174.00	74880.0
175.00	6367.0
176.00	78656.0
177.00	5295.0
178.00	143.0
178.60	57.0
191.10	171.0
192.90	348.0
207.10	174.0
248.90	146.0
250.00	108.0
251.10	103.0
265.10	202.0
280.00	89.0
281.10	2137.0
282.10	757.0
283.20	292.0
284.10	70.0

Instrument :
MSVOA_W
ClientSampleId :
BFB472