
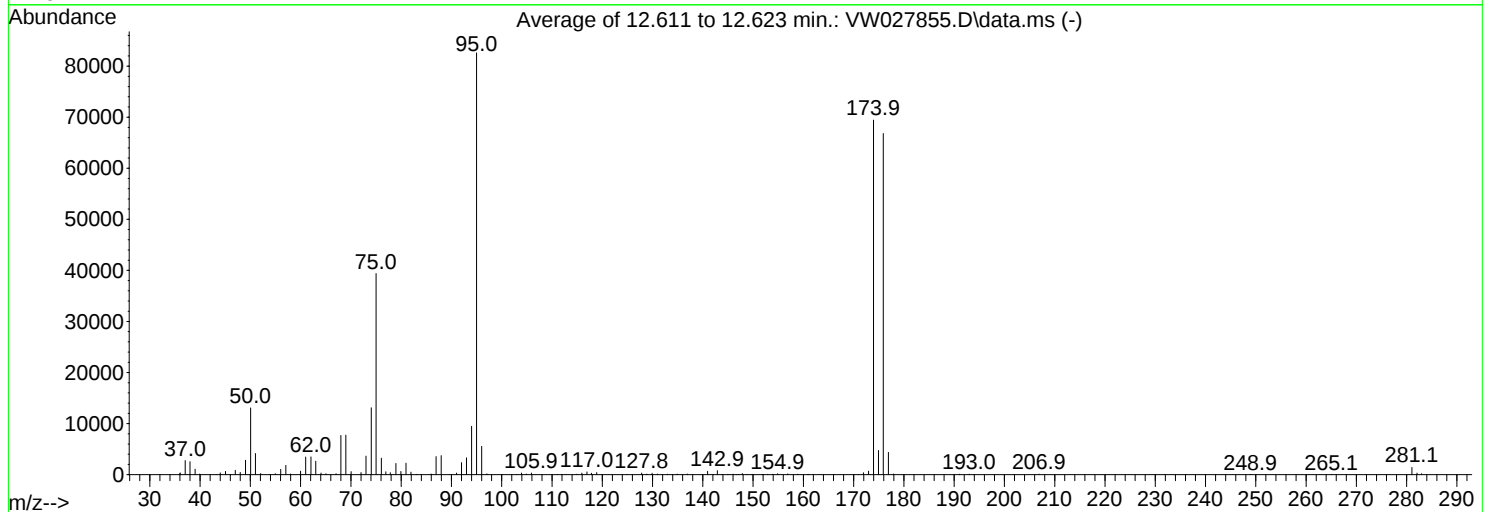


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012624\
Data File : VW027855.D
Acq On : 26 Jan 2024 08:55
Operator : SY/MD
Sample : BFB427
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB427

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Title : SFAM01.0
Last Update : Thu Jan 25 00:24:22 2024

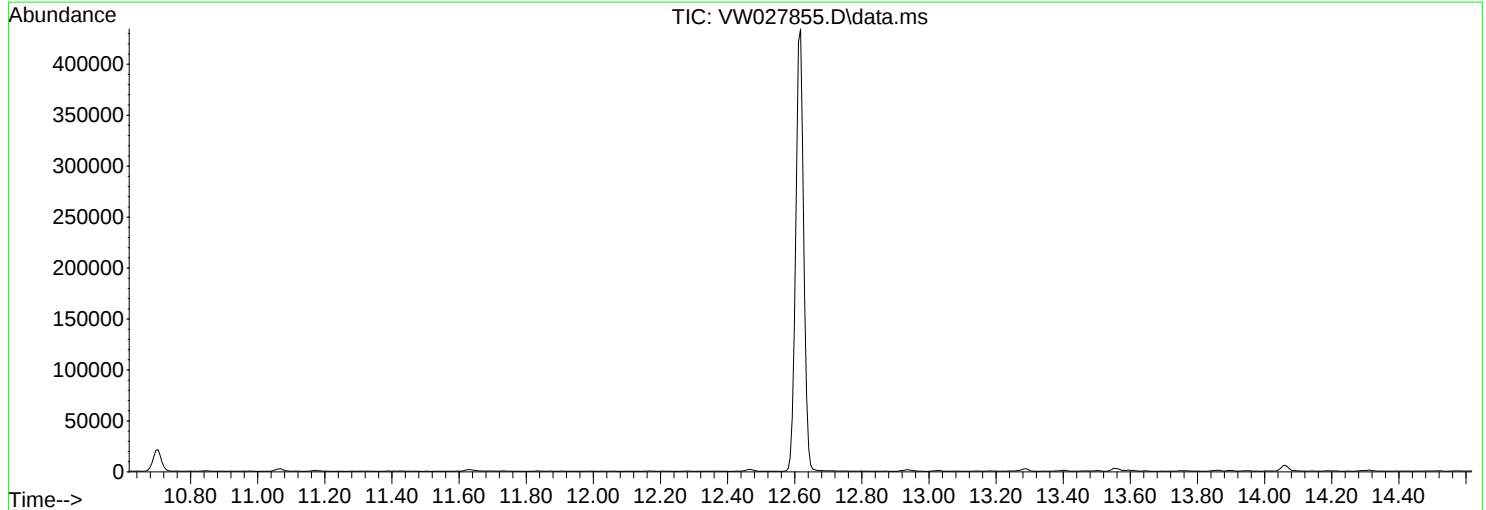

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	13069	PASS
75	95	30	80	47.7	39387	PASS
95	95	100	100	100.0	82605	PASS
96	95	5	9	6.7	5538	PASS
173	174	0.00	2	1.0	679	PASS
174	95	50	120	84.1	69451	PASS
175	174	5	9	6.8	4750	PASS
176	174	95	101	96.2	66803	PASS
177	176	5	9	6.5	4360	PASS

m/z	Abundance
40.00	440.0
43.90	190.0

Instrument :
MSVOA_W
ClientSampleId :
BFB427

m/z	Abundance
35.90	527.0
37.10	3125.0
38.00	2980.0
39.00	1376.0
40.00	556.0
43.20	60.0
44.00	610.0
45.10	595.0
47.00	943.0
48.00	464.0
49.10	3033.0
50.00	14718.0
51.00	4820.0
52.10	257.0
54.90	202.0
56.10	1210.0
57.00	1956.0
58.00	160.0
60.00	746.0
61.00	3824.0
62.00	3963.0
63.00	2763.0
64.00	347.0
65.00	213.0
67.10	172.0
68.00	8314.0
69.00	8379.0
70.00	596.0
72.00	473.0
73.00	3739.0
74.10	14007.0
75.00	42752.0
76.10	3710.0
77.00	596.0
77.90	531.0
78.90	2611.0
79.90	719.0
80.90	2395.0
81.90	603.0
83.10	77.0
86.00	159.0
86.90	4044.0
87.90	3589.0
91.00	351.0
92.00	2445.0
93.00	3660.0
94.00	9758.0
95.00	89560.0
96.00	6050.0
97.00	261.0
103.90	347.0
104.90	111.0
105.90	313.0
111.10	65.0
111.90	86.0
112.90	62.0
114.90	117.0
115.90	346.0
116.90	590.0
117.90	252.0
118.90	461.0
124.90	86.0
127.80	309.0
128.90	139.0
129.80	271.0
131.00	99.0
133.00	200.0
133.90	102.0
134.80	145.0
136.90	121.0
139.90	69.0
141.00	577.0
142.10	98.0
142.90	806.0
145.00	89.0
146.00	63.0
146.70	68.0
147.90	185.0
148.80	61.0
149.90	57.0
151.80	57.0
152.90	69.0
153.80	82.0
155.00	212.0
156.90	107.0
158.90	98.0
160.80	102.0
170.90	58.0
171.90	407.0
173.00	722.0
174.00	70424.0
174.90	4692.0

Instrument :
MSVOA_W
ClientSampleId :
BFB427

175.90	70832.0
176.90	4070.0
177.90	107.0
191.00	133.0
193.00	164.0
193.90	53.0
206.90	216.0
248.90	100.0
265.10	153.0
281.10	2474.0
282.10	525.0
282.90	324.0

Instrument :
MSVOA_W
ClientSampleId :
BFB427

m/z	Abundance
36.10	576.0
37.00	3005.0
38.00	2934.0
39.00	1114.0
39.90	592.0
44.10	565.0
45.00	742.0
46.00	92.0
47.00	884.0
48.00	517.0
49.00	3039.0
50.00	14092.0
51.00	4445.0
52.00	190.0
55.00	216.0
56.00	1248.0
57.10	2128.0
58.00	127.0
60.00	728.0
61.00	3900.0
62.10	3533.0
63.00	3157.0
64.10	323.0
65.00	231.0
67.00	264.0
68.00	8633.0
69.00	8766.0
70.10	685.0
71.90	416.0
73.00	4082.0
74.00	14724.0
75.00	44728.0
76.00	3625.0
76.90	663.0
77.80	453.0
79.00	2245.0
80.00	618.0
81.00	2467.0
82.00	502.0
83.10	68.0
85.90	112.0
87.00	3861.0
88.00	4274.0
91.00	299.0
92.00	2637.0
93.00	3757.0
94.00	11160.0
95.00	90416.0
96.00	6402.0
97.10	169.0
103.00	79.0
104.00	347.0
104.90	176.0
105.90	403.0
106.80	74.0
111.00	79.0
112.00	57.0
112.70	58.0
115.00	91.0
115.90	330.0
117.00	563.0
117.80	330.0
118.90	440.0
124.90	57.0
127.90	483.0
128.80	169.0
129.90	326.0
130.90	141.0
132.80	102.0
135.00	131.0
136.90	147.0
140.90	750.0
142.90	878.0
143.80	62.0
145.00	143.0
146.10	129.0
146.80	52.0
147.90	285.0
148.80	55.0
149.80	92.0
153.90	65.0
154.80	217.0
156.90	180.0
158.90	117.0
161.00	141.0
170.90	78.0
172.00	407.0
172.90	679.0
174.00	80008.0
175.00	5018.0
175.90	68800.0
176.90	5162.0

Instrument :
MSVOA_W
ClientSampleId :
BFB427

178.00	144.0
191.00	126.0
193.00	109.0
206.90	100.0
249.00	89.0
281.00	1223.0
282.00	347.0
283.00	126.0

Instrument :
MSVOA_W
ClientSampleId :
BFB427

m/z	Abundance
36.00	466.0
37.00	2176.0
38.00	1709.0
39.00	670.0
40.00	562.0
44.00	409.0
45.00	528.0
47.00	691.0
47.90	304.0
49.00	2372.0
50.10	10396.0
51.00	3196.0
52.00	209.0
54.90	160.0
56.00	674.0
57.10	1416.0
58.00	77.0
60.00	568.0
61.00	2608.0
62.00	2980.0
63.00	2003.0
64.00	295.0
65.10	165.0
67.10	152.0
68.00	6082.0
69.00	6062.0
70.00	504.0
72.10	351.0
73.00	3086.0
74.00	10567.0
75.00	30680.0
76.00	2360.0
77.00	452.0
77.90	176.0
78.90	1731.0
79.90	501.0
81.00	1948.0
81.90	372.0
85.90	73.0
87.00	2701.0
88.00	3305.0
91.00	253.0
92.00	1935.0
93.00	2460.0
94.00	7515.0
95.00	67840.0
96.00	4163.0
97.00	90.0
103.00	82.0
103.90	218.0
104.80	83.0
105.90	277.0
106.80	50.0
111.00	56.0
112.80	50.0
115.00	66.0
116.00	271.0
116.90	433.0
117.80	270.0
118.90	331.0
127.80	172.0
128.90	104.0
130.00	229.0
130.90	129.0
134.90	115.0
136.90	140.0
140.90	696.0
142.90	642.0
146.00	137.0
147.10	61.0
147.80	191.0
148.80	91.0
149.60	61.0
152.90	98.0
154.90	170.0
156.90	163.0
158.90	105.0
161.10	81.0
172.00	372.0
172.90	635.0
173.90	57920.0
175.00	4541.0
175.90	60776.0
176.90	3848.0
178.00	121.0
280.90	545.0
282.10	104.0
282.90	79.0

Instrument :
MSVOA_W
ClientSampleId :
BFB427