




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012725\
Data File : VW031591.D
Acq On : 27 Jan 2025 14:29
Operator : SY/MD
Sample : Q1190-16
Misc : 8.08g/10mL/MSVOA_W/SOIL/A
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44T6

Manual IntegrationsAPPROVED

Quant Time: Jan 28 00:24:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 28 00:17:29 2025
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/28/2025
Supervised By :Mahesh Dadoda 01/28/2025

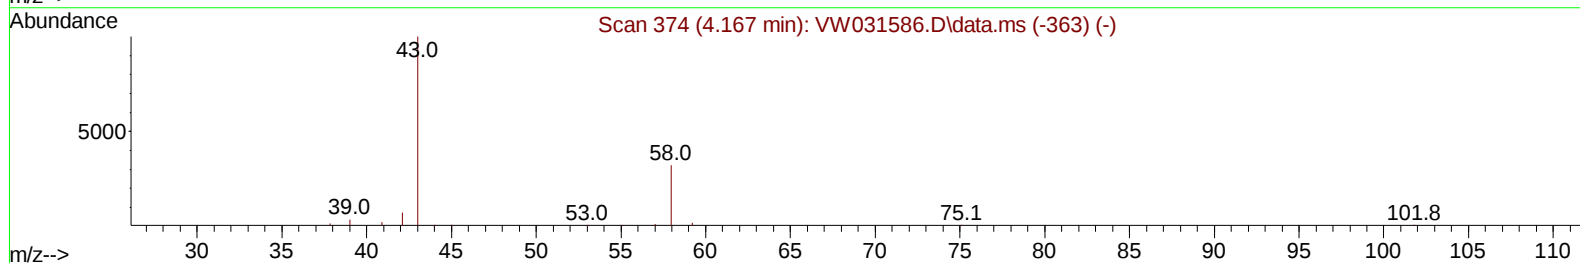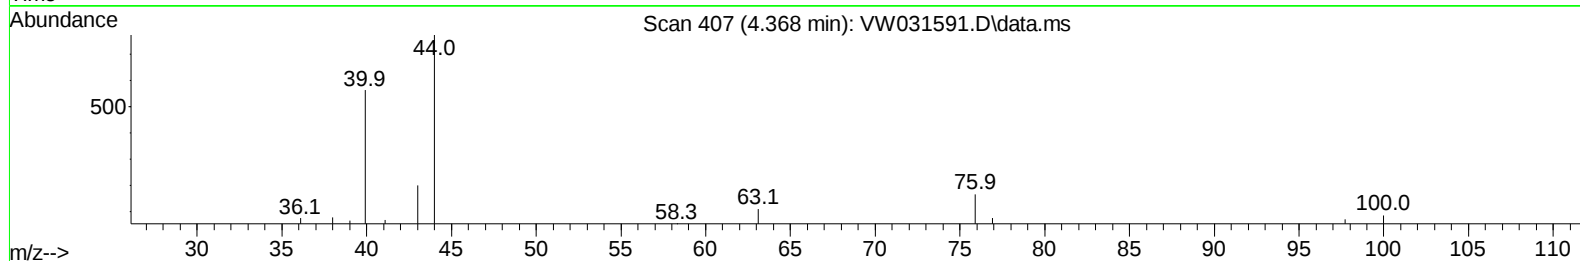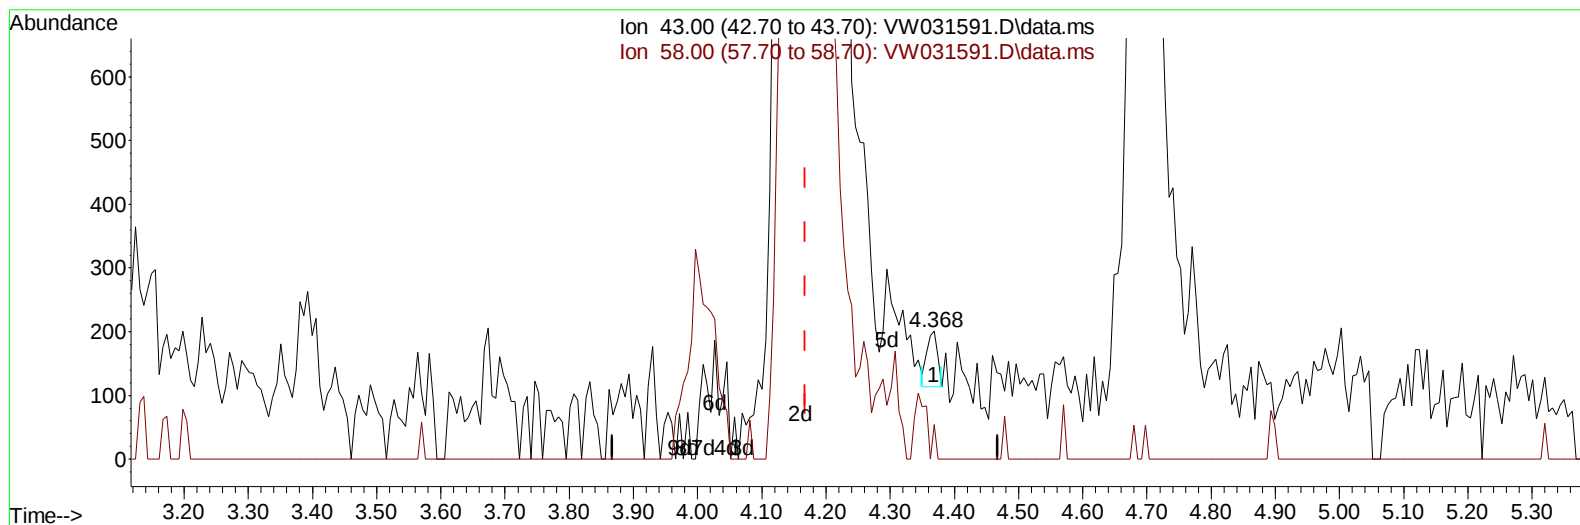

TIC: VW031591.D\data.ms

(13) Acetone (T)

4.368min (+ 0.201) 0.05 ug/L

response 97

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	20.62
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012725\
Data File : VW031591.D
Acq On : 27 Jan 2025 14:29
Operator : SY/MD
Sample : Q1190-16
Misc : 8.08g/10mL/MSVOA_W/SOIL/A
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44T6

Manual IntegrationsAPPROVED

Quant Time: Jan 28 00:24:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 28 00:17:29 2025
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/28/2025
Supervised By :Mahesh Dadoda 01/28/2025

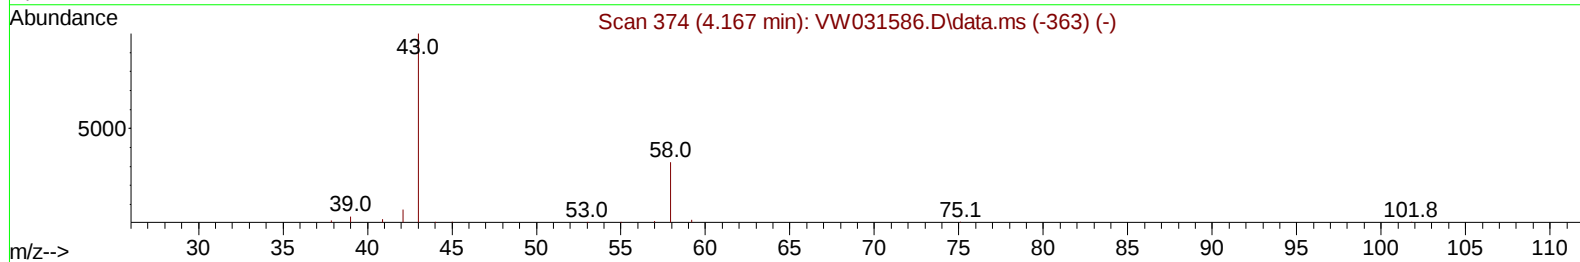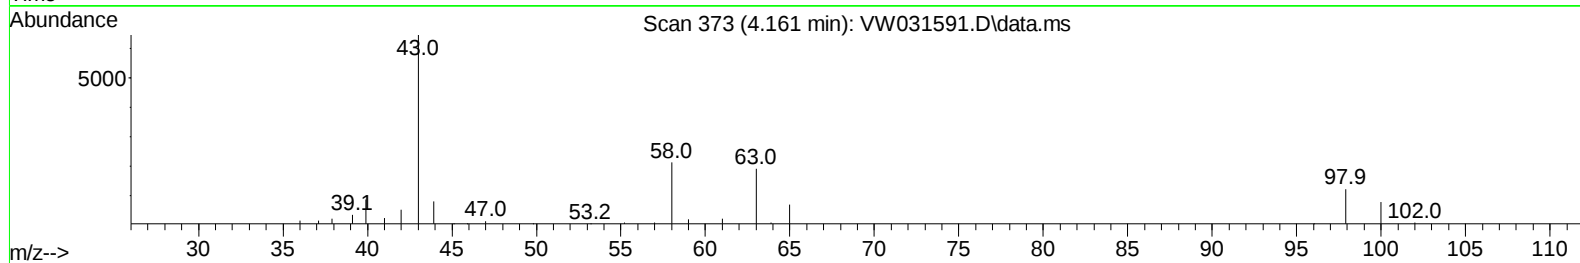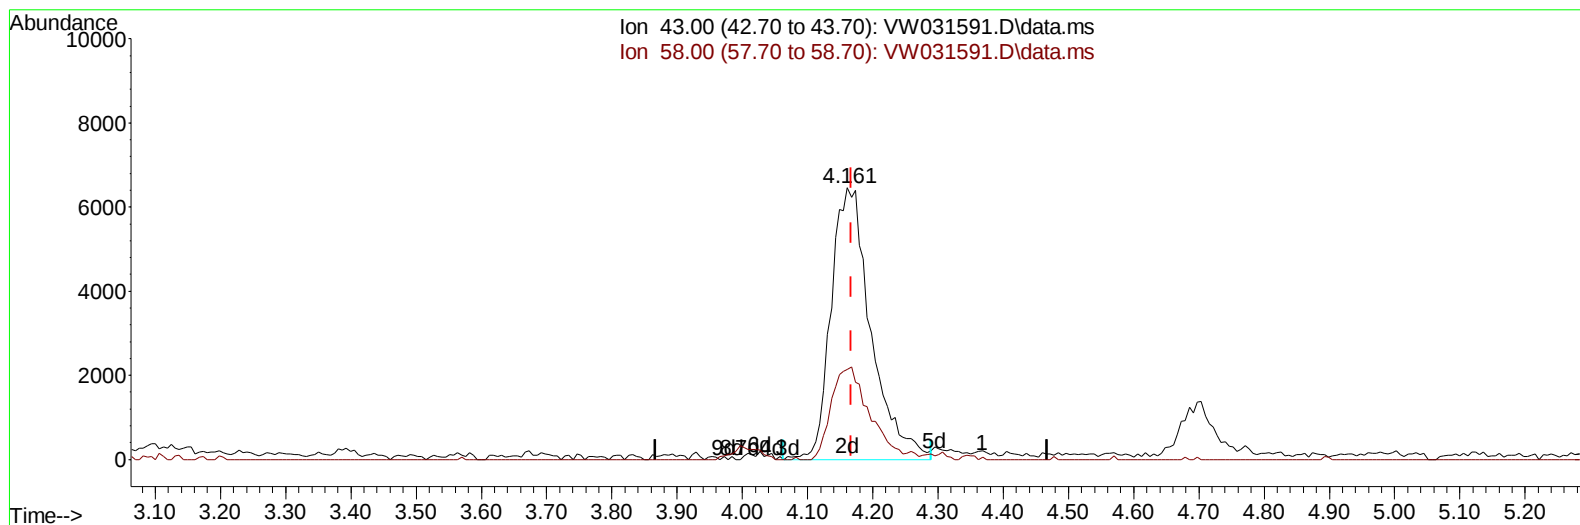

TIC: VW031591.D\data.ms

(13) Acetone (T)

4.161min (-0.006) 13.06 ug/L m

response 27446

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	0.07
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012725\
 Data File : VW031591.D
 Acq On : 27 Jan 2025 14:29
 Operator : SY/MD
 Sample : Q1190-16
 Misc : 8.08g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44T6

Manual IntegrationsAPPROVED

Quant Time: Jan 28 00:24:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jan 28 00:17:29 2025
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/28/2025
 Supervised By :Mahesh Dadoda 01/28/2025

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		1082408	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		970548	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152		472302	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		307026	18.076	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	72.320%	
7) Chloroethane-d5	2.899	69		231797	19.110	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	76.440%	
11) 1,1-Dichloroethene-d2	4.015	65		146425	19.376	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	77.520%	
21) 2-Butanone-d5	7.087	46		181223	66.373	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	132.740%	
24) Chloroform-d	7.642	84		630126	22.494	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	89.960%	
26) 1,2-Dichloroethane-d4	8.307	65		345119	25.031	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	100.120%	
32) Benzene-d6	8.270	84		1310787	21.501	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	86.000%	
36) 1,2-Dichloropropane-d6	9.270	67		402529	22.363	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	89.440%	
41) Toluene-d8	10.318	98		1166956	21.204	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	84.800%	
43) trans-1,3-Dichloroprop...	10.574	79		175220	23.705	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	94.840%	
47) 2-Hexanone-d5	10.922	63		135877	73.971	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	147.940%#	
56) 1,1,2,2-Tetrachloroeth...	12.684	84		326059	29.621	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	118.480%	
66) 1,2-Dichlorobenzene-d4	13.848	152		374461	22.605	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	90.400%	
Target Compounds							
13) Acetone	4.161	43		27446m	13.061	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012725\
Data File : VW031591.D
Acq On : 27 Jan 2025 14:29
Operator : SY/MD
Sample : Q1190-16
Misc : 8.08g/10mL/MSVOA_W/SOIL/A
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44T6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/28/2025
Supervised By :Mahesh Dadoda 01/28/2025

Quant Time: Jan 28 00:24:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 28 00:17:29 2025
Response via : Initial Calibration

