




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012725\
Data File : VW031593.D
Acq On : 27 Jan 2025 15:17
Operator : SY/MD
Sample : Q1190-01
Misc : 11.11g/10mL/MSVOA_W/SOIL/A
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44S2

Manual IntegrationsAPPROVED

Quant Time: Jan 28 00:25:30 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 28 00:17:29 2025
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/28/2025
Supervised By :Mahesh Dadoda 01/28/2025

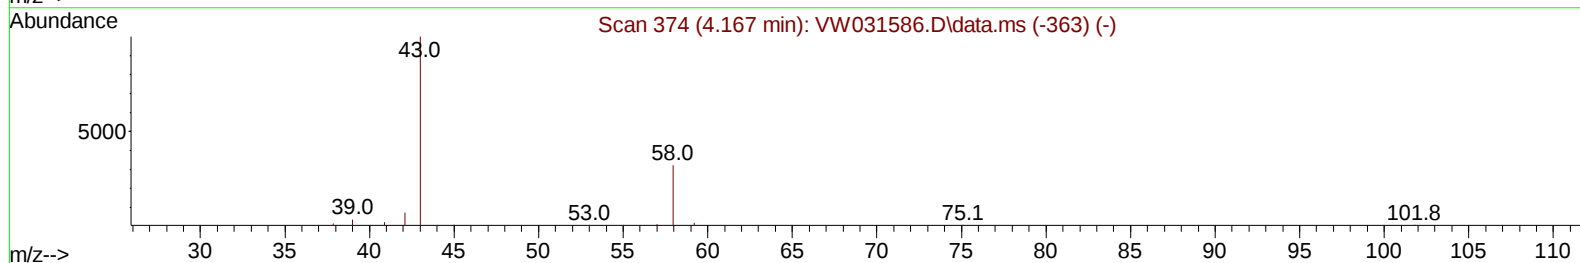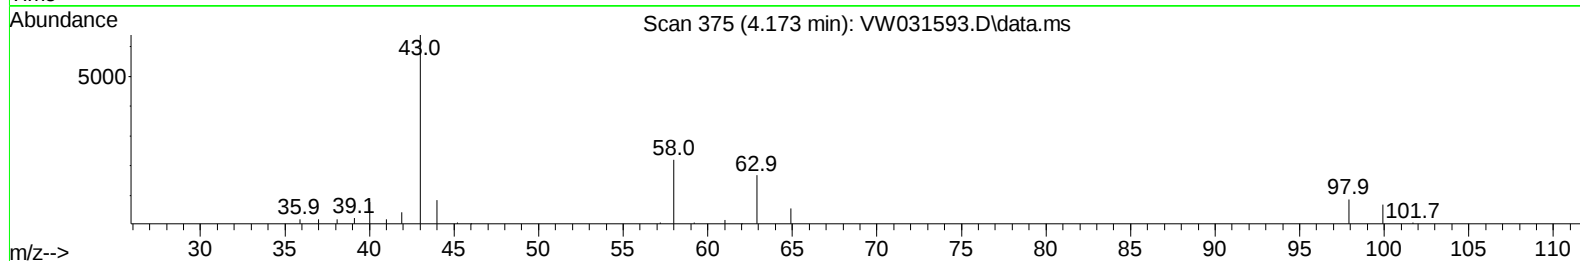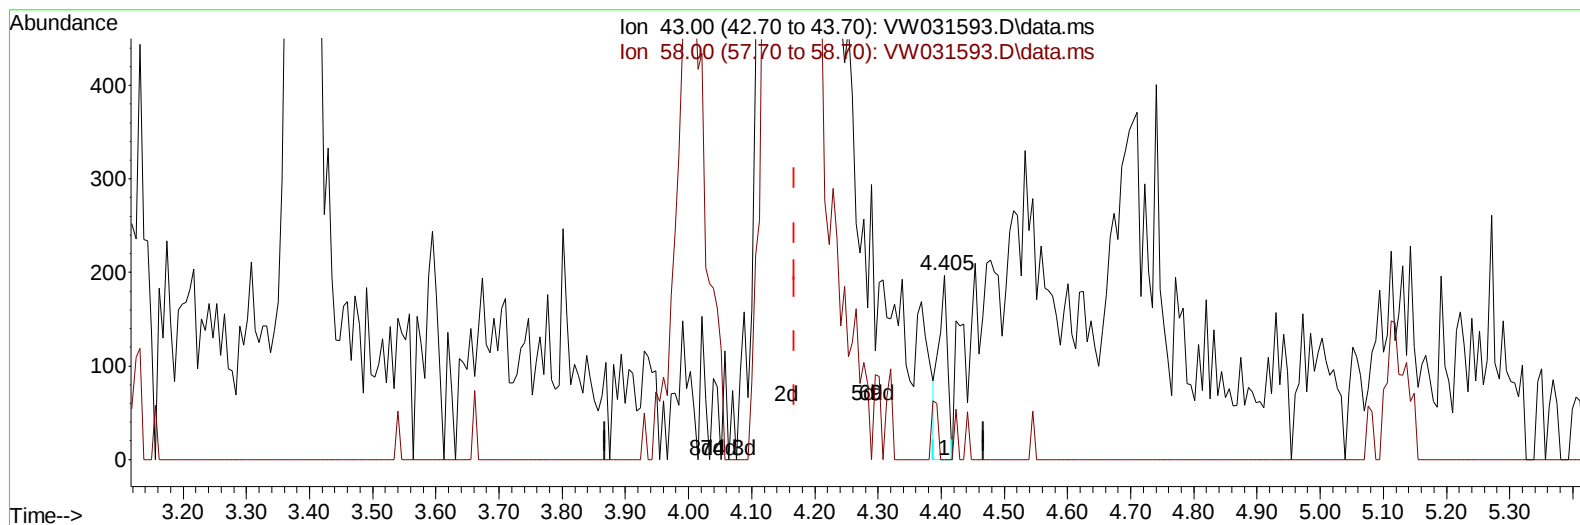

TIC: VW031593.D\data.ms

(13) Acetone (T)

4.405min (+ 0.238) 0.10 ug/L

response 196

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	22.96
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012725\
Data File : VW031593.D
Acq On : 27 Jan 2025 15:17
Operator : SY/MD
Sample : Q1190-01
Misc : 11.11g/10mL/MSVOA_W/SOIL/A
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44S2

Manual IntegrationsAPPROVED

Quant Time: Jan 28 00:25:30 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 28 00:17:29 2025
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/28/2025
Supervised By :Mahesh Dadoda 01/28/2025

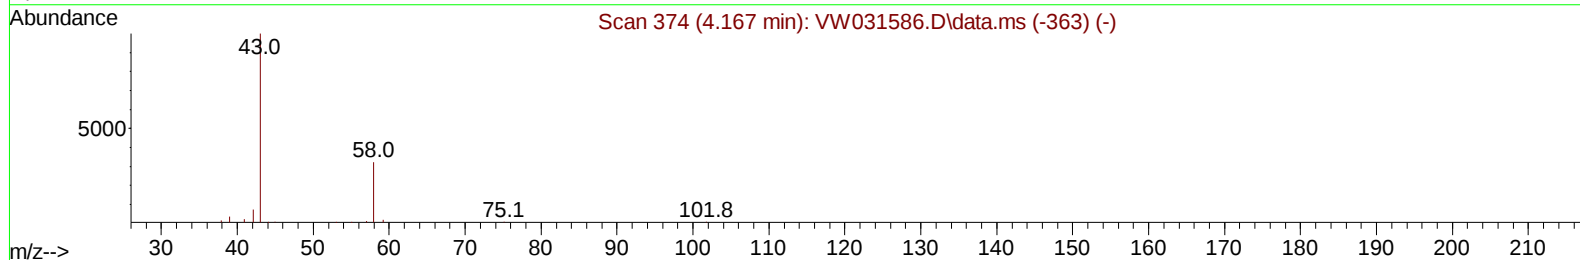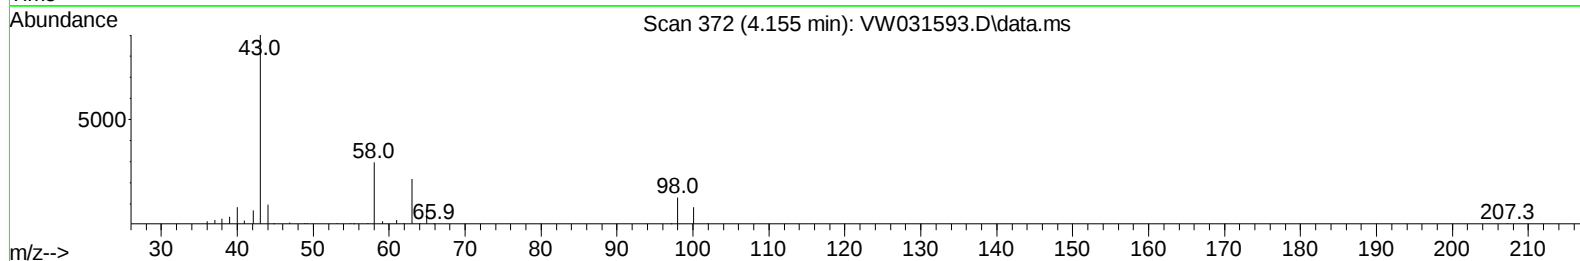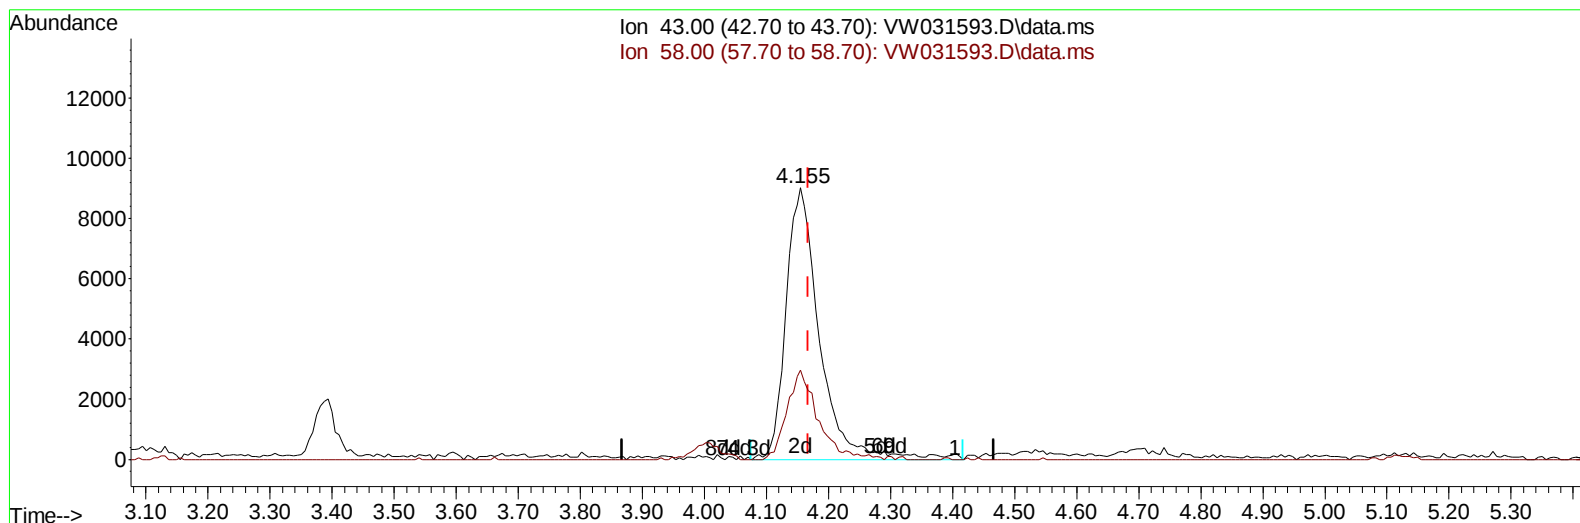

TIC: VW031593.D\data.ms

(13) Acetone (T)

4.155min (-0.012) 16.63 ug/L m

response 33943

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	14.10	0.13
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012725\
 Data File : VW031593.D
 Acq On : 27 Jan 2025 15:17
 Operator : SY/MD
 Sample : Q1190-01
 Misc : 11.11g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A44S2

Manual IntegrationsAPPROVED

Quant Time: Jan 28 00:25:30 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jan 28 00:17:29 2025
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/28/2025
 Supervised By :Mahesh Dadoda 01/28/2025

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		1051454	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		869277	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		346498	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		294537	17.852	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	71.400%		
7) Chloroethane-d5	2.899	69		241383	20.486	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	81.960%		
11) 1,1-Dichloroethene-d2	4.015	65		154871	21.097	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	84.400%		
21) 2-Butanone-d5	7.088	46		227059	85.609	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	171.220%#		
24) Chloroform-d	7.642	84		648534	23.833	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	95.320%		
26) 1,2-Dichloroethane-d4	8.301	65		379248	28.316	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	113.280%		
32) Benzene-d6	8.270	84		1336242	24.472	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	97.880%		
36) 1,2-Dichloropropane-d6	9.270	67		424001	26.300	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	105.200%		
41) Toluene-d8	10.319	98		1147272	23.275	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	93.120%		
43) trans-1,3-Dichloroprop...	10.575	79		190067	28.709	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	114.840%		
47) 2-Hexanone-d5	10.922	63		165095	100.348	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	200.700%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		365455	37.068	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	148.280%#		
66) 1,2-Dichlorobenzene-d4	13.849	152		290248	23.883	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	95.520%		
Target Compounds							
13) Acetone	4.155	43		33943m	16.628	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012725\
Data File : VW031593.D
Acq On : 27 Jan 2025 15:17
Operator : SY/MD
Sample : Q1190-01
Misc : 11.11g/10mL/MSVOA_W/SOIL/A
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A44S2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/28/2025
Supervised By :Mahesh Dadoda 01/28/2025

Quant Time: Jan 28 00:25:30 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 28 00:17:29 2025
Response via : Initial Calibration

